

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
 Data File : FF012772.D
 Signal(s) : FID2B.ch
 Acq On : 26 May 2023 21:21
 Operator : YP\AJ
 Sample : 02953-05
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 27 02:53:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
 Quant Title :
 QLast Update : Fri May 05 16:23:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	1028480	8.520 ug/ml
Target Compounds			
7) N-EICOSANE	12.971f	516075	3.728 ug/ml
10) N-TETRACOSANE	15.193	323608	2.425 ug/ml
12) N-OCTACOSANE	17.100f	277863	2.193 ug/ml
13) N-TRIACONTANE	18.050	348495	2.786 ug/ml
14) N-DOTRIACONTANE	18.880	398590	3.337 ug/ml
15) N-TETRATRIACONTANE	19.663	152215	1.384 ug/ml
16) N-HEXATRIACONTANE	20.410	1045117	10.044 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012772.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 21:21
Operator : YP\AJ
Sample : 02953-05
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 27 02:53:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

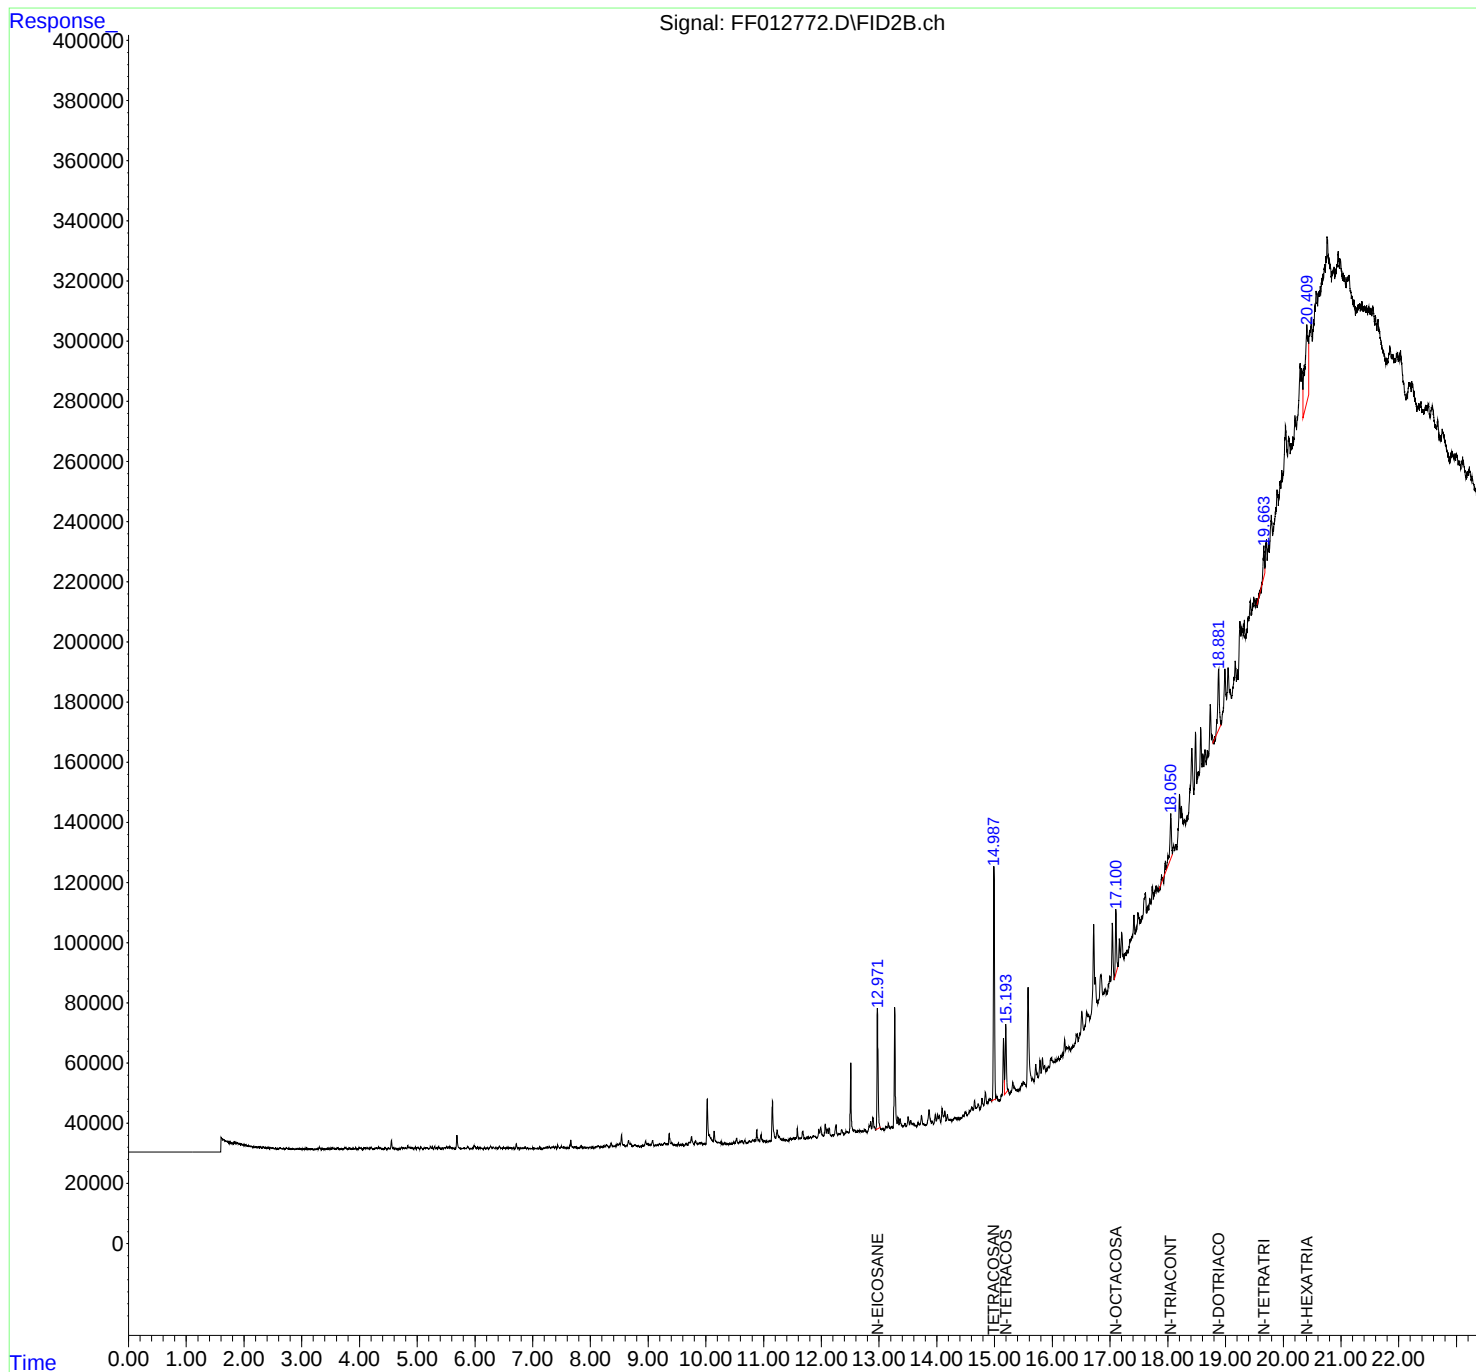


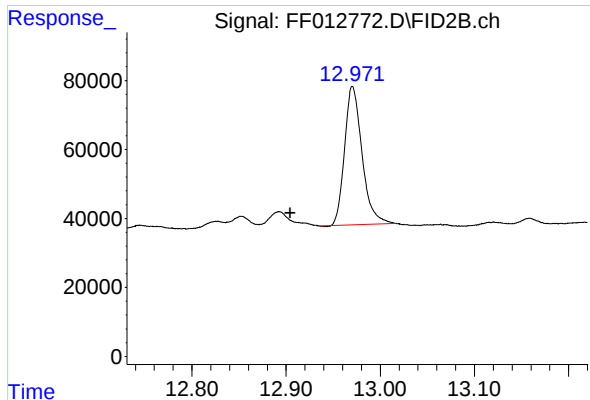

#7 N-EICOSANE


R.T.: 12.971 min
Delta R.T.: 0.066 min
Response: 516075
Conc: 3.73 ug/ml

Instrument :
FID_F
ClientSampleId :

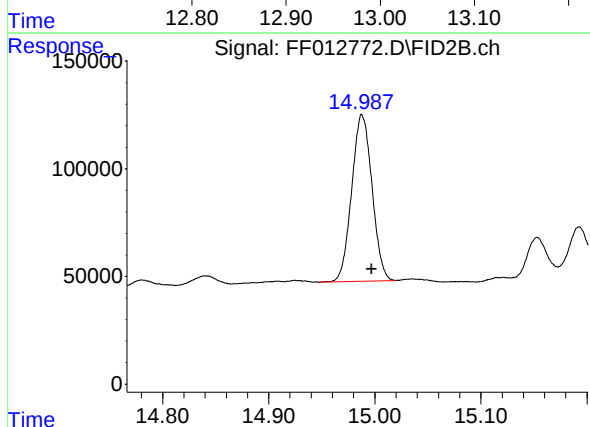


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.988 min
Delta R.T.: -0.009 min
Response: 1028480
Conc: 8.52 ug/ml

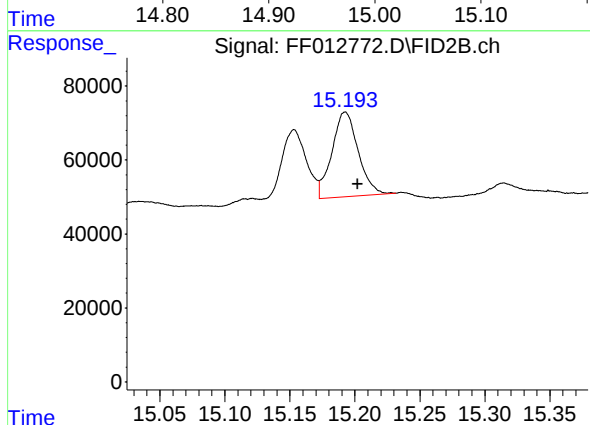


#10 N-TETRACOSANE

R.T.: 15.193 min
Delta R.T.: -0.010 min
Response: 323608
Conc: 2.43 ug/ml

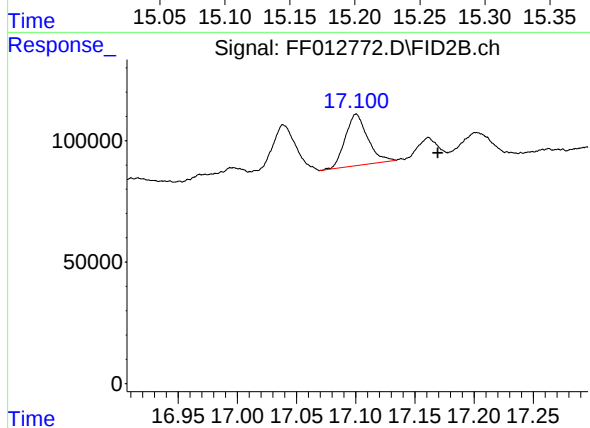

#12 N-OCTACOSANE


R.T.: 17.100 min
Delta R.T.: -0.069 min
Response: 277863
Conc: 2.19 ug/ml

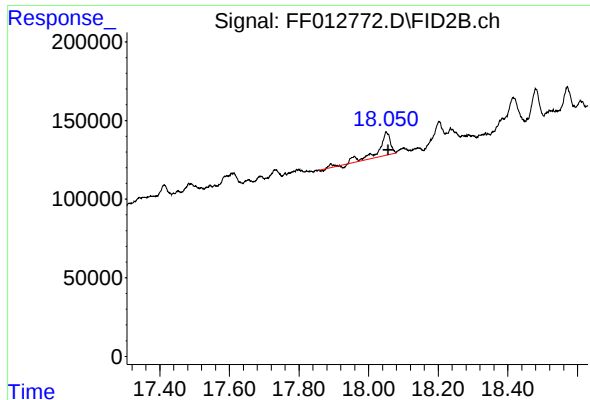

#13 N-TRIACONTANE


R.T.: 18.050 min
Delta R.T.: -0.006 min
Response: 348495
Conc: 2.79 ug/ml

Instrument :
FID_F
ClientSampleId :

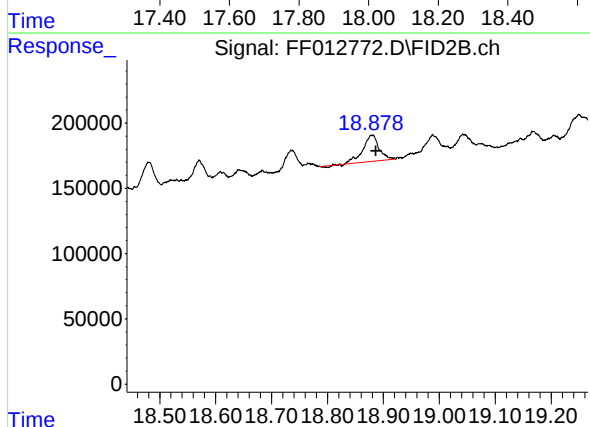


#14 N-DOTRIACONTANE

R.T.: 18.880 min
Delta R.T.: -0.007 min
Response: 398590
Conc: 3.34 ug/ml

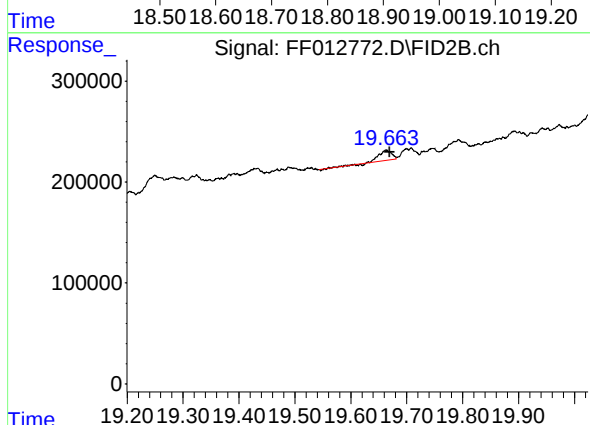

#15 N-TETRATRIACONTANE

R.T.: 19.663 min
Delta R.T.: -0.006 min
Response: 152215
Conc: 1.38 ug/ml

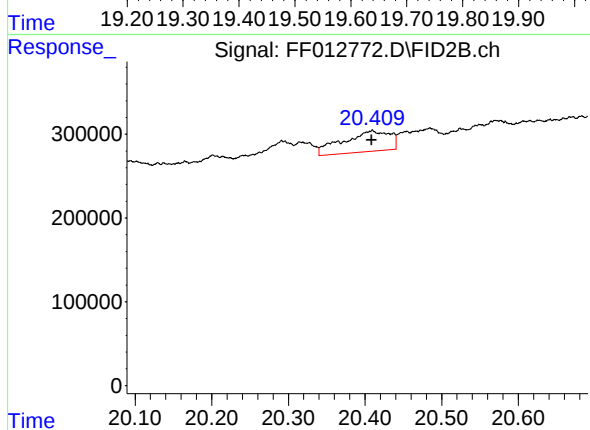

#16 N-HEXATRIACONTANE

R.T.: 20.410 min
Delta R.T.: 0.001 min
Response: 1045117
Conc: 10.04 ug/ml