

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012773.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 21:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 27 02:53:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.989	1848872	15.316 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.877	121666	1.018 ug/ml
16) N-HEXATRIACONTANE	20.411	488639	4.696 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012773.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 21:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 27 02:53:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

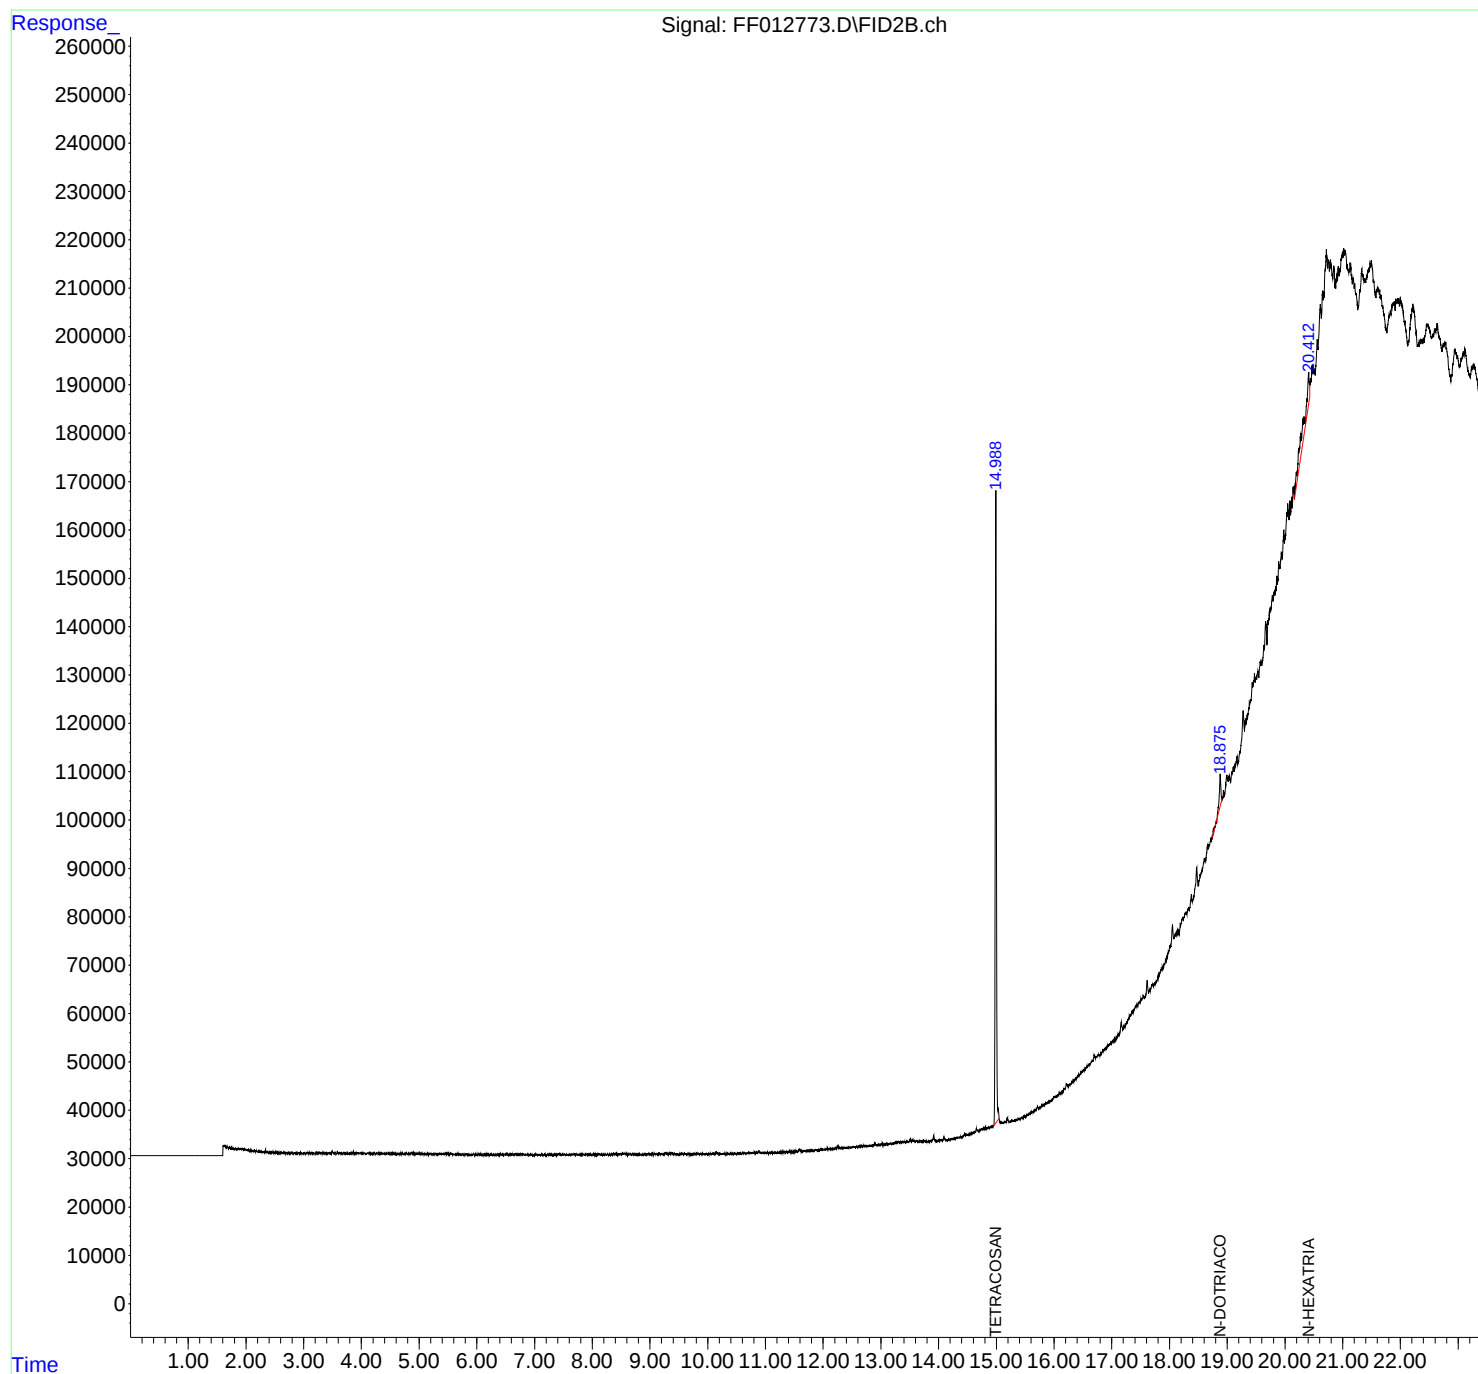


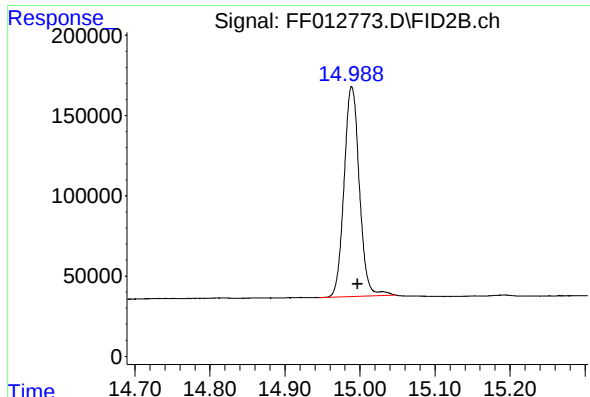

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.989 min
Delta R.T.: -0.008 min
Response: 1848872
Conc: 15.32 ug/ml

Instrument :
FID_F
ClientSampleId :

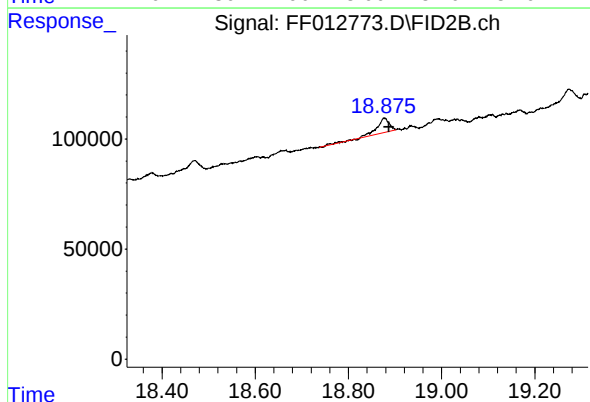

#14 N-DOTRIACONTANE

R.T.: 18.877 min
Delta R.T.: -0.010 min
Response: 121666
Conc: 1.02 ug/ml

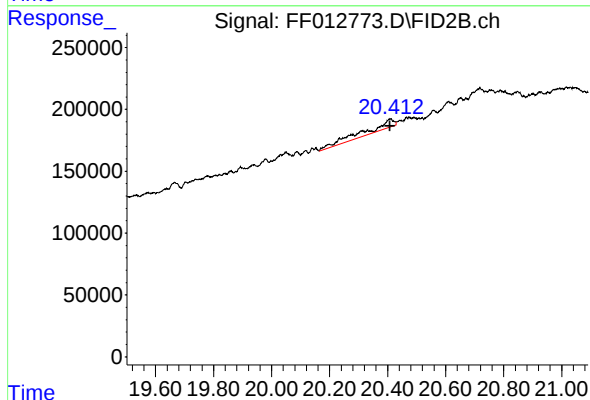

#16 N-HEXATRIACONTANE

R.T.: 20.411 min
Delta R.T.: 0.003 min
Response: 488639
Conc: 4.70 ug/ml