

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012764.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 15:00
Operator : YP\AJ
Sample : PB153083BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB153083BL

Integration File: autoint1.e
Quant Time: May 27 02:52:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.984	1758108	14.564 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012764.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 15:00
Operator : YP\AJ
Sample : PB153083BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PB153083BL

Integration File: autoint1.e
Quant Time: May 27 02:52:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

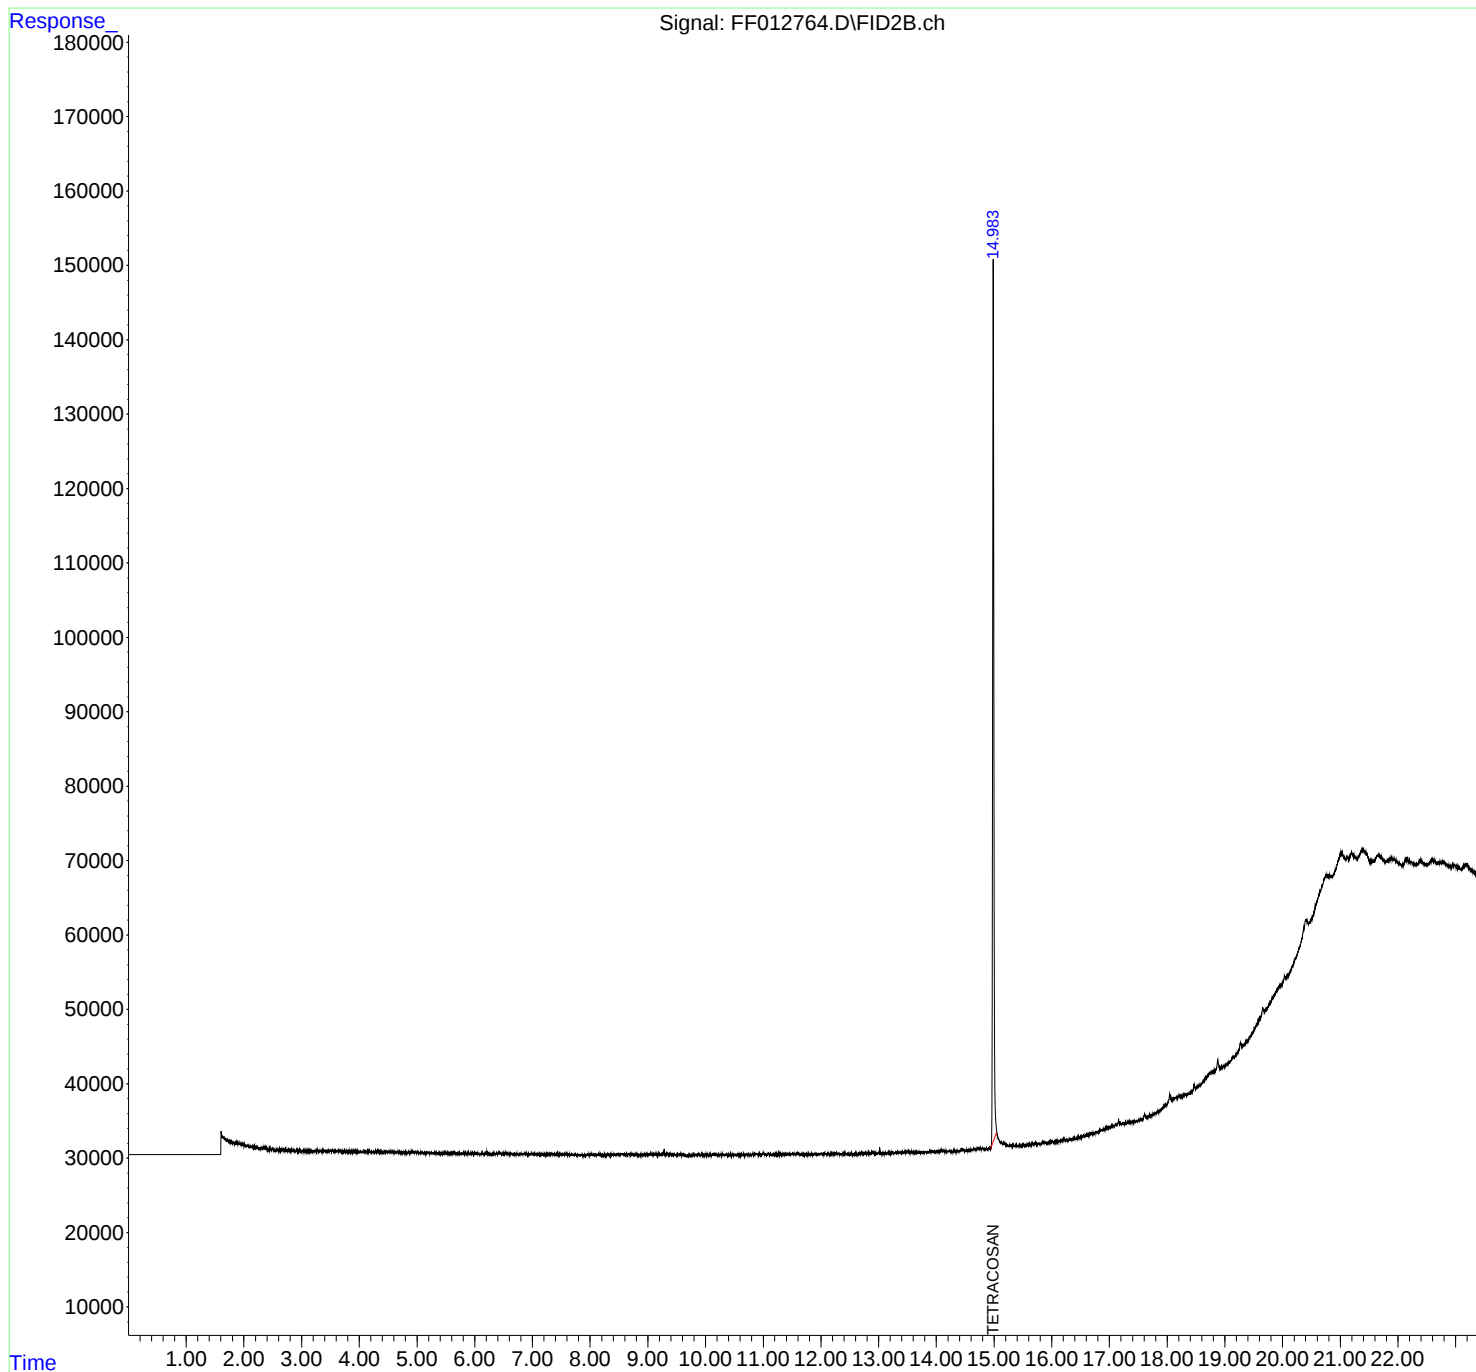

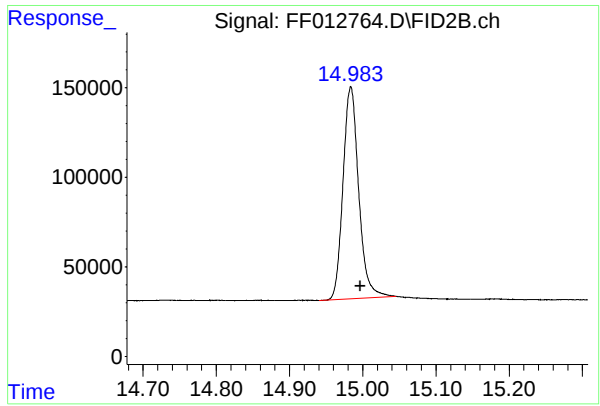

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.984 min
Delta R.T.: -0.013 min
Response: 1758108
Conc: 14.56 ug/ml

Instrument :
FID_F
ClientSampleId :
PB153083BL