

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012766.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 16:28
Operator : YP\AJ
Sample : 02937-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AU-06-052423

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

Integration File: autoint1.e
Quant Time: May 27 02:52:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.986	1772762	14.685 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052623\
Data File : FF012766.D
Signal(s) : FID2B.ch
Acq On : 26 May 2023 16:28
Operator : YP\AJ
Sample : 02937-01
Misc :
ALS Vial : 63 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
AU-06-052423


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/30/2023
Supervised By :Ankita Jodhani 05/30/2023

Integration File: autoint1.e
Quant Time: May 27 02:52:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

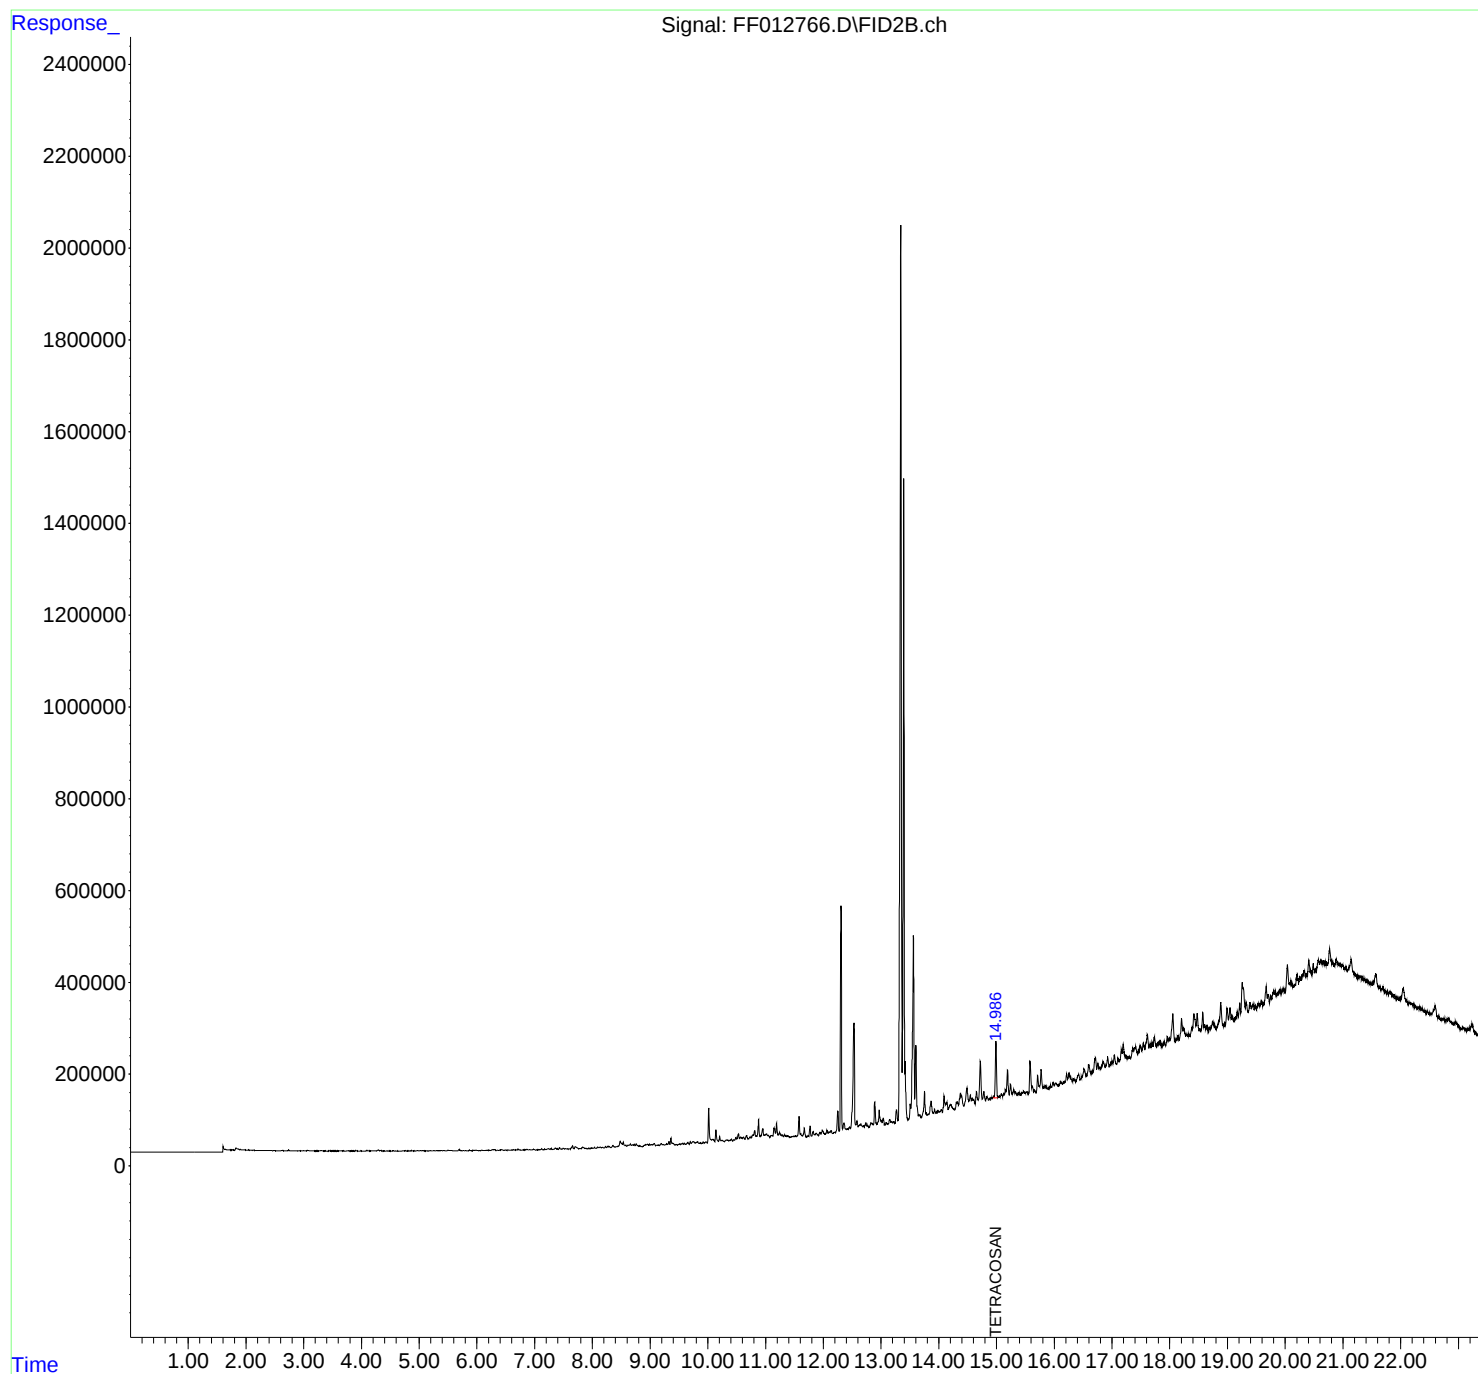

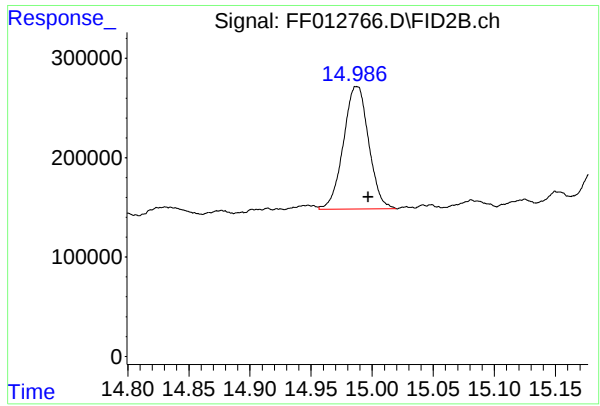

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.986 min
Delta R.T.: -0.011 min
Response: 1772762
Conc: 14.69 ug/ml

Instrument :

FID_F

ClientSampleId :

AU-06-052423

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 05/30/2023

Supervised By :Ankita Jodhani 05/30/2023