

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052819\
 Data File : FF004638.D
 Signal(s) : FID2B.ch
 Acq On : 28 May 2019 13:46
 Operator : AJ\SJ
 Sample : K3053-01MS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: May 29 01:16:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.698	2432394	19.920 ug/ml
Target Compounds			
2) N-DECANE	4.418	2872012	19.613 ug/ml
3) N-DODECANE	6.440	2989404	20.201 ug/ml
4) N-TETRADECANE	8.234	2984674	20.319 ug/ml
5) N-HEXADECANE	9.836	3030188	20.523 ug/ml
6) N-OCTADECANE	11.281	3026957	20.849 ug/ml
7) N-EICOSANE	12.594	2975775	20.547 ug/ml
8) N-DOCOSANE	13.796	2876364	20.356 ug/ml
10) N-TETRACOSANE	14.902	2812848	20.297 ug/ml
11) N-HEXACOSANE	15.927	2783962	20.432 ug/ml
12) N-OCTACOSANE	16.880	2834730	20.850 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052819\
Data File : FF004638.D
Signal(s) : FID2B.ch
Acq On : 28 May 2019 13:46
Operator : AJ\SJ
Sample : K3053-01MS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: May 29 01:16:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

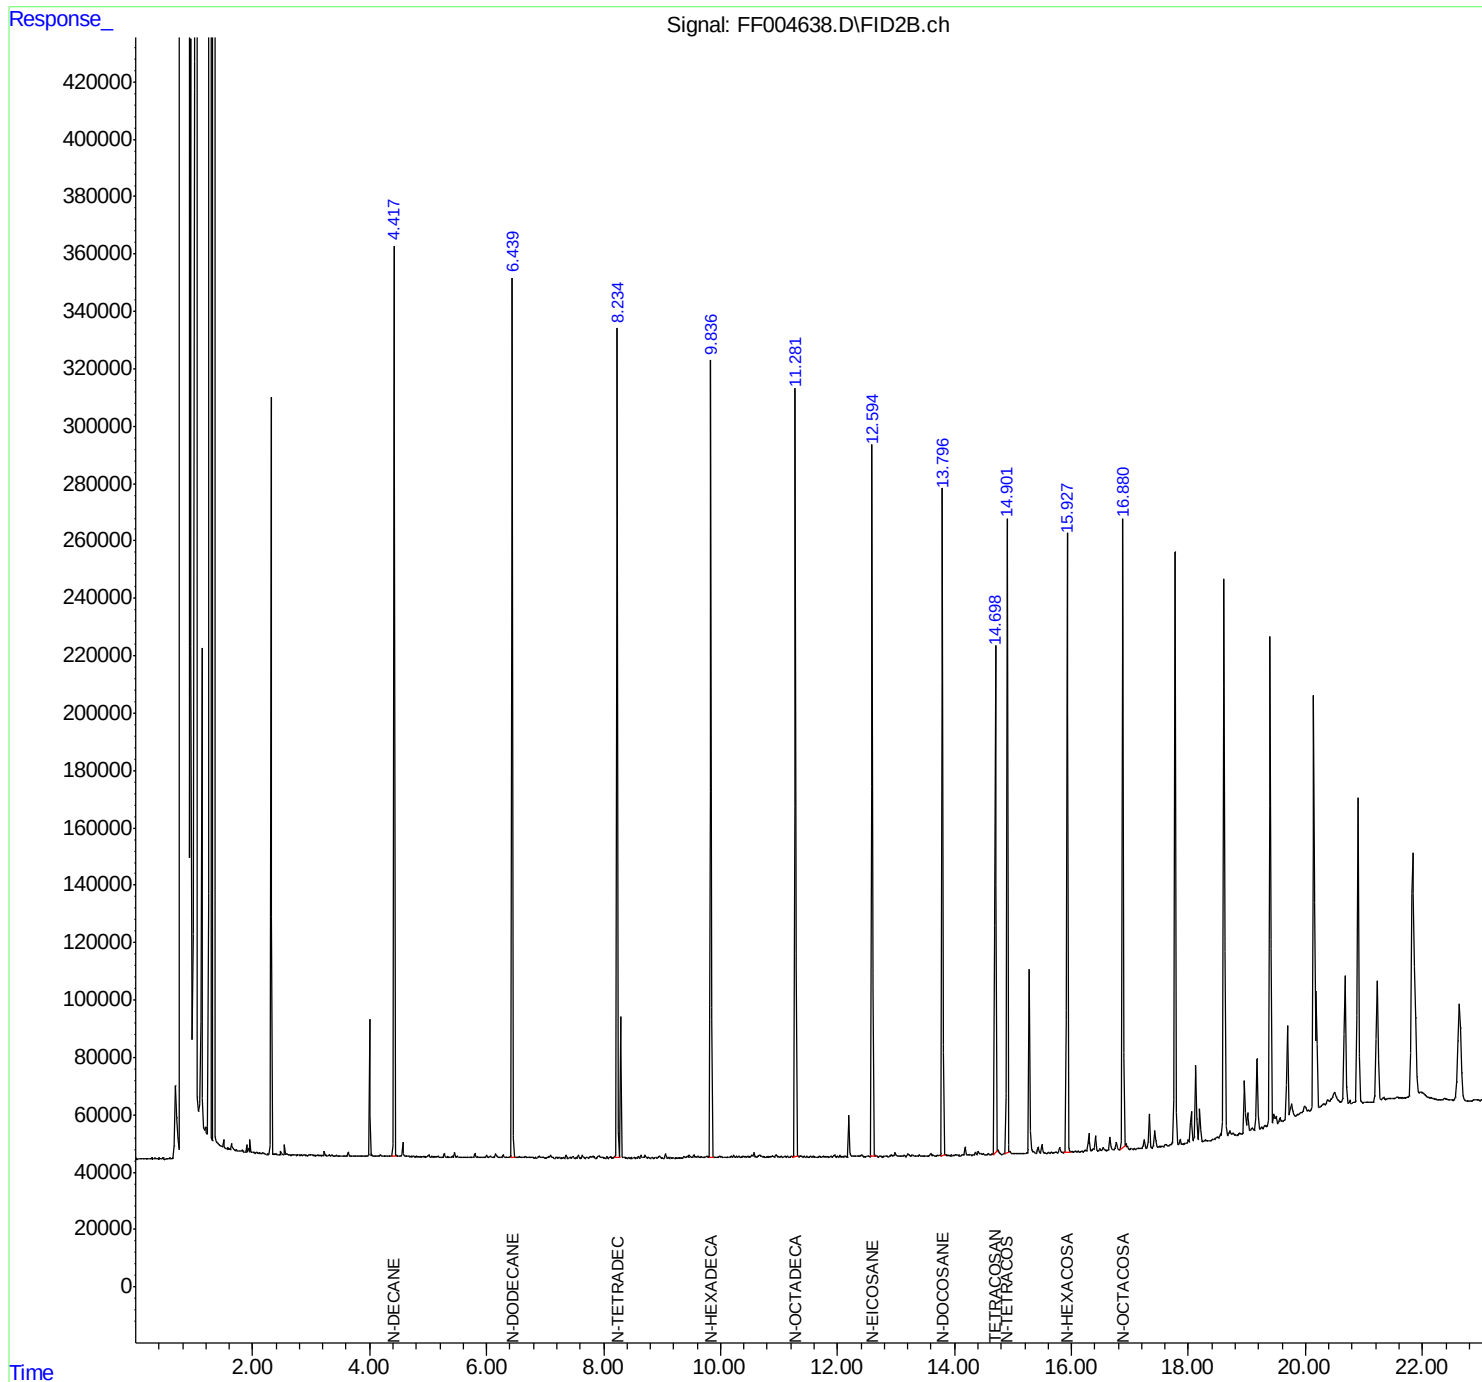

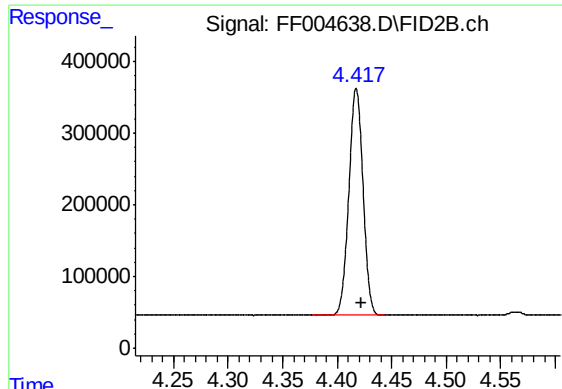


#2 N-DECANE

R.T.: 4.418 min
Delta R.T.: -0.005 min
Response: 2872012
Conc: 19.61 ug/ml

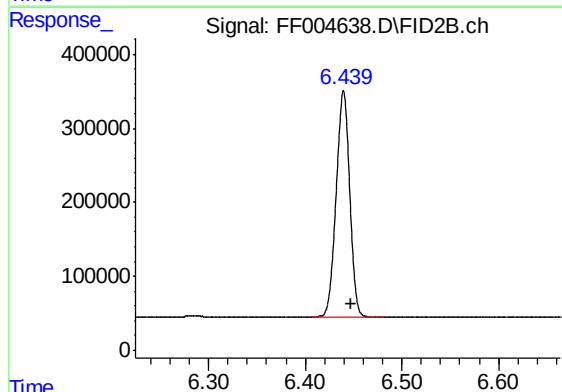


#3 N-DODECANE

R.T.: 6.440 min
Delta R.T.: -0.008 min
Response: 2989404
Conc: 20.20 ug/ml

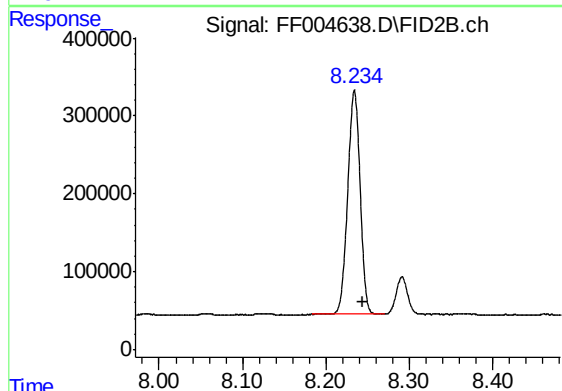


#4 N-TETRADECANE

R.T.: 8.234 min
Delta R.T.: -0.009 min
Response: 2984674
Conc: 20.32 ug/ml

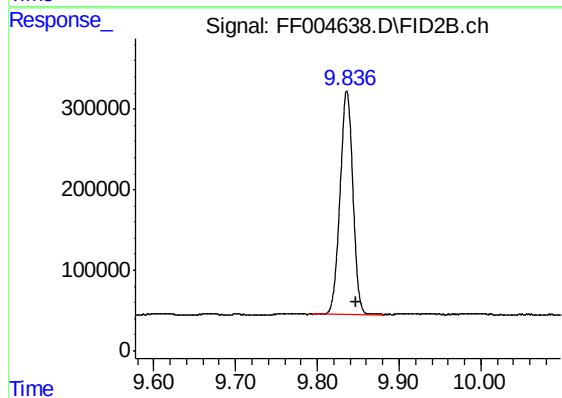


#5 N-HEXADECANE

R.T.: 9.836 min
Delta R.T.: -0.011 min
Response: 3030188
Conc: 20.52 ug/ml

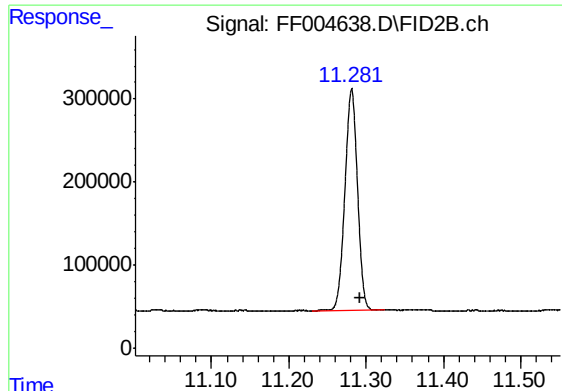


#6 N-OCTADECANE

R.T.: 11.281 min
Delta R.T.: -0.010 min
Response: 3026957
Conc: 20.85 ug/ml

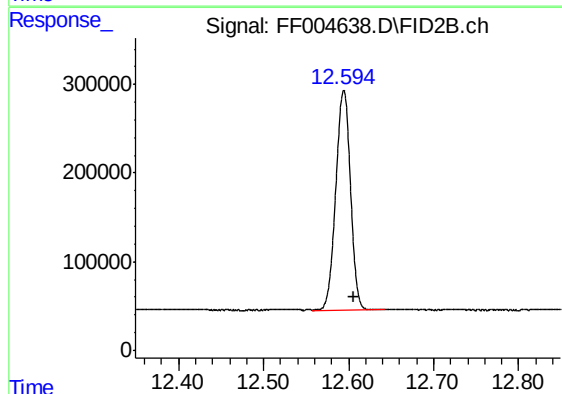


#7 N-EICOSANE

R.T.: 12.594 min
Delta R.T.: -0.011 min
Response: 2975775
Conc: 20.55 ug/ml

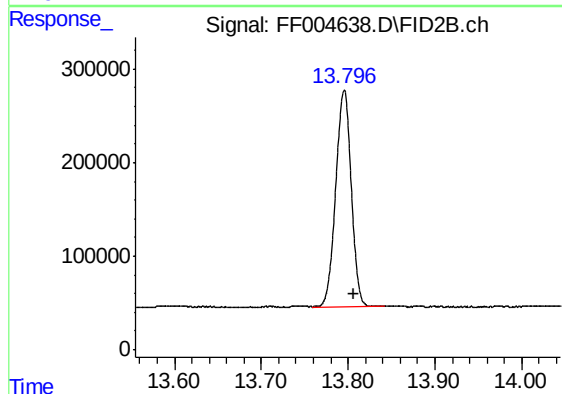


#8 N-DOCOSANE

R.T.: 13.796 min
Delta R.T.: -0.011 min
Response: 2876364
Conc: 20.36 ug/ml

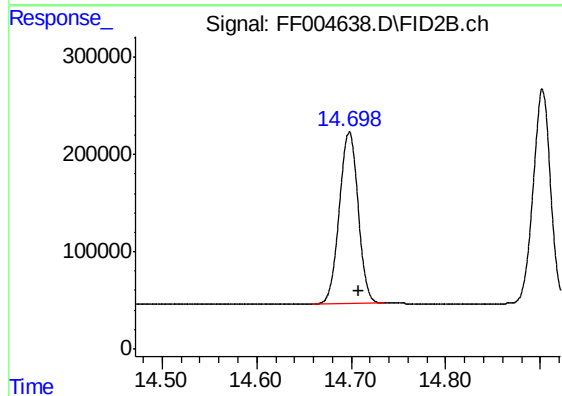


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.698 min
Delta R.T.: -0.010 min
Response: 2432394
Conc: 19.92 ug/ml

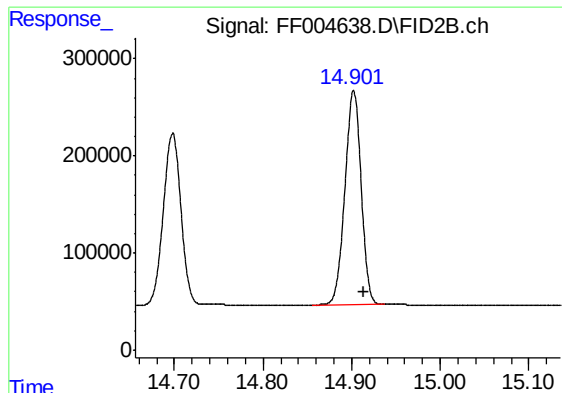


#10 N-TETRACOSANE

R.T.: 14.902 min
Delta R.T.: -0.011 min
Response: 2812848
Conc: 20.30 ug/ml

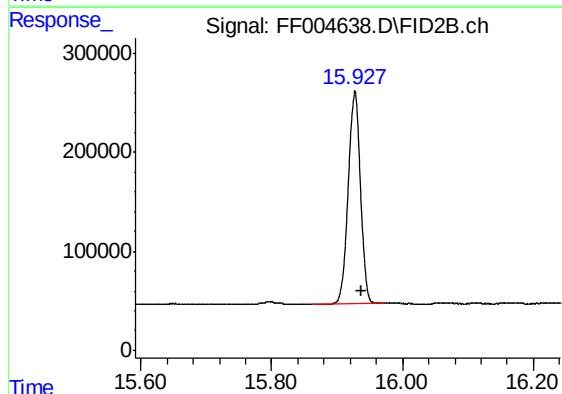

#11 N-HEXACOSANE

R.T.: 15.927 min
Delta R.T.: -0.010 min
Response: 2783962
Conc: 20.43 ug/ml

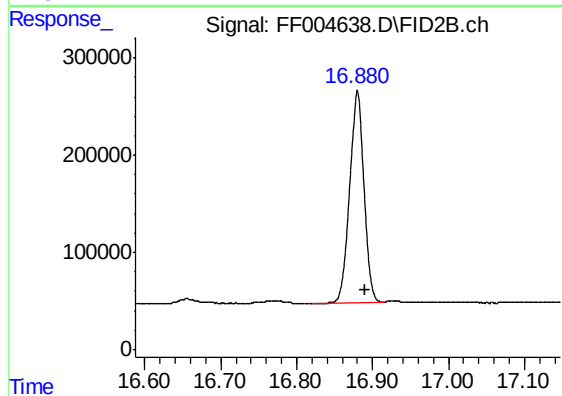

#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: -0.010 min
Response: 2834730
Conc: 20.85 ug/ml