

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052822\
 Data File : FF010679.D
 Signal(s) : FID2B.ch
 Acq On : 28 May 2022 14:16
 Operator : AJ\MA
 Sample : N3000-02 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 29 23:49:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052722.M
 Quant Title :
 QLast Update : Fri May 27 13:05:08 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.827	204910	1.768 ug/ml
Target Compounds			
7) N-EICOSANE	12.775	151108	1.133 ug/ml
10) N-TETRACOSANE	14.986	112868	0.861 ug/ml
13) N-TRIACONTANE	17.878	81042	0.657 ug/ml
14) N-DOTRIACONTANE	18.718	143760	1.180 ug/ml
16) N-HEXATRIACONTANE	20.272f	345439	4.519 ug/ml
17) N-OCTATRIACONTANE	20.929	1270420	19.937 ug/ml
18) N-TETRACONTANE	21.811f	1086416	13.312 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052822\
Data File : FF010679.D
Signal(s) : FID2B.ch
Acq On : 28 May 2022 14:16
Operator : AJ\MA
Sample : N3000-02 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 29 23:49:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052722.M
Quant Title :
QLast Update : Fri May 27 13:05:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

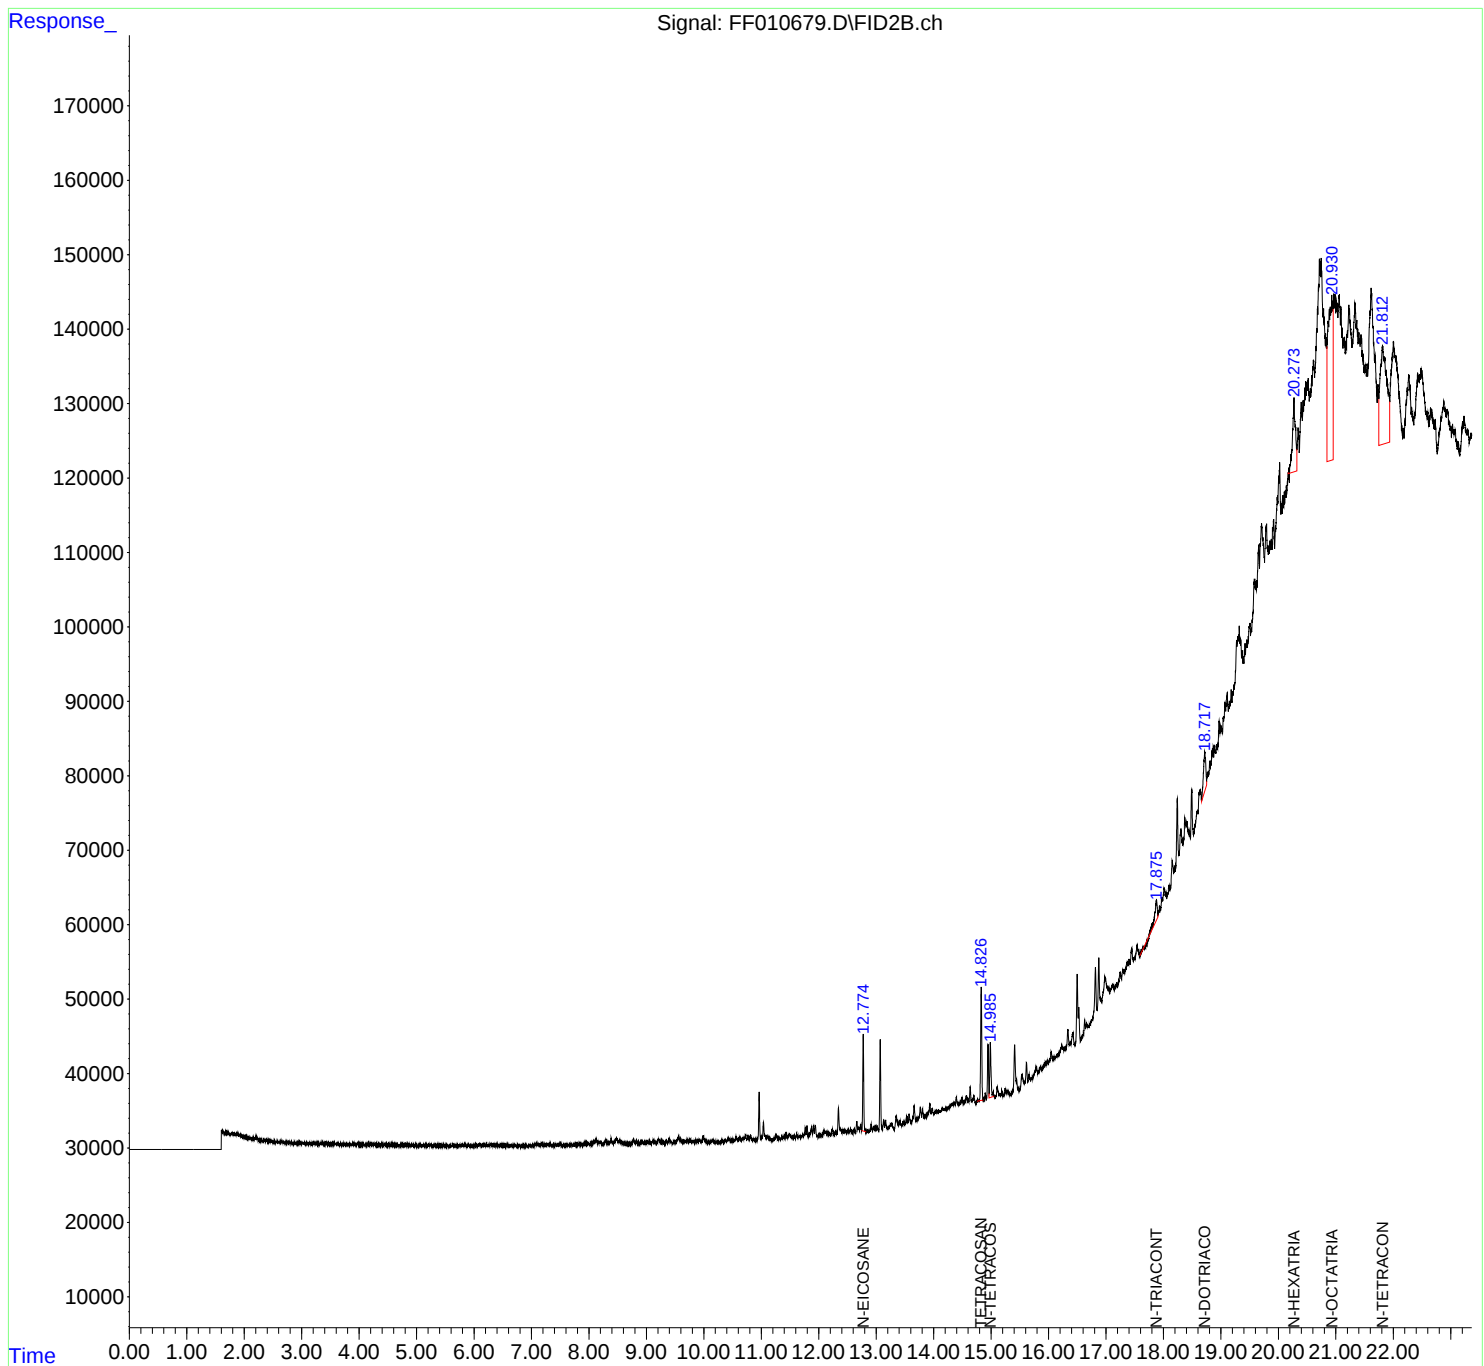


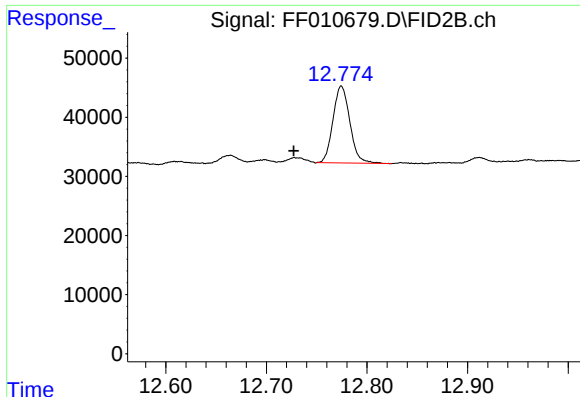

#7 N-EICOSANE


R.T.: 12.775 min
Delta R.T.: 0.047 min
Response: 151108
Conc: 1.13 ug/ml

Instrument :
FID_F
ClientSampleId :

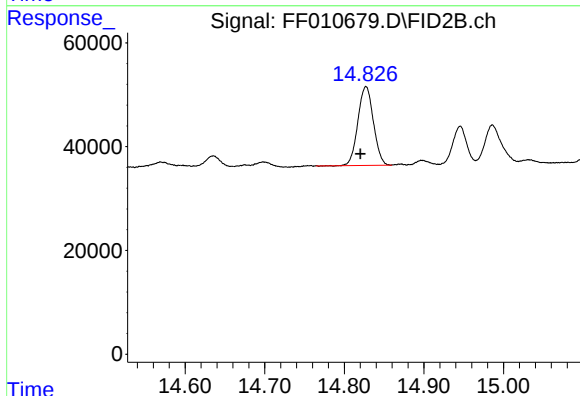


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.827 min
Delta R.T.: 0.007 min
Response: 204910
Conc: 1.77 ug/ml

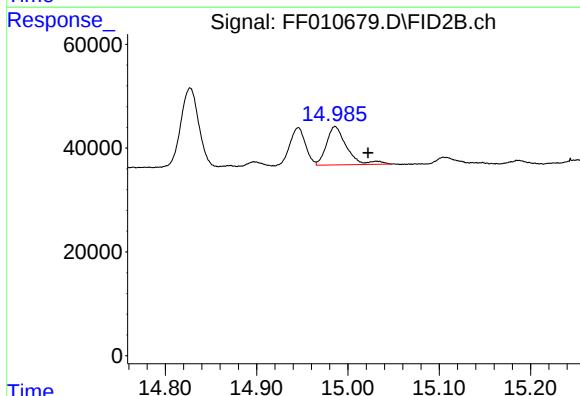


#10 N-TETRACOSANE

R.T.: 14.986 min
Delta R.T.: -0.036 min
Response: 112868
Conc: 0.86 ug/ml

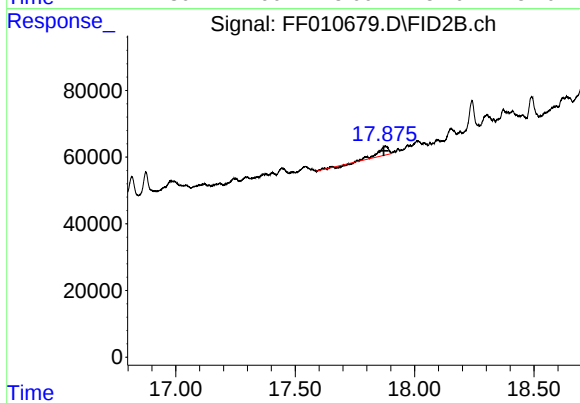

#13 N-TRIACONTANE


R.T.: 17.878 min
Delta R.T.: 0.008 min
Response: 81042
Conc: 0.66 ug/ml

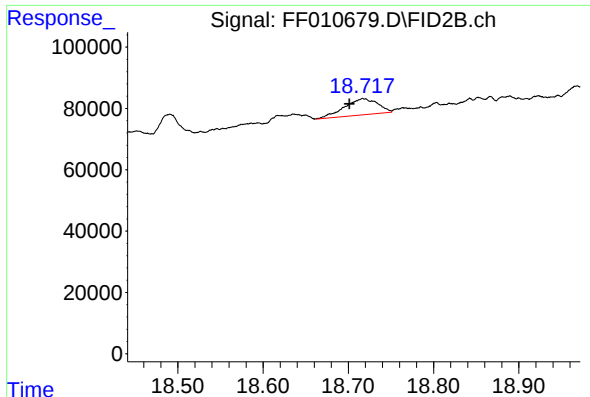

#14 N-DOTRIACONTANE


R.T.: 18.718 min
Delta R.T.: 0.017 min
Response: 143760
Conc: 1.18 ug/ml

Instrument :
FID_F
ClientSampleId :

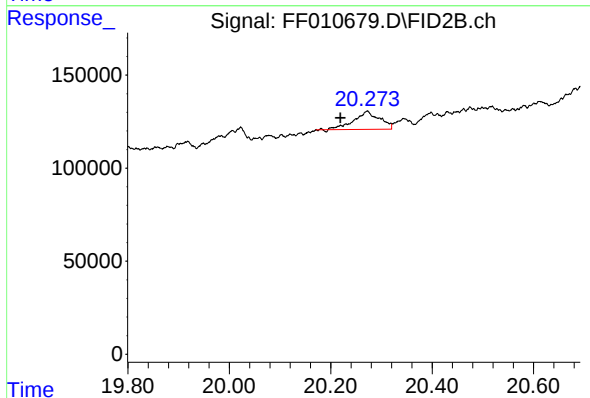


#16 N-HEXATRIACONTANE

R.T.: 20.272 min
Delta R.T.: 0.053 min
Response: 345439
Conc: 4.52 ug/ml

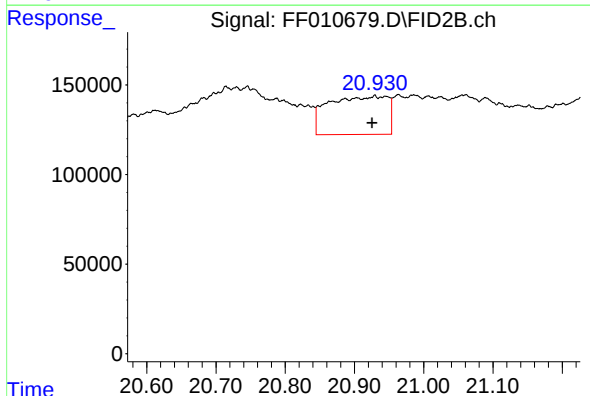

#17 N-OCTATRIACONTANE

R.T.: 20.929 min
Delta R.T.: 0.003 min
Response: 1270420
Conc: 19.94 ug/ml

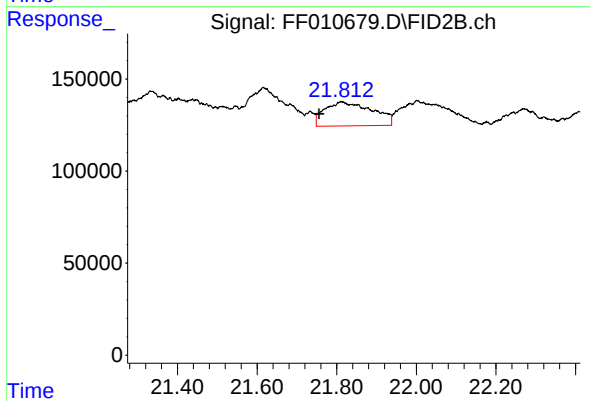

#18 N-TETRACONTANE

R.T.: 21.811 min
Delta R.T.: 0.056 min
Response: 1086416
Conc: 13.31 ug/ml