

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052824\
 Data File : FF014272.D
 Signal(s) : FID2B.ch
 Acq On : 28 May 2024 11:16
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: May 29 03:59:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
 Quant Title :
 QLast Update : Fri May 10 13:22:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.648	2468135	21.233	ug/ml
12) N-OCTACOSANE	17.109	2307901	21.036	ug/ml
14) N-DOTRIACONTANE	18.828	51592	0.404	ug/ml
15) N-TETRATRIACONTANE	19.615	54821	0.540	ug/ml
16) N-HEXATRIACONTANE	20.390	39695	0.415	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF052824\
Data File : FF014272.D
Signal(s) : FID2B.ch
Acq On : 28 May 2024 11:16
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: May 29 03:59:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF051024.M
Quant Title :
QLast Update : Fri May 10 13:22:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

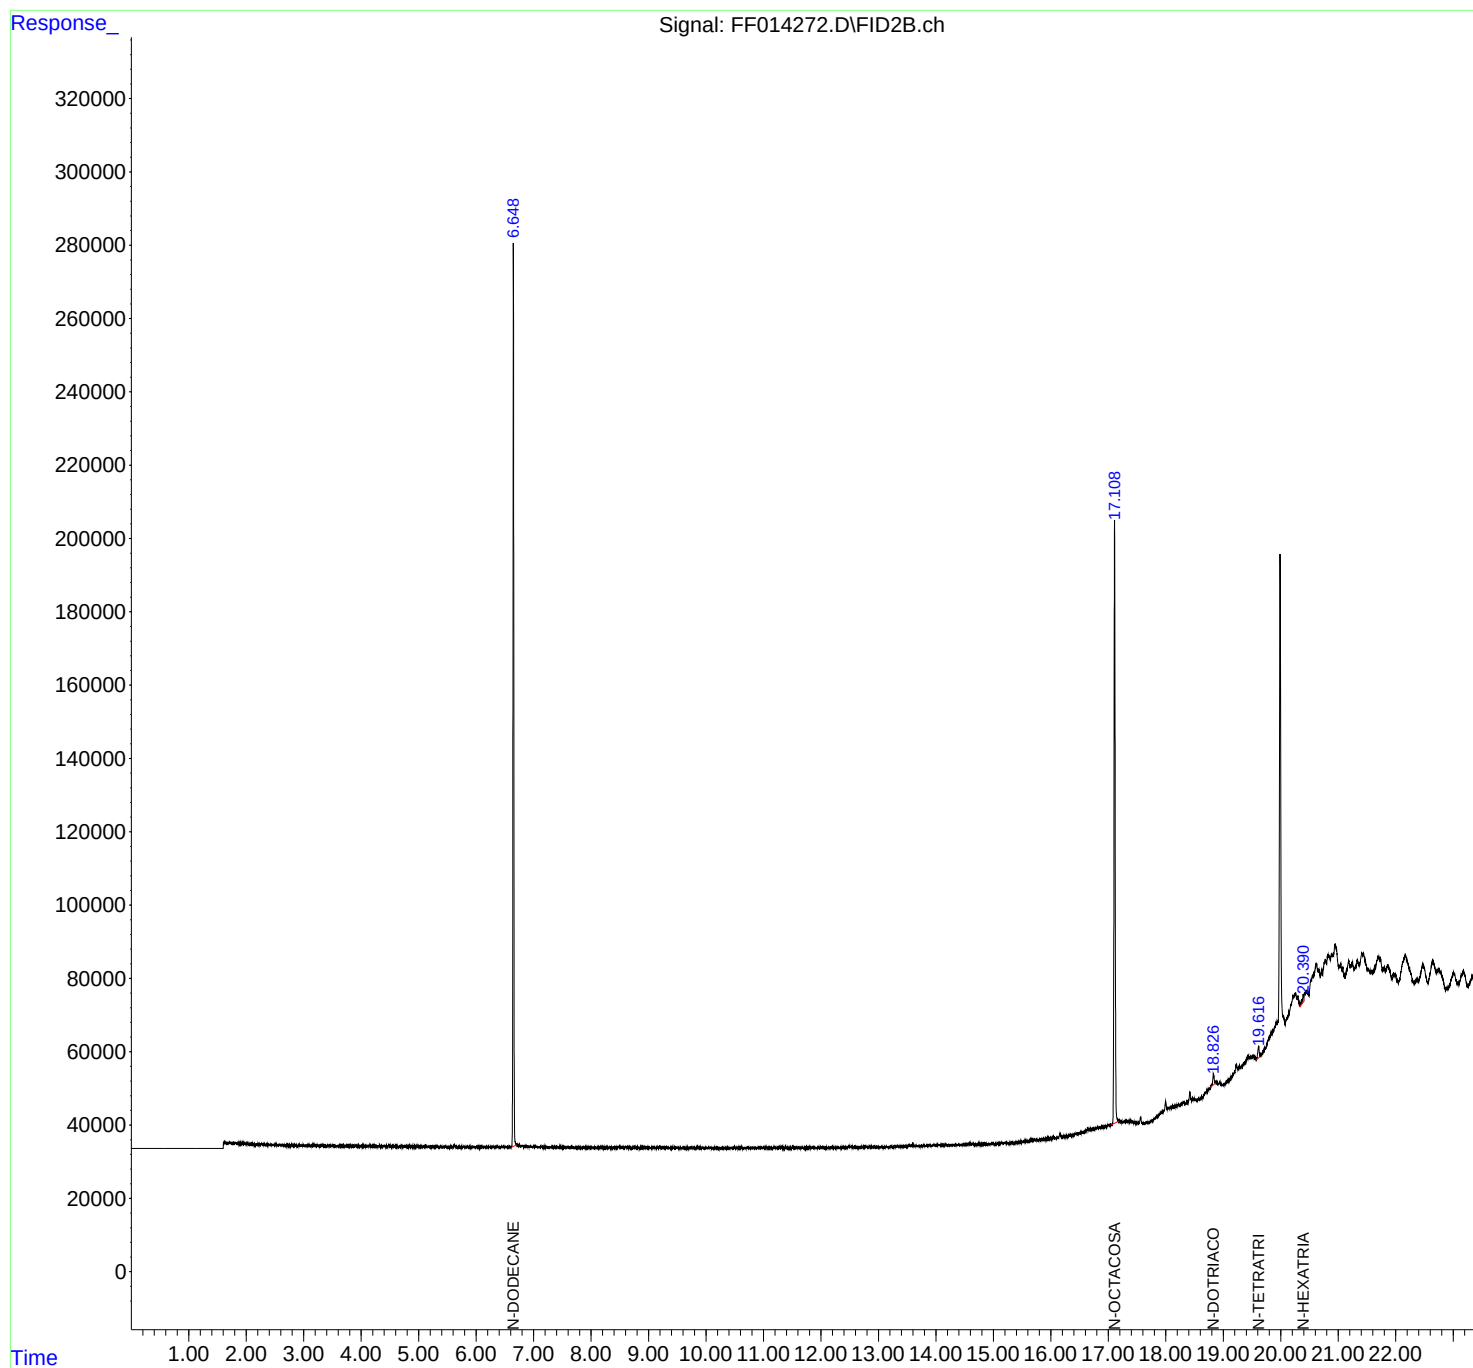


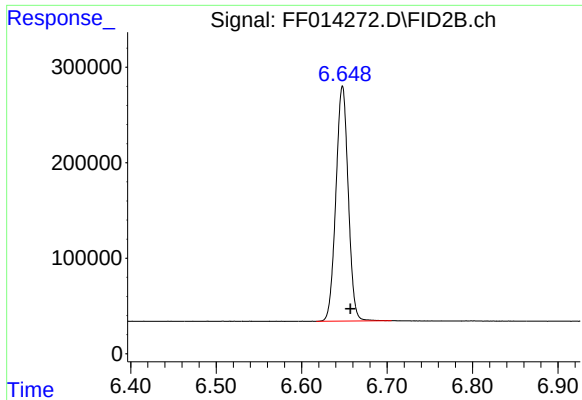

#3 N-DODECANE


R.T.: 6.648 min
Delta R.T.: -0.009 min
Response: 2468135
Conc: 21.23 ug/ml

Instrument :
FID_F
ClientSampleId :

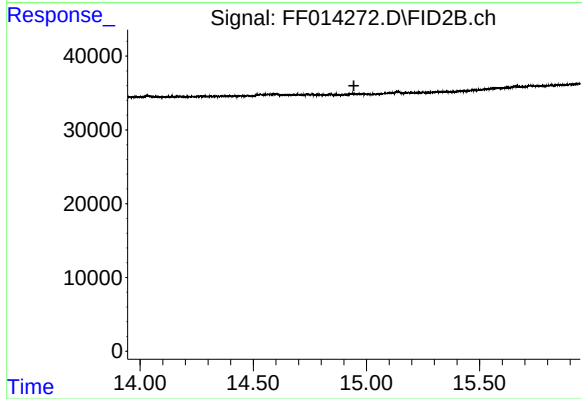


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.944 min
Response: 0
Conc: N.D.

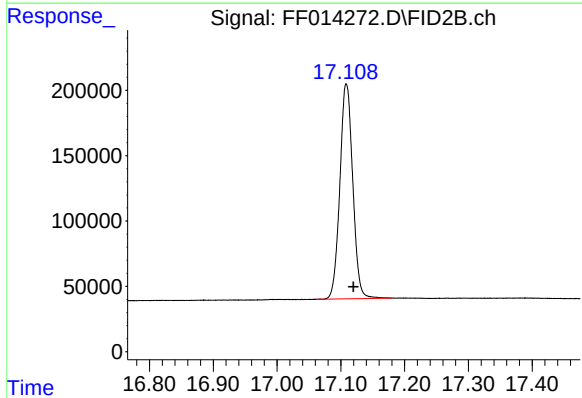


#12 N-OCTACOSANE

R.T.: 17.109 min
Delta R.T.: -0.011 min
Response: 2307901
Conc: 21.04 ug/ml

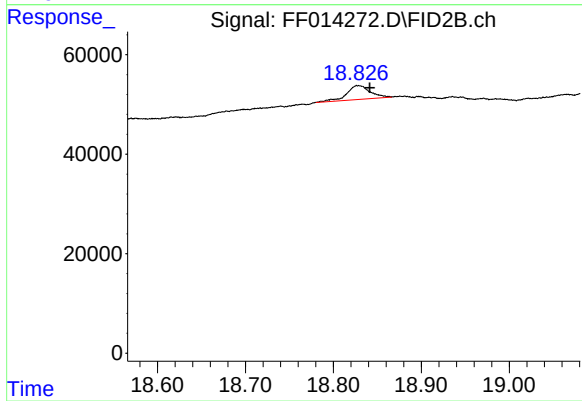

#14 N-DOTRIACONTANE


R.T.: 18.828 min
Delta R.T.: -0.013 min
Response: 51592
Conc: 0.40 ug/ml

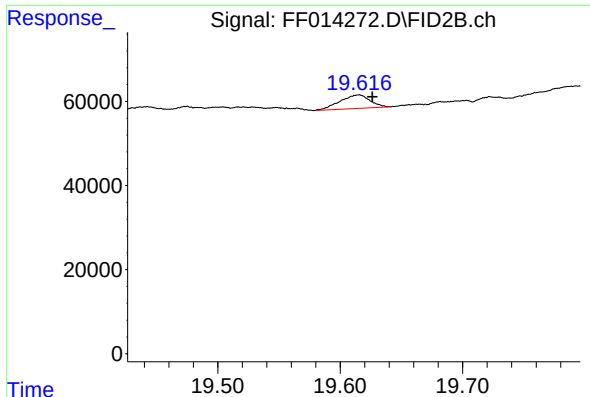

#15 N-TETRATRIACONTANE

R.T.: 19.615 min
Delta R.T.: -0.011 min
Response: 54821
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :

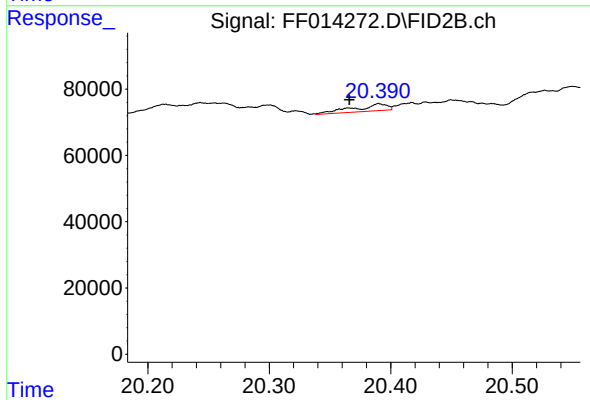

#16 N-HEXATRIACONTANE

R.T.: 20.390 min
Delta R.T.: 0.024 min
Response: 39695
Conc: 0.41 ug/ml