

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF052920\  
Data File : FF007000.D  
Signal(s) : FID2B.ch  
Acq On : 29 May 2020 14:43  
Operator : DD\AJ  
Sample : L2790-10  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 30 02:03:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF051520.M  
Quant Title :  
QLast Update : Sat May 16 03:36:49 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                          | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.726 | 2152158  | 15.571 ug/ml |
| Target Compounds            |                          |        |          |              |
| 4)                          | N-TETRADECANE            | 8.334f | 1235154  | 7.380 ug/ml  |
| 11)                         | N-HEXACOSANE             | 15.948 | 414187   | 2.700 ug/ml  |
| 12)                         | N-OCTACOSANE             | 16.898 | 1205770  | 8.101 ug/ml  |
| 13)                         | N-TRIACONTANE            | 17.786 | 1539203  | 10.651 ug/ml |
| 14)                         | N-DOTRIACONTANE          | 18.617 | 858201   | 6.447 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF052920\  
Data File : FF007000.D  
Signal(s) : FID2B.ch  
Acq On : 29 May 2020 14:43  
Operator : DD\AJ  
Sample : L2790-10  
Misc :  
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: May 30 02:03:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF051520.M  
Quant Title :  
QLast Update : Sat May 16 03:36:49 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

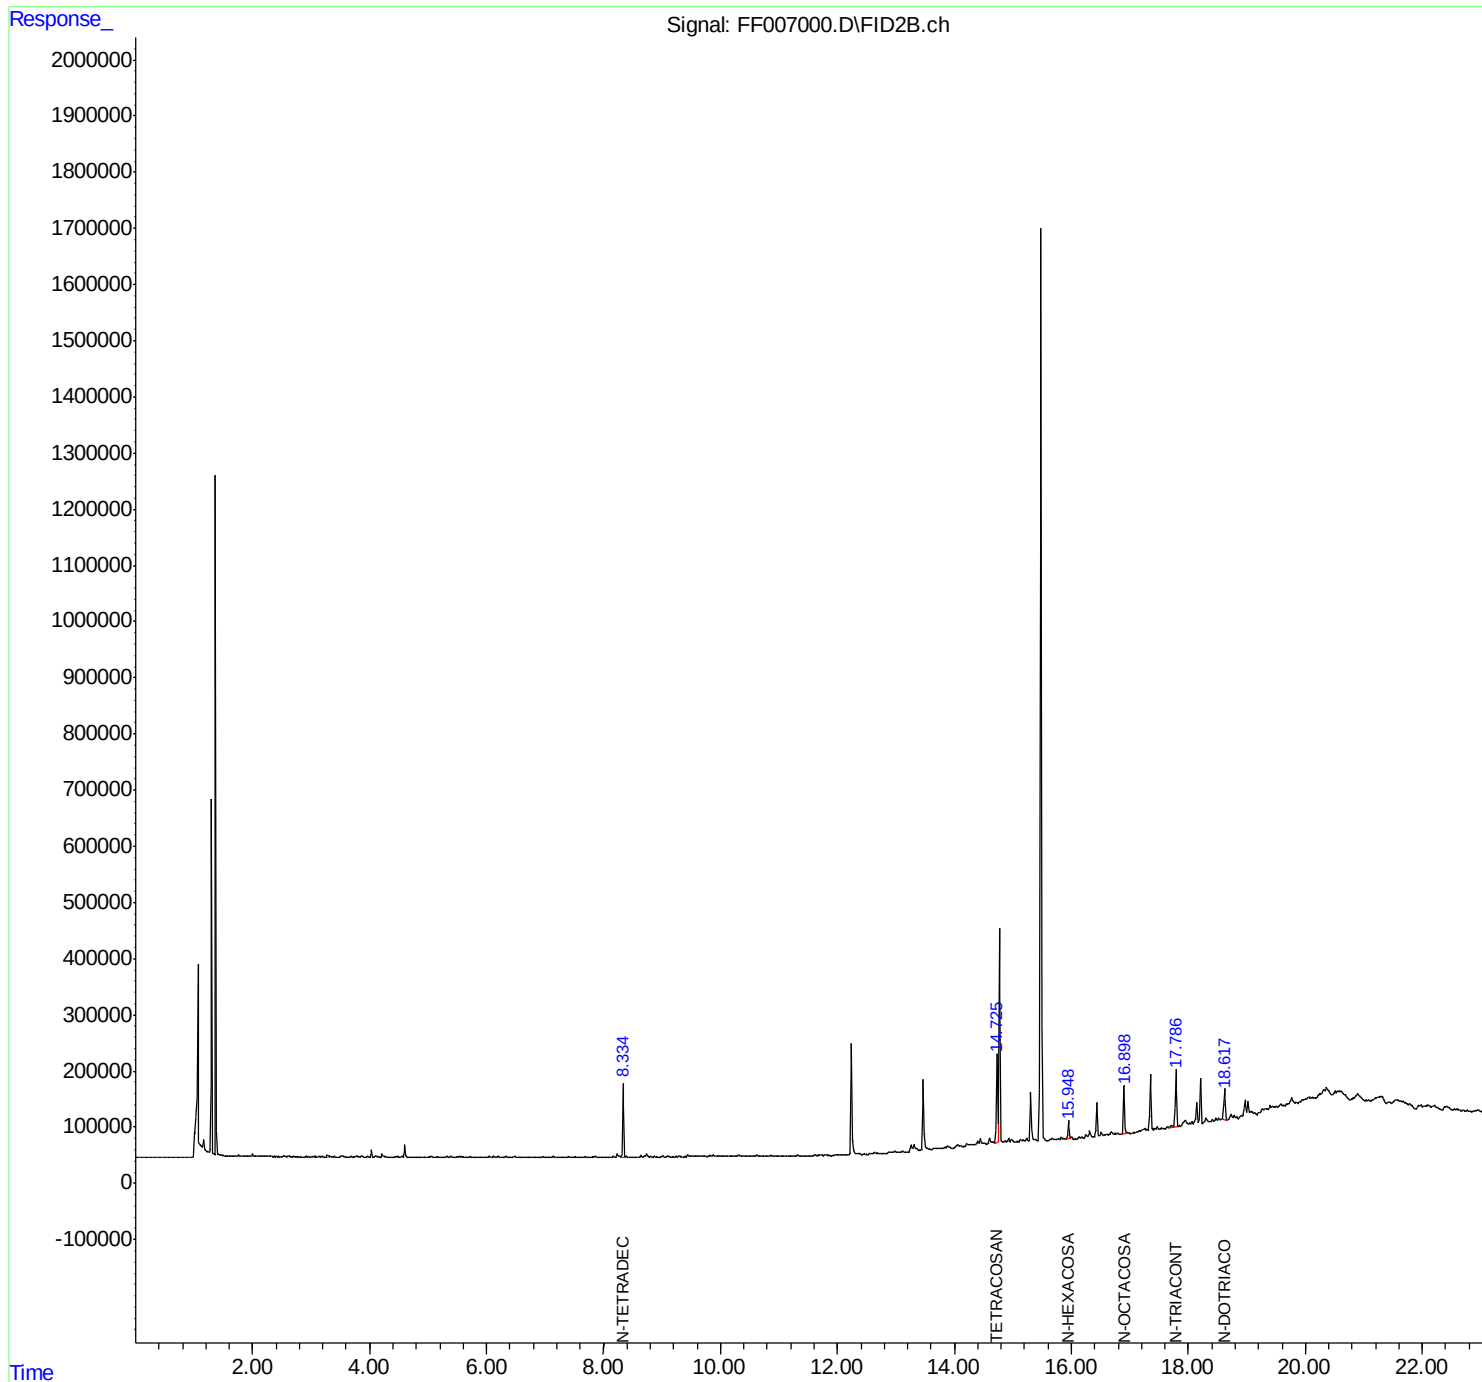

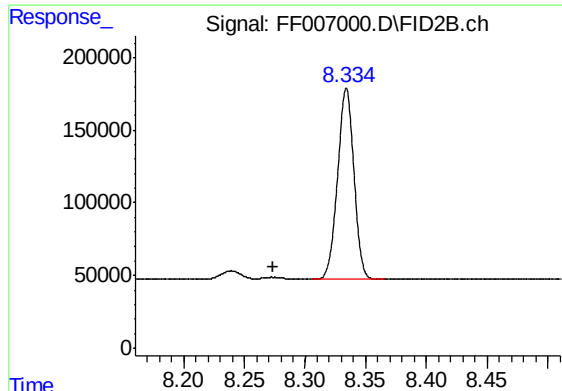


#4 N-TETRADECANE

R.T.: 8.334 min  
Delta R.T.: 0.060 min  
Response: 1235154  
Conc: 7.38 ug/ml

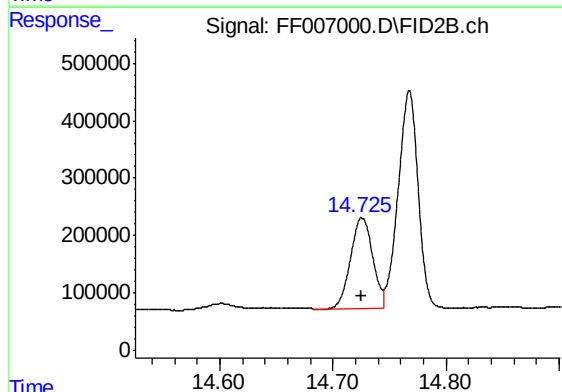


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.726 min  
Delta R.T.: 0.000 min  
Response: 2152158  
Conc: 15.57 ug/ml

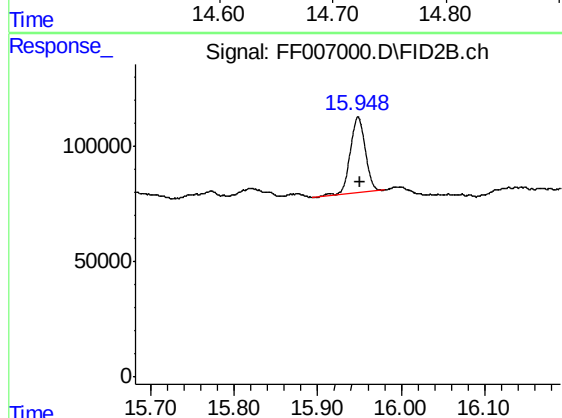


#11 N-HEXACOSANE

R.T.: 15.948 min  
Delta R.T.: -0.002 min  
Response: 414187  
Conc: 2.70 ug/ml

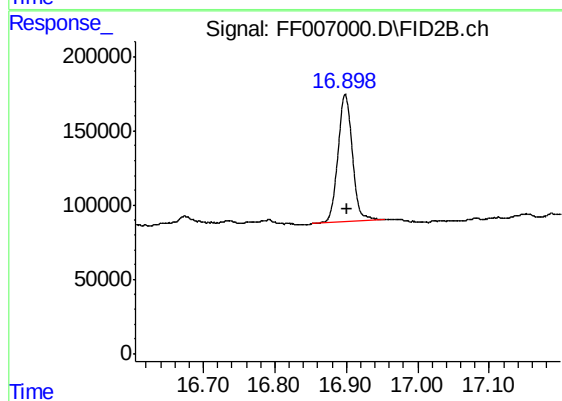


#12 N-OCTACOSANE

R.T.: 16.898 min  
Delta R.T.: -0.002 min  
Response: 1205770  
Conc: 8.10 ug/ml

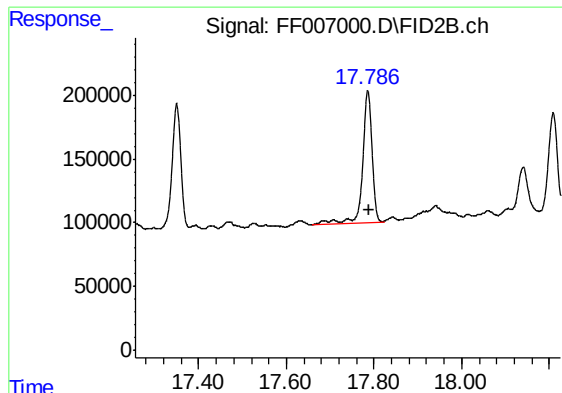

#13 N-TRIACONTANE

R.T.: 17.786 min  
Delta R.T.: -0.002 min  
Response: 1539203  
Conc: 10.65 ug/ml

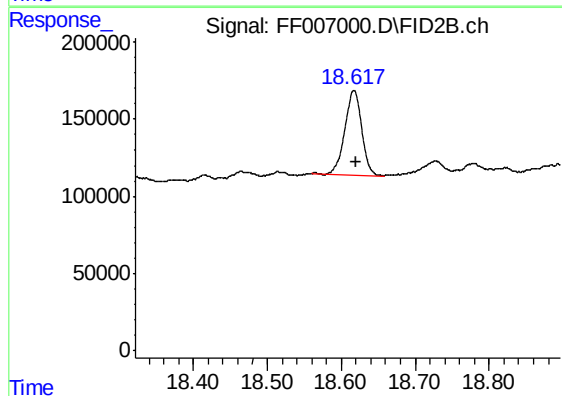

#14 N-DOTRIACONTANE

R.T.: 18.617 min  
Delta R.T.: -0.003 min  
Response: 858201  
Conc: 6.45 ug/ml