

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF053123\
 Data File : FF012791.D
 Signal(s) : FID2B.ch
 Acq On : 31 May 2023 17:07
 Operator : YP\AJ
 Sample : 02983-07
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 01 07:56:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
 Quant Title :
 QLast Update : Fri May 05 16:23:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.987	1909277	15.816 ug/ml
Target Compounds			
7) N-EICOSANE	12.970f	247238	1.786 ug/ml
13) N-TRIACONTANE	18.052	656461	5.249 ug/ml
14) N-DOTRIACONTANE	18.878	631432	5.286 ug/ml
15) N-TETRATRIACONTANE	19.672	133913	1.217 ug/ml
16) N-HEXATRIACONTANE	20.405	250713	2.409 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF053123\
Data File : FF012791.D
Signal(s) : FID2B.ch
Acq On : 31 May 2023 17:07
Operator : YP\AJ
Sample : 02983-07
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 01 07:56:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050523.M
Quant Title :
QLast Update : Fri May 05 16:23:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

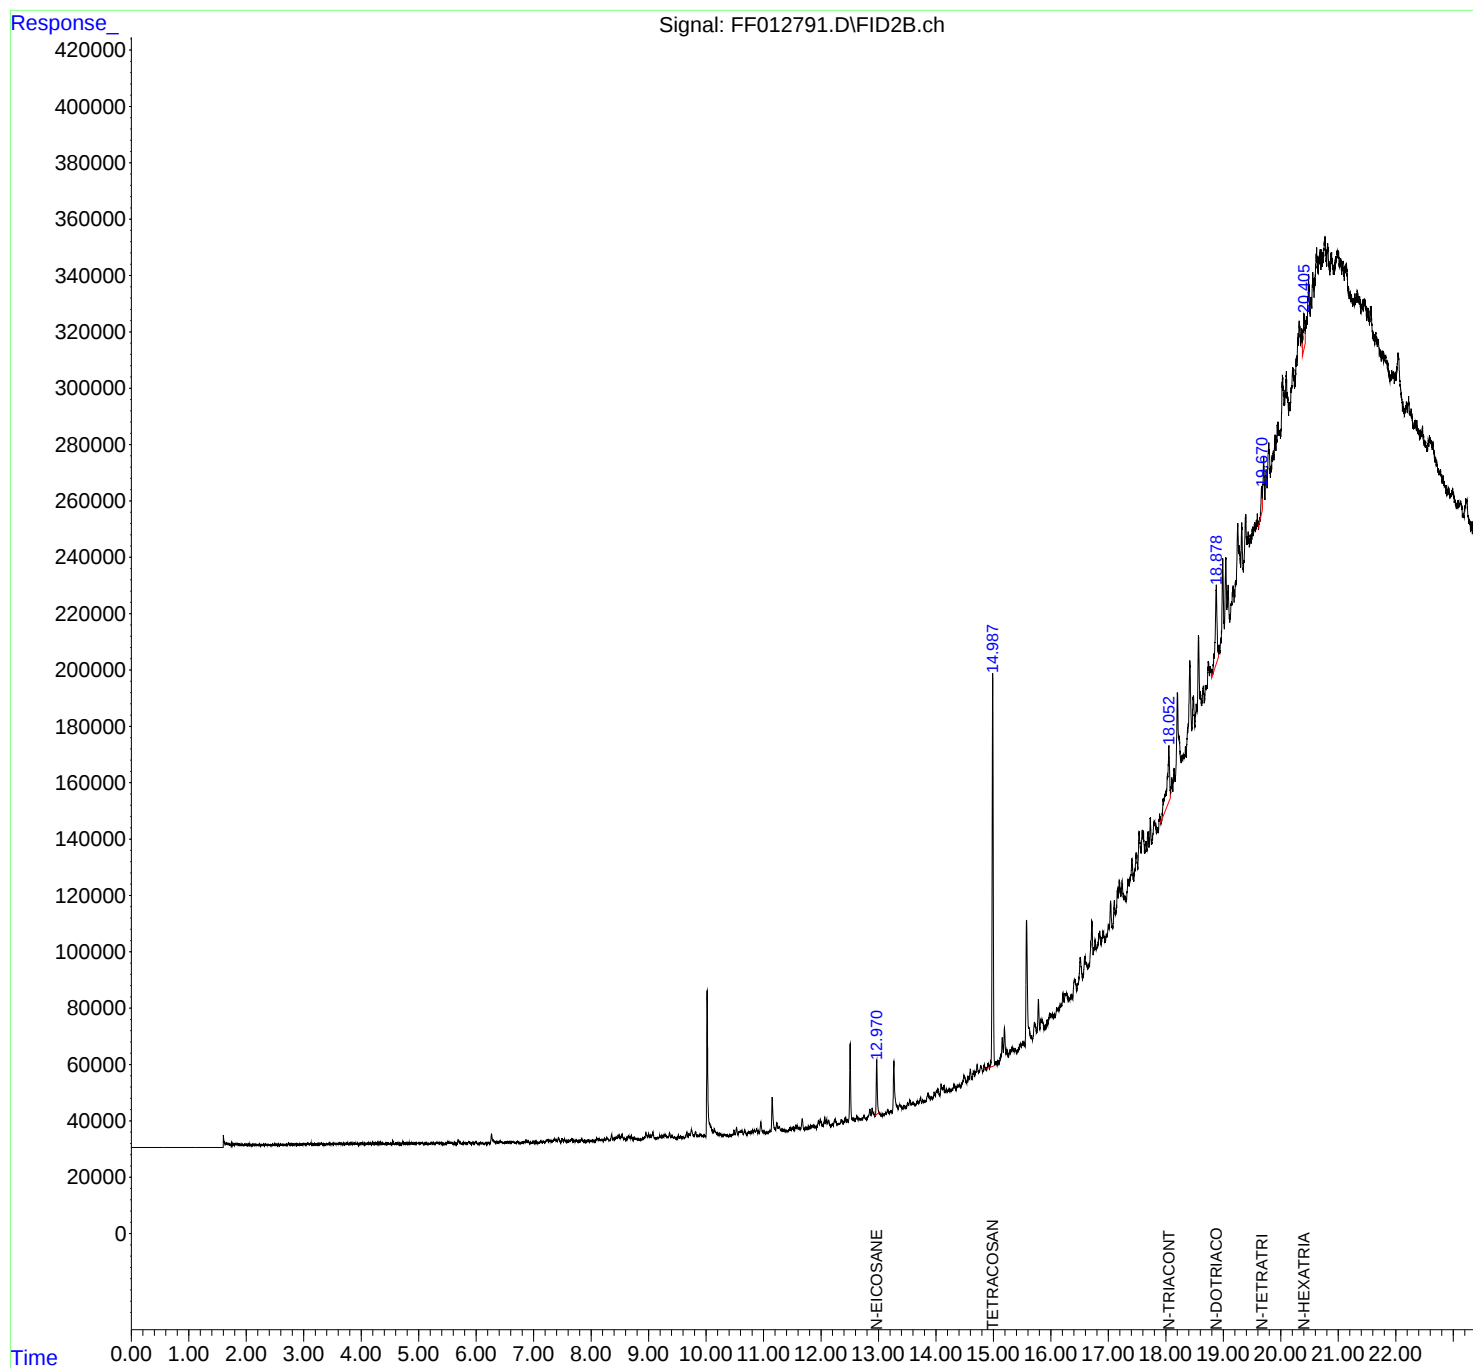


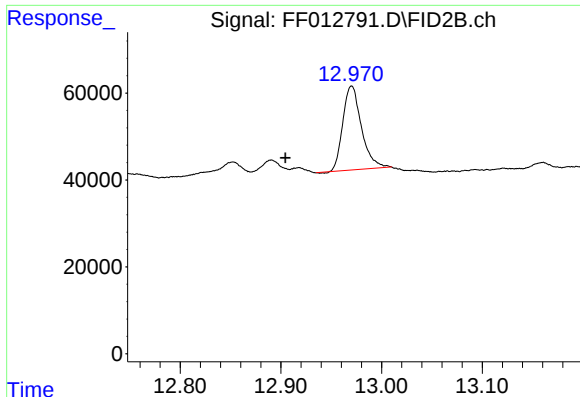

#7 N-EICOSANE


R.T.: 12.970 min
Delta R.T.: 0.066 min
Response: 247238
Conc: 1.79 ug/ml

Instrument :
FID_F
ClientSampleId :

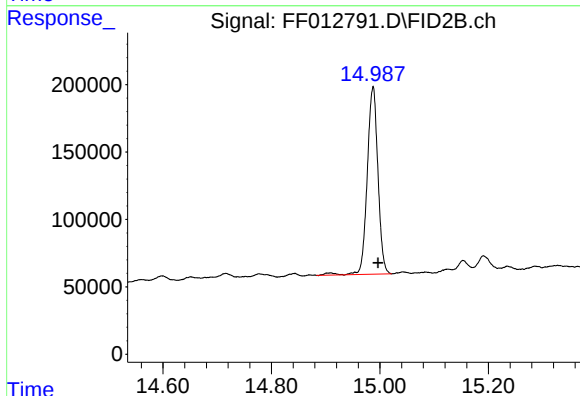


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.987 min
Delta R.T.: -0.009 min
Response: 1909277
Conc: 15.82 ug/ml

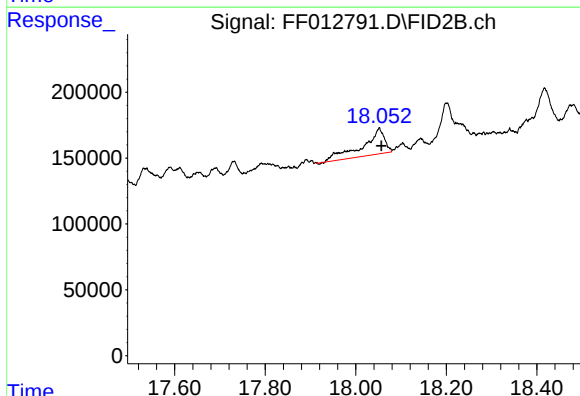


#13 N-TRIACONTANE

R.T.: 18.052 min
Delta R.T.: -0.005 min
Response: 656461
Conc: 5.25 ug/ml

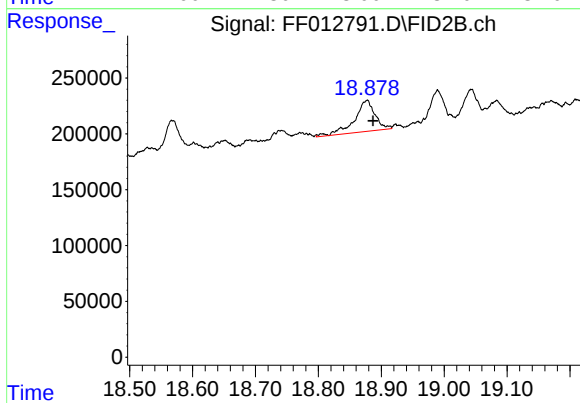

#14 N-DOTRIACONTANE


R.T.: 18.878 min
Delta R.T.: -0.009 min
Response: 631432
Conc: 5.29 ug/ml

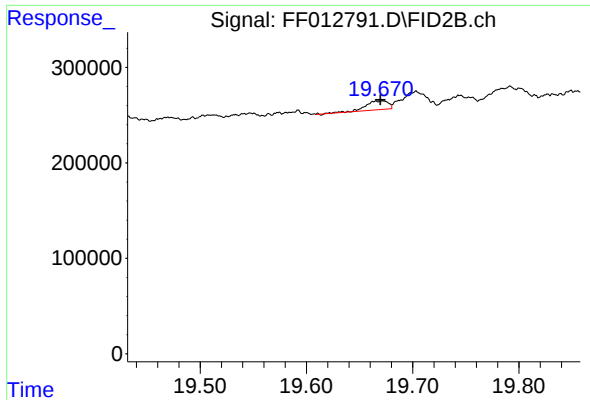

#15 N-TETRATRIACONTANE

R.T.: 19.672 min
Delta R.T.: 0.003 min
Response: 133913
Conc: 1.22 ug/ml

Instrument :
FID_F
ClientSampleId :

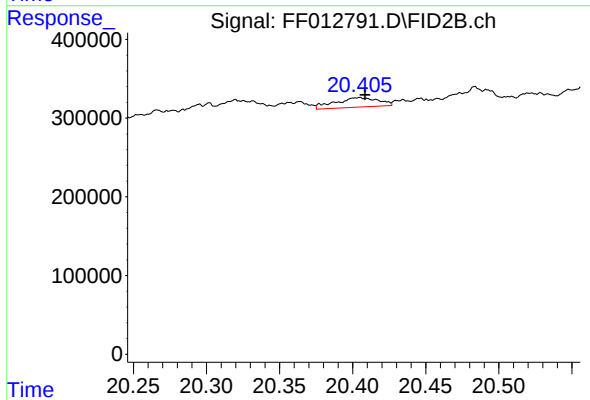

#16 N-HEXATRIACONTANE

R.T.: 20.405 min
Delta R.T.: -0.004 min
Response: 250713
Conc: 2.41 ug/ml