

Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000699.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 14:06
 Operator : UA\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 01 14:40:06 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 14:39:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.490	5801413	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.170	7141771	50.000 ug/ml
2) N-DECANE	4.252	7132028	50.000 ug/ml
3) N-DODECANE	6.266	7131372	50.000 ug/ml
4) N-TETRADECANE	8.054	7068511	50.000 ug/ml
5) N-HEXADECANE	9.650	6978148	50.000 ug/ml
6) N-OCTADECANE	11.088	6898074	50.000 ug/ml
7) N-EICOSANE	12.396	6755094	50.000 ug/ml
8) N-DOCOSANE	13.590	6648913	50.000 ug/ml
10) N-TETRACOSANE	14.692	6532303	50.000 ug/ml
11) N-HEXACOSANE	15.711	6453503	50.000 ug/ml
12) N-OCTACOSANE	16.658	6365555	50.000 ug/ml
13) N-TRIACONTANE	17.545	6284155	50.000 ug/ml
14) N-DOTRIACONTANE	18.375	6072693	50.000 ug/ml
15) N-TETRATRIACONTANE	19.159	5965985	50.000 ug/ml
16) N-HEXATRIACONTANE	19.899	5678189	50.000 ug/ml
17) N-OCTATRIACONTANE	20.612	5121732	50.000 ug/ml
18) N-TETRACONTANE	21.451	5103900	50.000 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000699.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 14:06
 Operator : UA\AJ
 Sample : 50 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampled :

Integration File: autoint1.e
 Quant Time: Jun 01 14:40:06 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 14:39:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

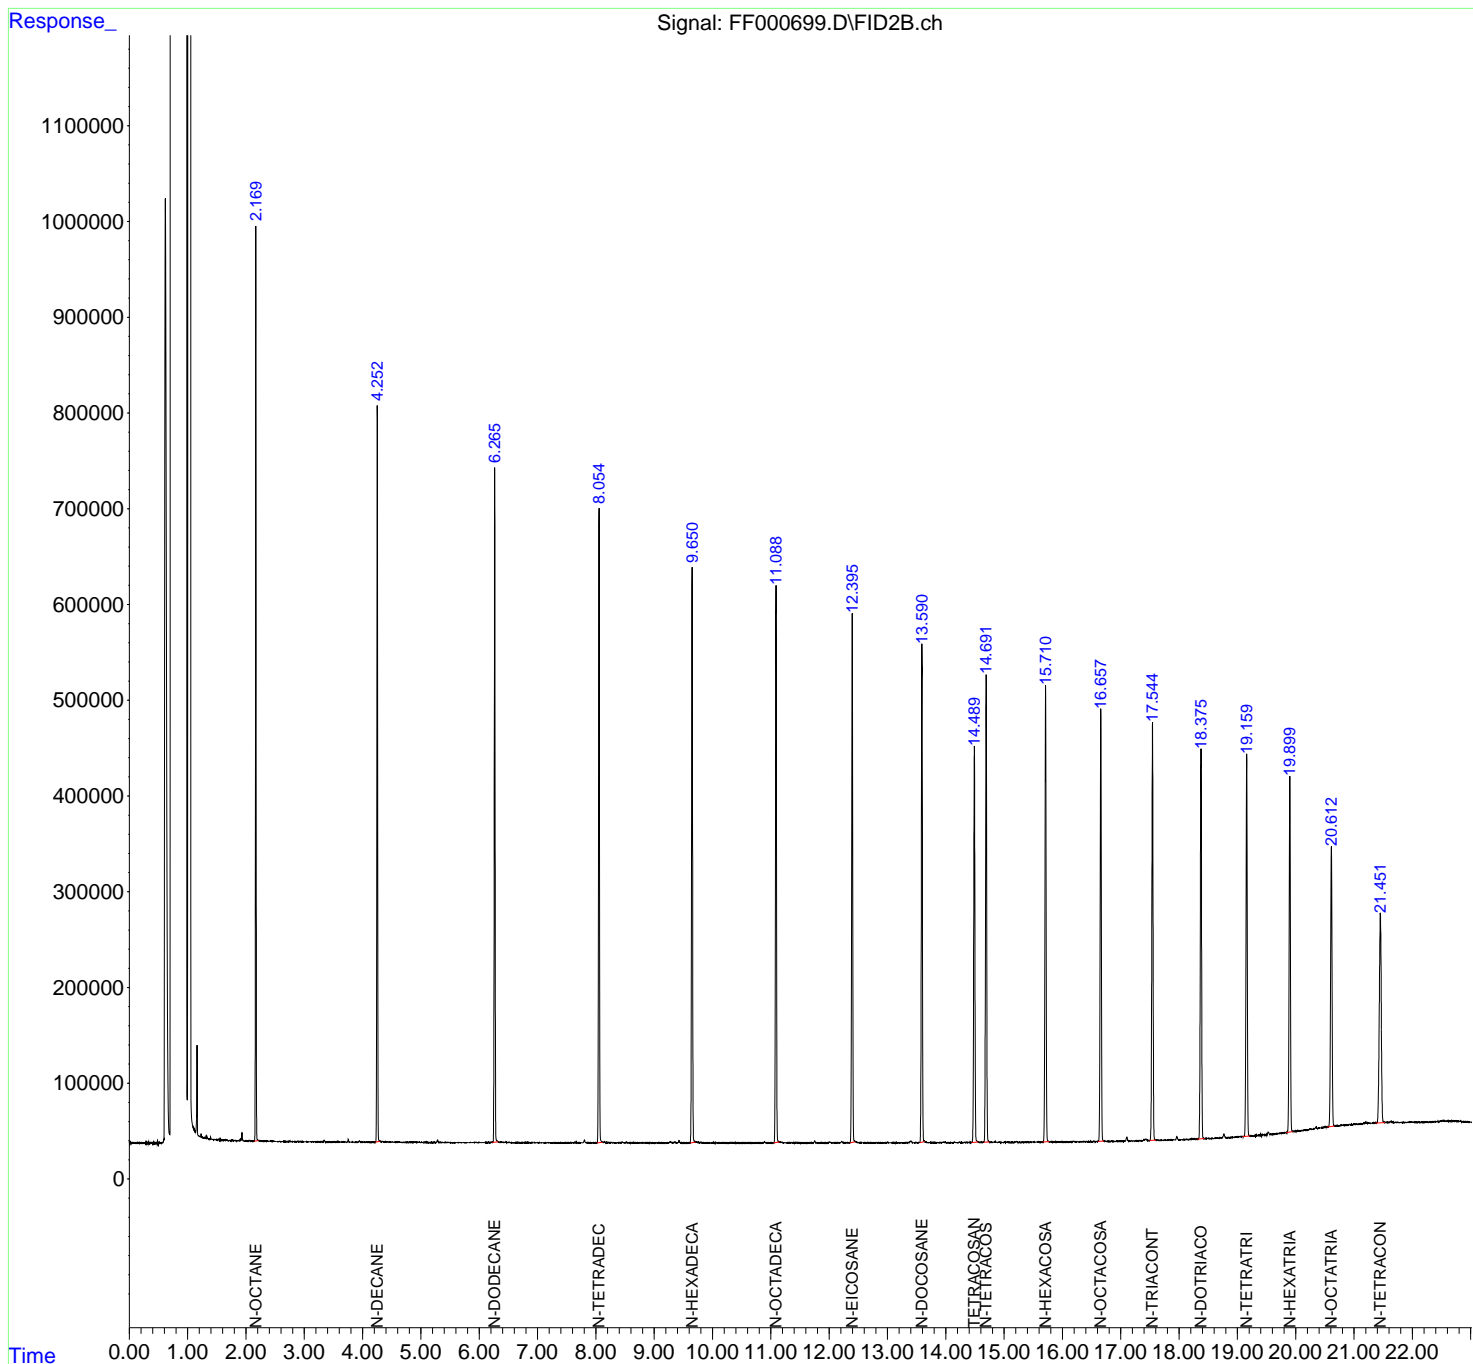

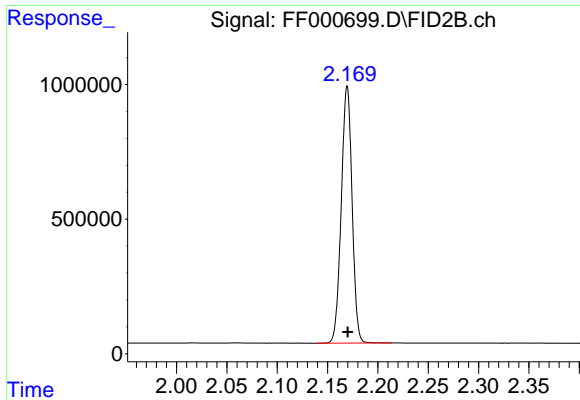


#1 N-OCTANE
 R.T.: 2.170 min
 Delta R.T.: 0.000 min
 Response: 7141771
 Conc: 50.00 ug/ml


Instrument :
 FID_F
 ClientSampleId :

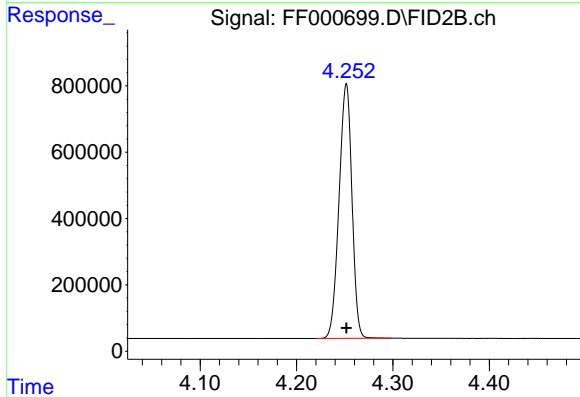


#2 N-DECANE
 R.T.: 4.252 min
 Delta R.T.: 0.000 min
 Response: 7132028
 Conc: 50.00 ug/ml

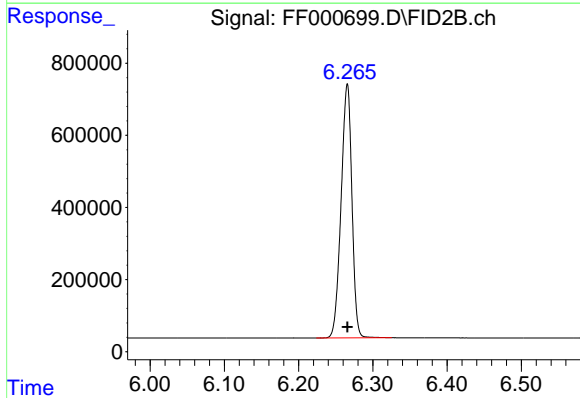

#3 N-DODECANE
 R.T.: 6.266 min
 Delta R.T.: 0.000 min
 Response: 7131372
 Conc: 50.00 ug/ml

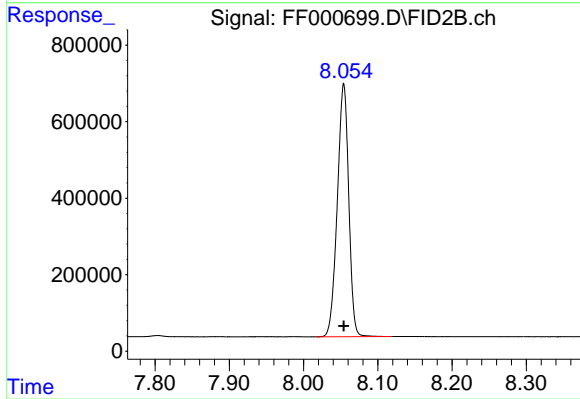


#4 N-TETRADECANE
 R.T.: 8.054 min
 Delta R.T.: 0.000 min
 Response: 7068511
 Conc: 50.00 ug/ml

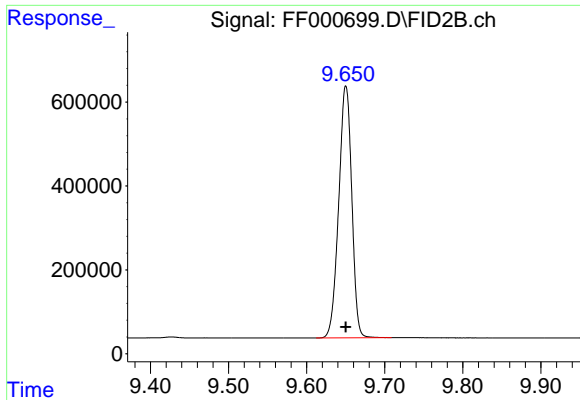


#5 N-HEXADECANE
 R.T.: 9.650 min
 Delta R.T.: 0.000 min
 Response: 6978148
 Conc: 50.00 ug/ml


Instrument :
 FID_F
 ClientSampleId :

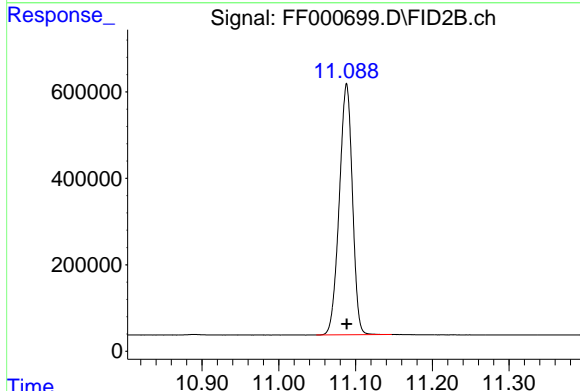


#6 N-OCTADECANE
 R.T.: 11.088 min
 Delta R.T.: 0.000 min
 Response: 6898074
 Conc: 50.00 ug/ml

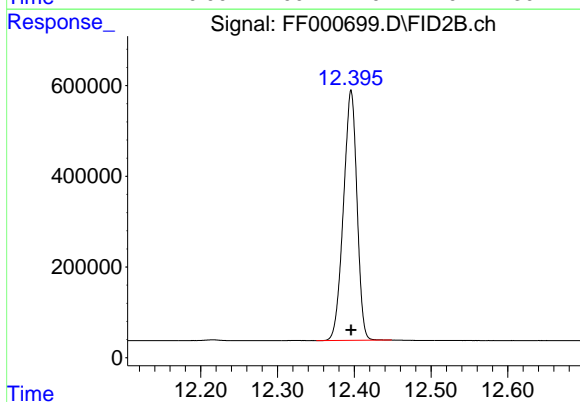

#7 N-EICOSANE
 R.T.: 12.396 min
 Delta R.T.: 0.000 min
 Response: 6755094
 Conc: 50.00 ug/ml

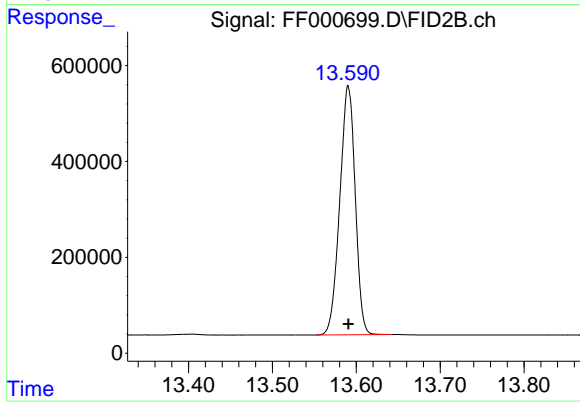


#8 N-DOCOSANE
 R.T.: 13.590 min
 Delta R.T.: 0.000 min
 Response: 6648913
 Conc: 50.00 ug/ml

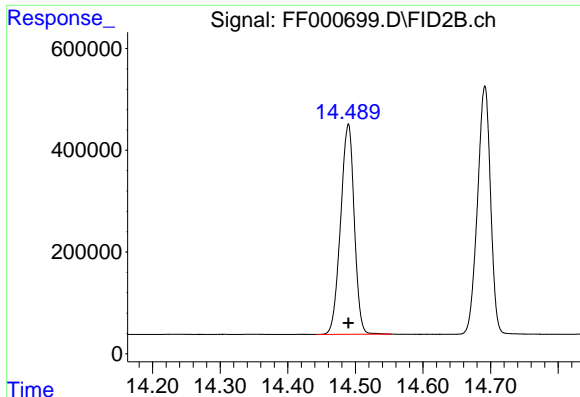

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.490 min
Delta R.T.: 0.000 min
Response: 5801413
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :

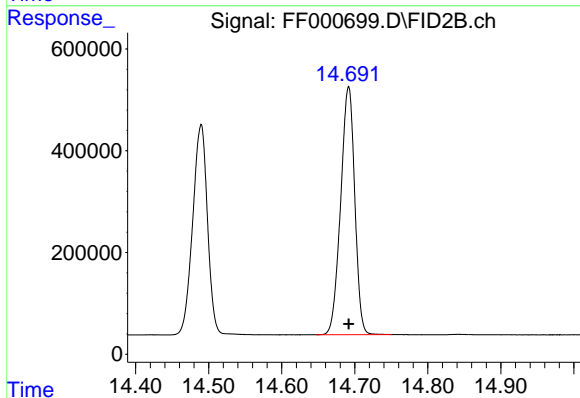


#10 N-TETRACOSANE

R.T.: 14.692 min
Delta R.T.: 0.000 min
Response: 6532303
Conc: 50.00 ug/ml

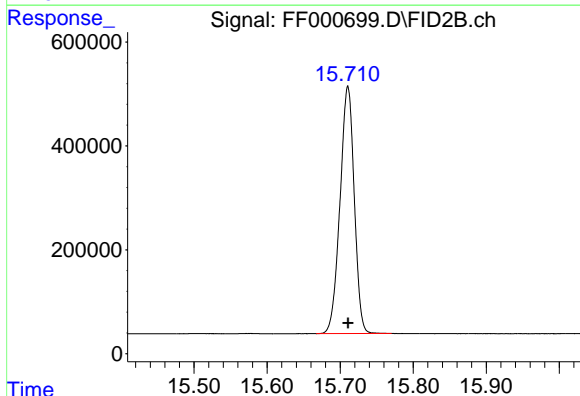


#11 N-HEXACOSANE

R.T.: 15.711 min
Delta R.T.: 0.000 min
Response: 6453503
Conc: 50.00 ug/ml

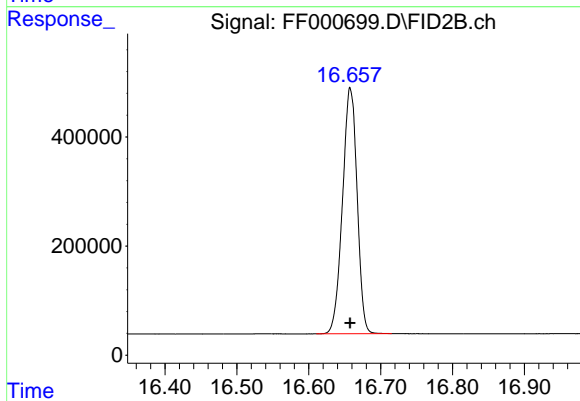

#12 N-OCTACOSANE


R.T.: 16.658 min
Delta R.T.: 0.000 min
Response: 6365555
Conc: 50.00 ug/ml

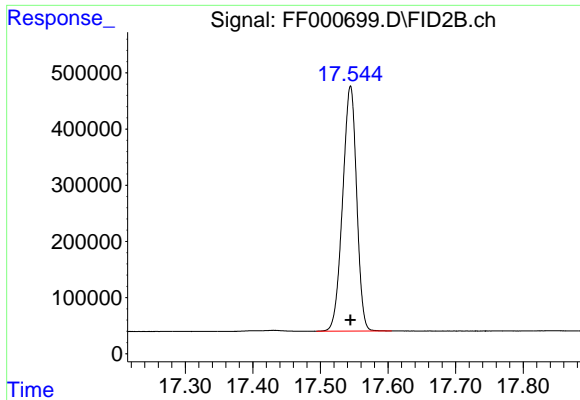

#13 N-TRIACONTANE


R.T.: 17.545 min
Delta R.T.: 0.000 min
Response: 6284155
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :

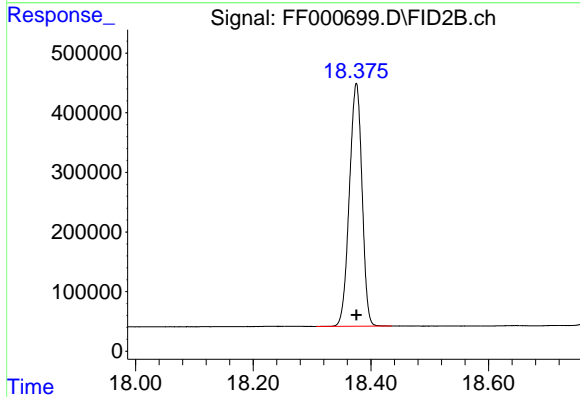


#14 N-DOTRIACONTANE

R.T.: 18.375 min
Delta R.T.: 0.000 min
Response: 6072693
Conc: 50.00 ug/ml

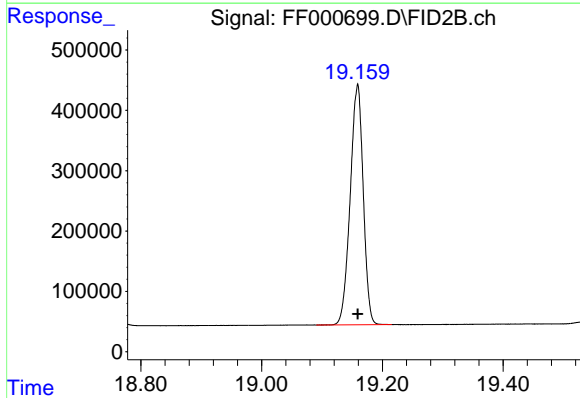


#15 N-TETRATRIACONTANE

R.T.: 19.159 min
Delta R.T.: 0.000 min
Response: 5965985
Conc: 50.00 ug/ml

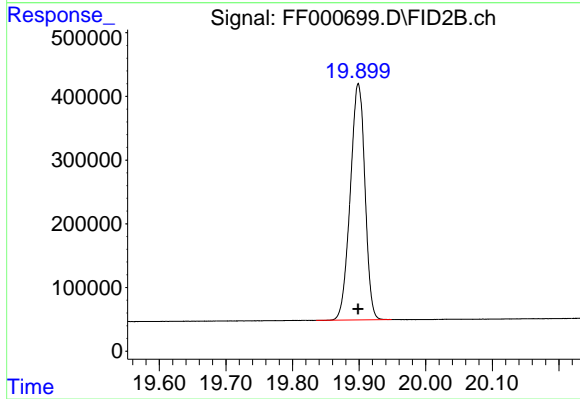

#16 N-HEXATRIACONTANE


R.T.: 19.899 min
Delta R.T.: 0.000 min
Response: 5678189
Conc: 50.00 ug/ml

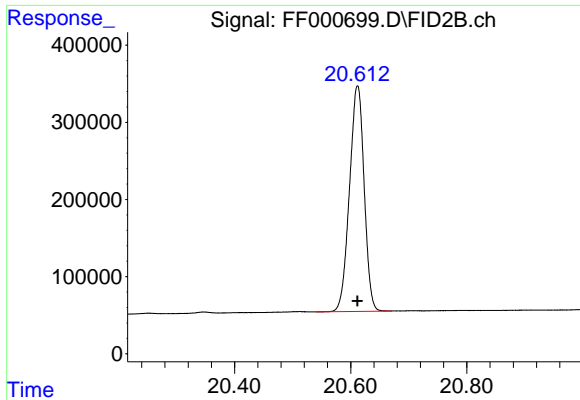

#17 N-OCTATRIACONTANE

R.T.: 20.612 min
Delta R.T.: 0.000 min
Response: 5121732
Conc: 50.00 ug/ml

Instrument :
FID_F
ClientSampleId :

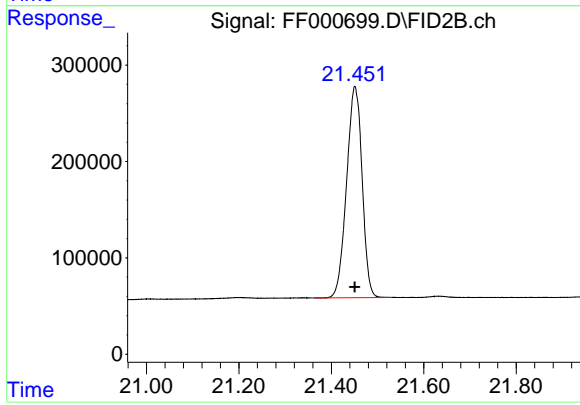

#18 N-TETRACONTANE

R.T.: 21.451 min
Delta R.T.: 0.000 min
Response: 5103900
Conc: 50.00 ug/ml