

Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000705.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 17:06
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 05:26:22 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.488	5872391	50.921 ug/ml
Target Compounds			
2) N-DECANE	4.251	7199454	51.382 ug/ml
3) N-DODECANE	6.265	7189616	51.299 ug/ml
4) N-TETRADECANE	8.054	7128149	51.197 ug/ml
5) N-HEXADECANE	9.650	7042383	51.077 ug/ml
6) N-OCTADECANE	11.088	6971699	51.055 ug/ml
7) N-EICOSANE	12.395	6843720	51.081 ug/ml
8) N-DOCOSANE	13.591	6748795	51.039 ug/ml
10) N-TETRACOSANE	14.692	6627332	51.094 ug/ml
11) N-HEXACOSANE	15.710	6558749	51.063 ug/ml
12) N-OCTACOSANE	16.659	6468962	50.873 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
Data File : FF000705.D
Signal(s) : FID2B.ch
Acq On : 01 Jun 2018 17:06
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 05:26:22 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

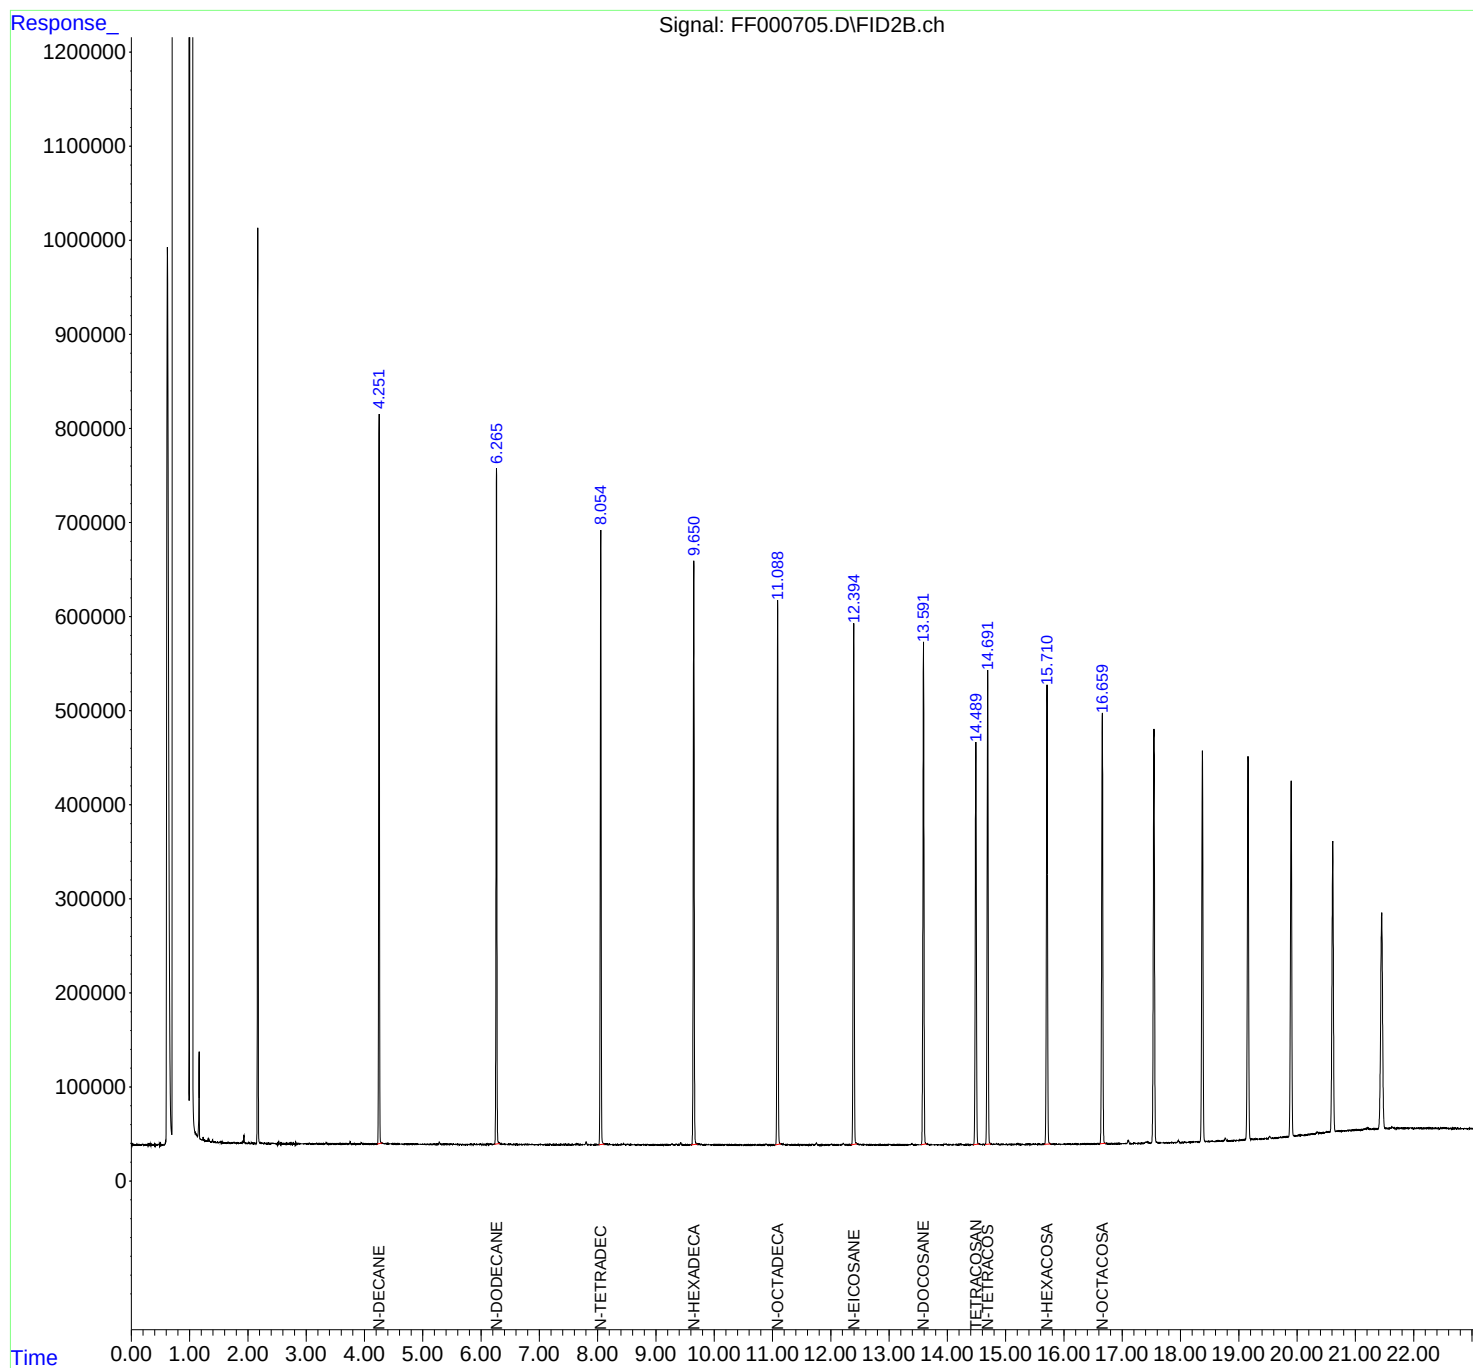


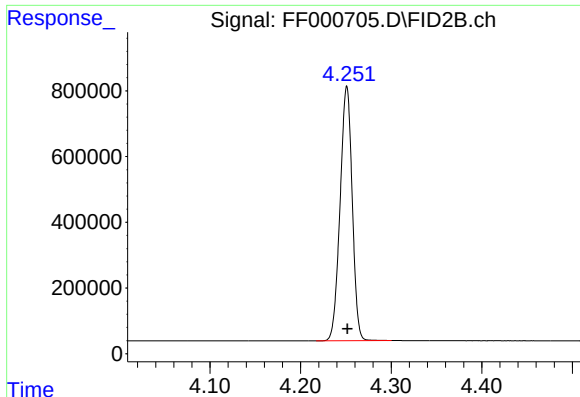

#2 N-DECANE


R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 7199454
Conc: 51.38 ug/ml

Instrument :
FID_F
ClientSampleId :

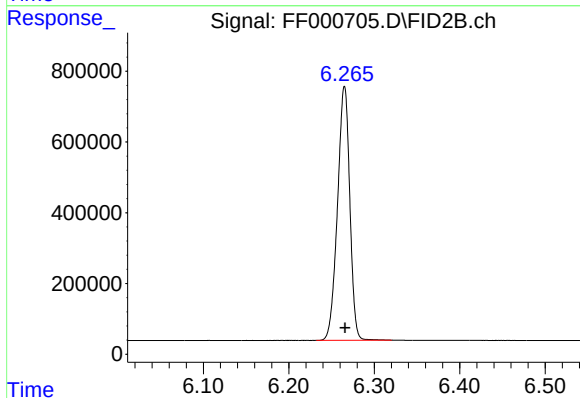


#3 N-DODECANE

R.T.: 6.265 min
Delta R.T.: 0.000 min
Response: 7189616
Conc: 51.30 ug/ml

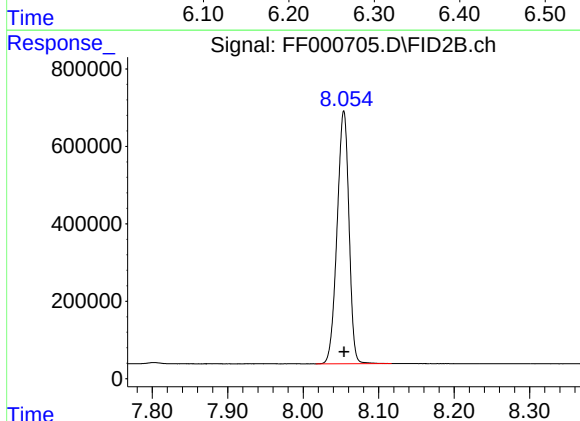


#4 N-TETRADECANE

R.T.: 8.054 min
Delta R.T.: 0.000 min
Response: 7128149
Conc: 51.20 ug/ml

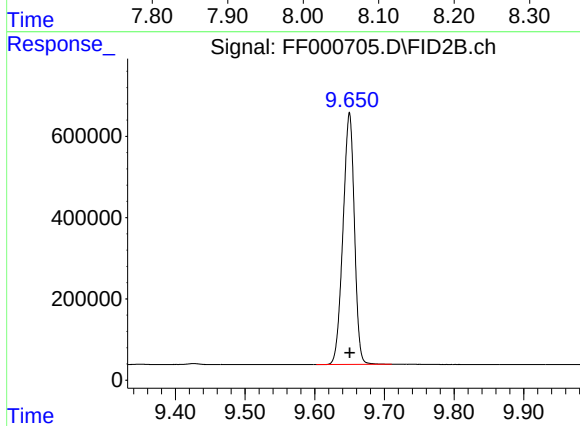

#5 N-HEXADECANE


R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 7042383
Conc: 51.08 ug/ml

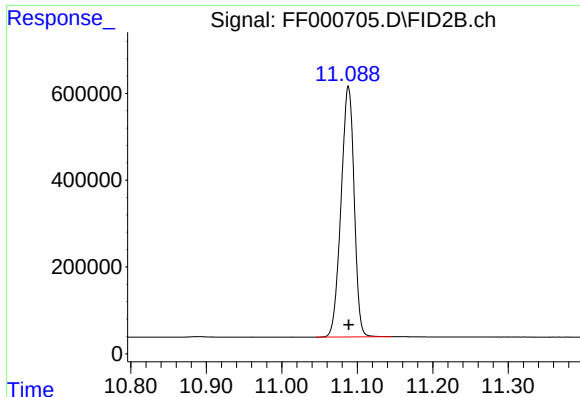

#6 N-OCTADECANE


R.T.: 11.088 min
Delta R.T.: 0.000 min
Response: 6971699
Conc: 51.05 ug/ml

Instrument :
FID_F
ClientSampleId :

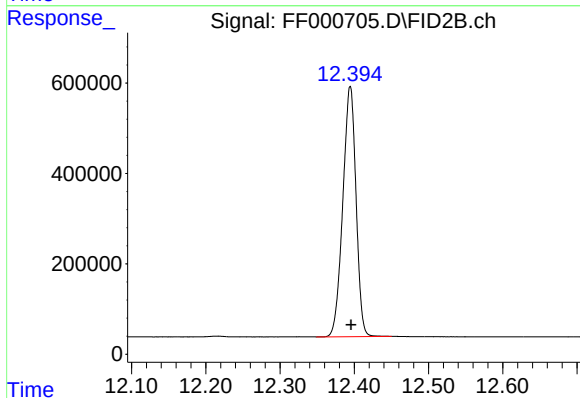


#7 N-EICOSANE

R.T.: 12.395 min
Delta R.T.: -0.001 min
Response: 6843720
Conc: 51.08 ug/ml

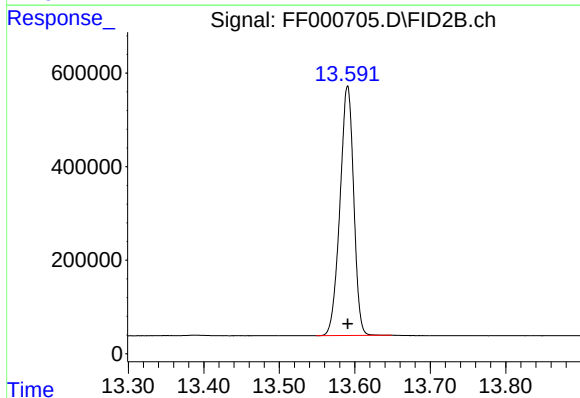


#8 N-DOCOSANE

R.T.: 13.591 min
Delta R.T.: 0.000 min
Response: 6748795
Conc: 51.04 ug/ml

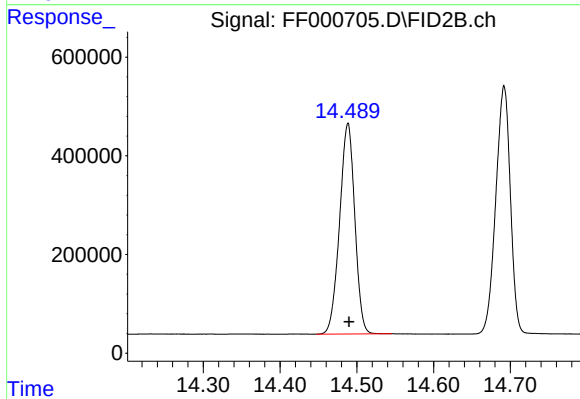

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.488 min
Delta R.T.: -0.001 min
Response: 5872391
Conc: 50.92 ug/ml

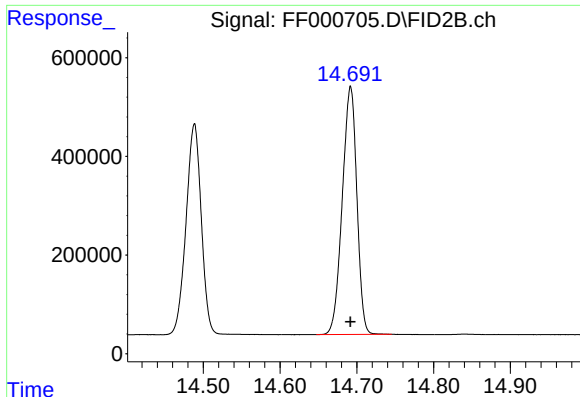

#10 N-TETRACOSANE


R.T.: 14.692 min
Delta R.T.: 0.000 min
Response: 6627332
Conc: 51.09 ug/ml

Instrument :
FID_F
ClientSampleId :

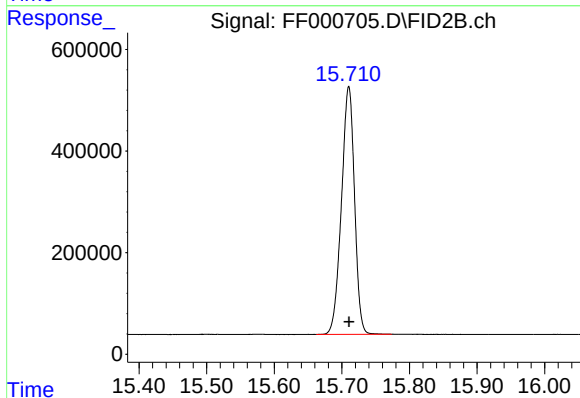

#11 N-HEXACOSANE

R.T.: 15.710 min
Delta R.T.: 0.000 min
Response: 6558749
Conc: 51.06 ug/ml

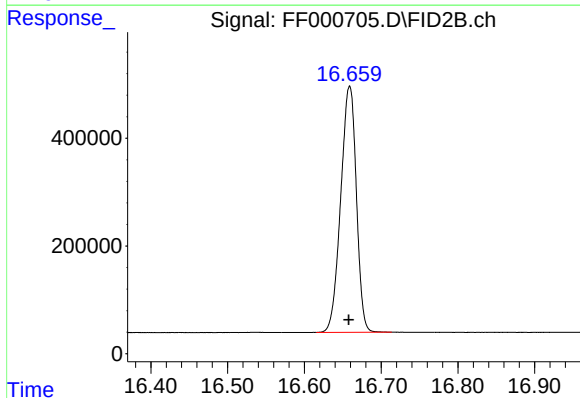

#12 N-OCTACOSANE

R.T.: 16.659 min
Delta R.T.: 0.001 min
Response: 6468962
Conc: 50.87 ug/ml