

Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000707.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 18:06
 Operator : UA\AJ
 Sample : J2923-05
 Misc : Precision Bias study water 01
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 05:26:49 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.487	2565844	22.249 ug/ml
Target Compounds			
2) N-DECANE	4.249	706871	5.045 ug/ml
3) N-DODECANE	6.262	709341	5.061 ug/ml
4) N-TETRADECANE	8.050	706387	5.074 ug/ml
5) N-HEXADECANE	9.646	702416	5.094 ug/ml
6) N-OCTADECANE	11.084	698077	5.112 ug/ml
7) N-EICOSANE	12.391	687293	5.130 ug/ml
8) N-DOCOSANE	13.587	684116	5.174 ug/ml
10) N-TETRACOSANE	14.688	666767	5.140 ug/ml
11) N-HEXACOSANE	15.706	663153	5.163 ug/ml
12) N-OCTACOSANE	16.655	672512	5.289 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
Data File : FF000707.D
Signal(s) : FID2B.ch
Acq On : 01 Jun 2018 18:06
Operator : UA\AJ
Sample : J2923-05
Misc : Precision Bias study water 01
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 05:26:49 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

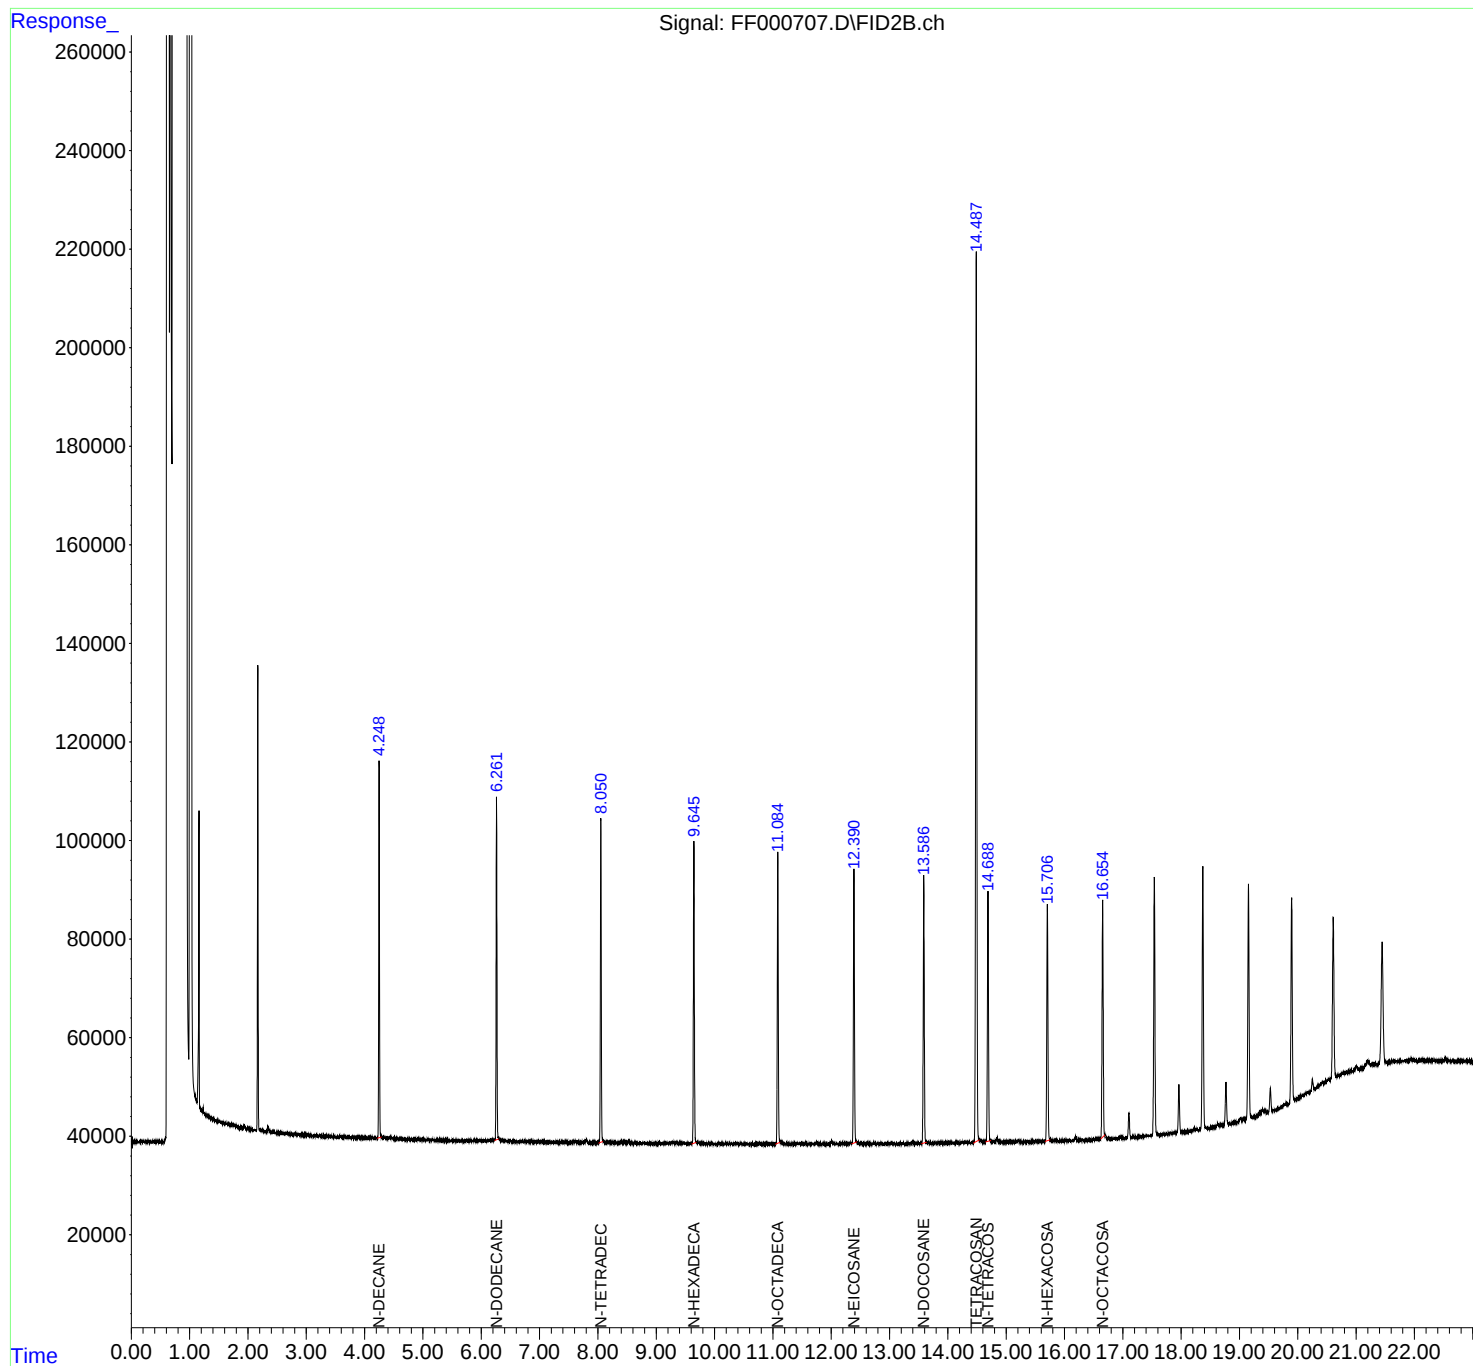


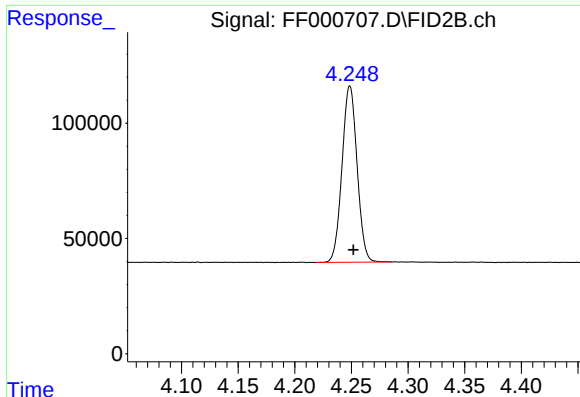

#2 N-DECANE


R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 706871
Conc: 5.04 ug/ml

Instrument :
FID_F
ClientSampleId :

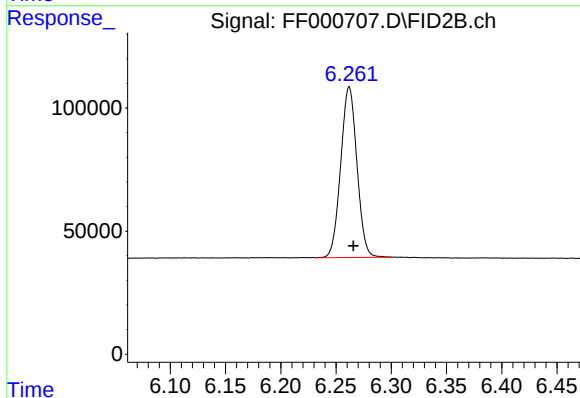


#3 N-DODECANE

R.T.: 6.262 min
Delta R.T.: -0.004 min
Response: 709341
Conc: 5.06 ug/ml

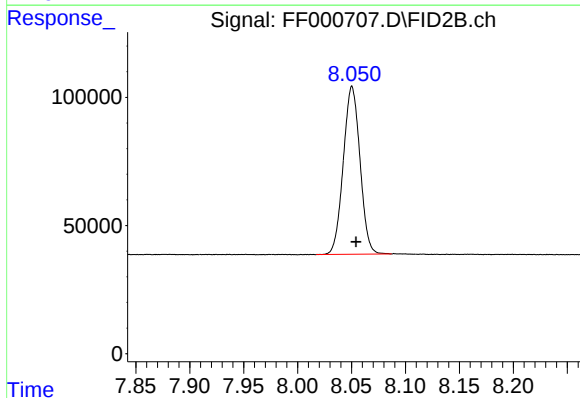


#4 N-TETRADECANE

R.T.: 8.050 min
Delta R.T.: -0.004 min
Response: 706387
Conc: 5.07 ug/ml

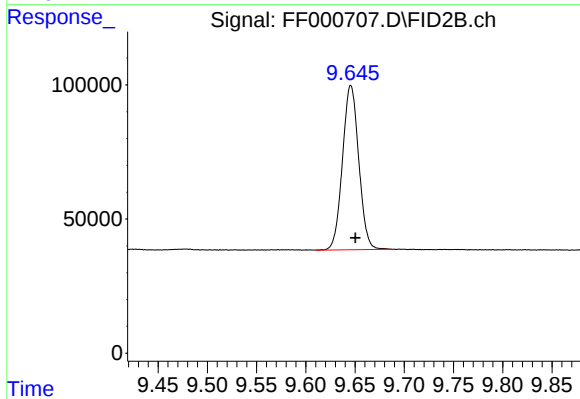

#5 N-HEXADECANE


R.T.: 9.646 min
Delta R.T.: -0.004 min
Response: 702416
Conc: 5.09 ug/ml

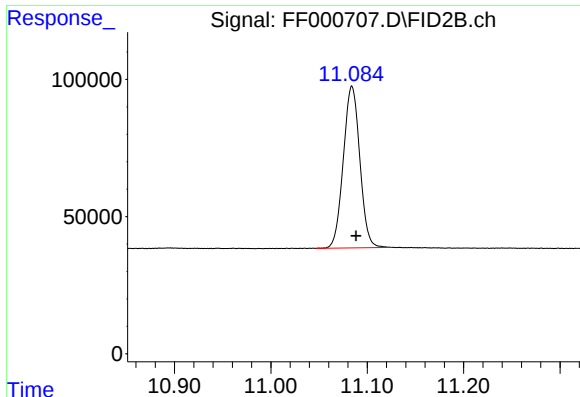

#6 N-OCTADECANE


R.T.: 11.084 min
Delta R.T.: -0.004 min
Response: 698077
Conc: 5.11 ug/ml

Instrument :
FID_F
ClientSampleId :

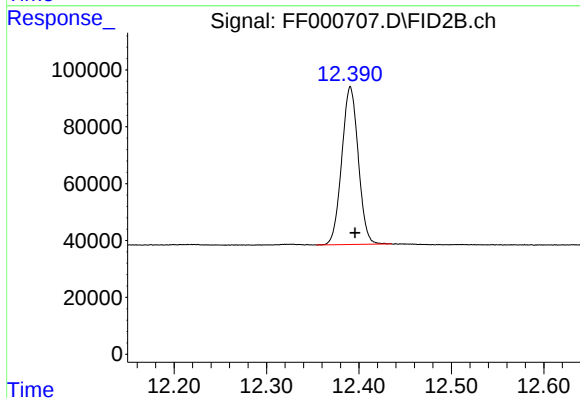


#7 N-EICOSANE

R.T.: 12.391 min
Delta R.T.: -0.005 min
Response: 687293
Conc: 5.13 ug/ml

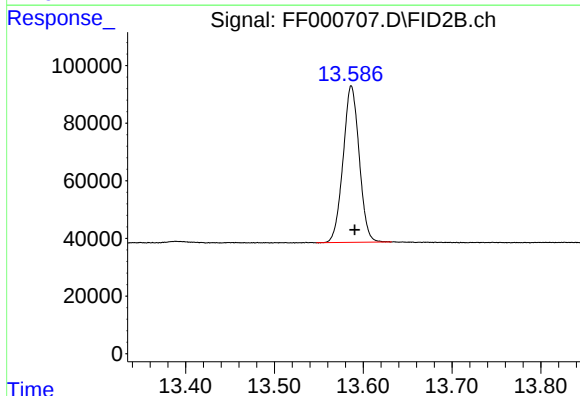


#8 N-DOCOSANE

R.T.: 13.587 min
Delta R.T.: -0.004 min
Response: 684116
Conc: 5.17 ug/ml

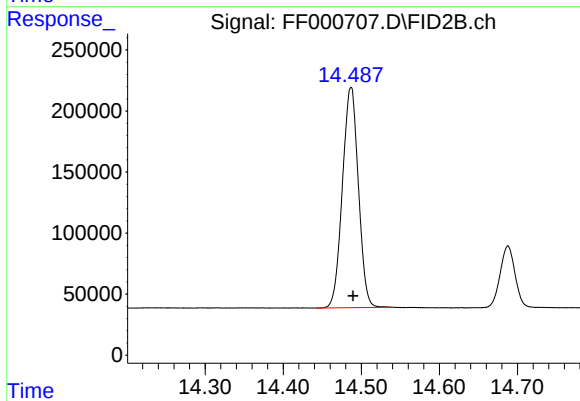

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.487 min
Delta R.T.: -0.003 min
Response: 2565844
Conc: 22.25 ug/ml

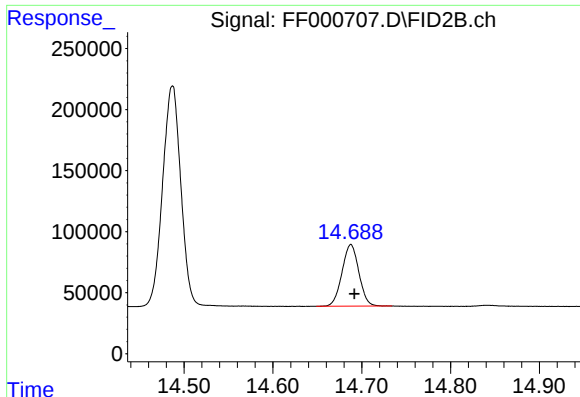

#10 N-TETRACOSANE


R.T.: 14.688 min
Delta R.T.: -0.004 min
Response: 666767
Conc: 5.14 ug/ml

Instrument :
FID_F
ClientSampleId :

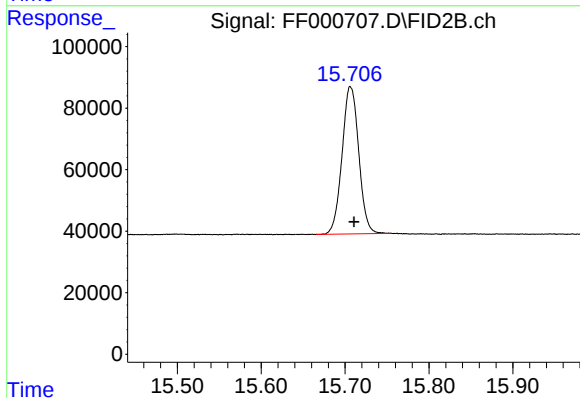

#11 N-HEXACOSANE

R.T.: 15.706 min
Delta R.T.: -0.004 min
Response: 663153
Conc: 5.16 ug/ml

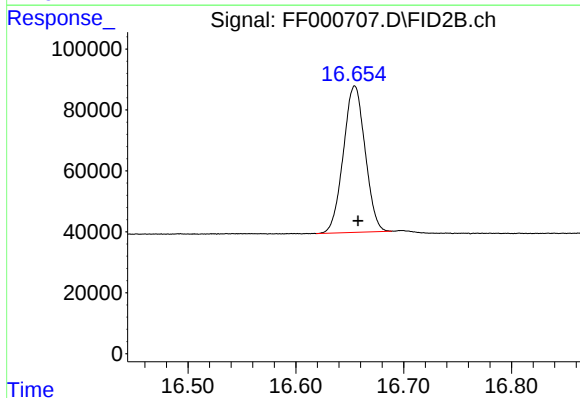

#12 N-OCTACOSANE

R.T.: 16.655 min
Delta R.T.: -0.003 min
Response: 672512
Conc: 5.29 ug/ml