

Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000708.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 18:37
 Operator : UA\AJ
 Sample : J2923-06
 Misc : Precision Bias study water 02
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 05:27:05 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.485	2656968	23.039 ug/ml
Target Compounds			
2) N-DECANE	4.248	730941	5.217 ug/ml
3) N-DODECANE	6.261	731070	5.216 ug/ml
4) N-TETRADECANE	8.050	730279	5.245 ug/ml
5) N-HEXADECANE	9.646	725066	5.259 ug/ml
6) N-OCTADECANE	11.083	720694	5.278 ug/ml
7) N-EICOSANE	12.390	710105	5.300 ug/ml
8) N-DOCOSANE	13.586	706914	5.346 ug/ml
10) N-TETRACOSANE	14.687	686595	5.293 ug/ml
11) N-HEXACOSANE	15.706	683669	5.323 ug/ml
12) N-OCTACOSANE	16.654	692046	5.442 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
Data File : FF000708.D
Signal(s) : FID2B.ch
Acq On : 01 Jun 2018 18:37
Operator : UA\AJ
Sample : J2923-06
Misc : Precision Bias study water 02
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 05:27:05 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

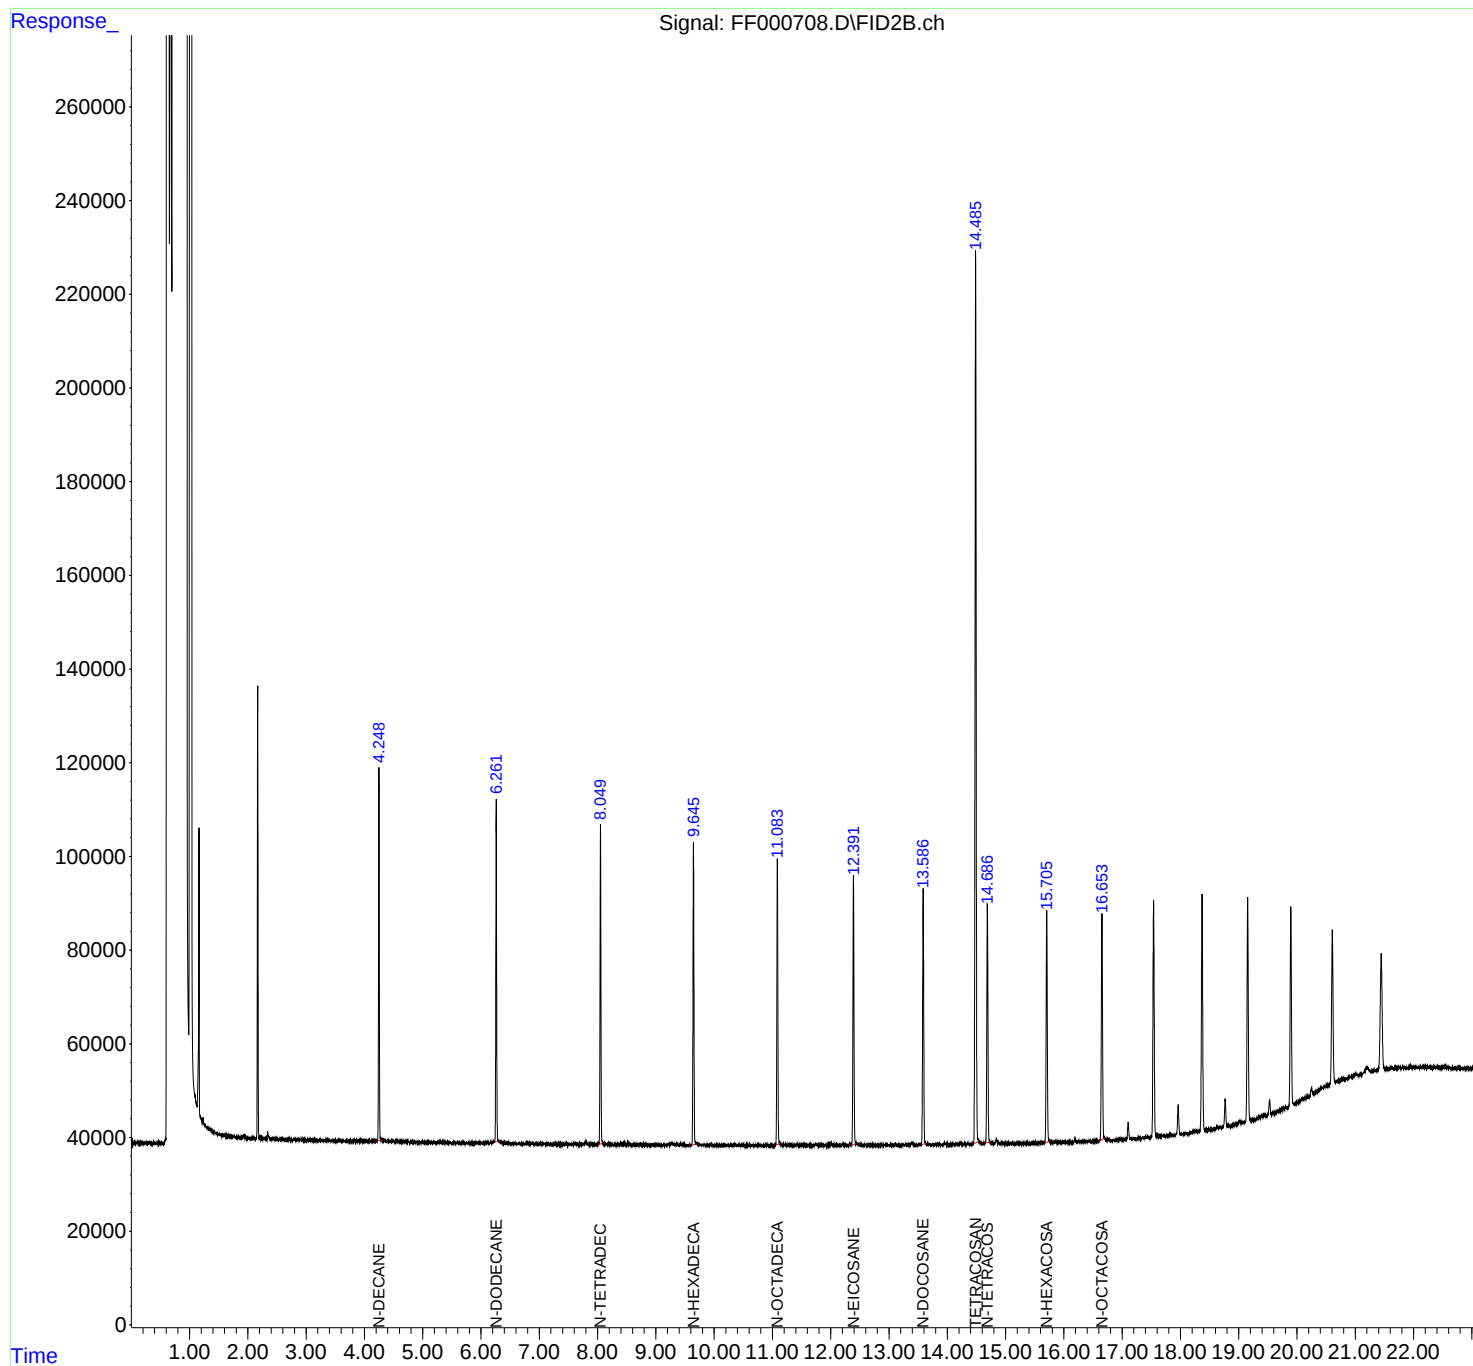


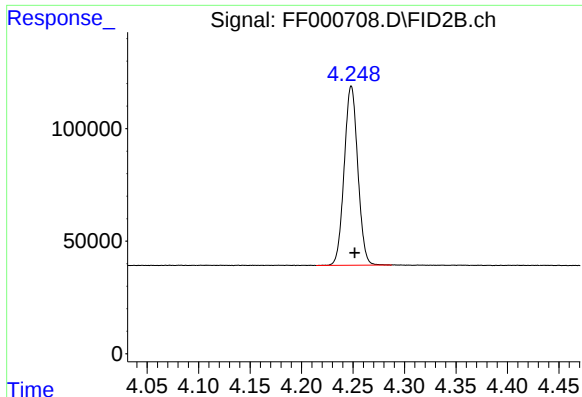

#2 N-DECANE


R.T.: 4.248 min
Delta R.T.: -0.003 min
Response: 730941
Conc: 5.22 ug/ml

Instrument :
FID_F
ClientSampleId :

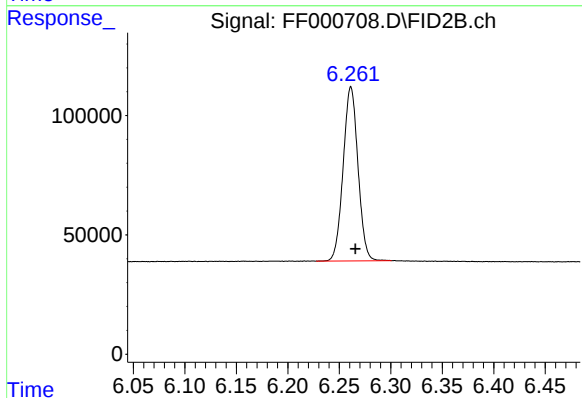


#3 N-DODECANE

R.T.: 6.261 min
Delta R.T.: -0.004 min
Response: 731070
Conc: 5.22 ug/ml

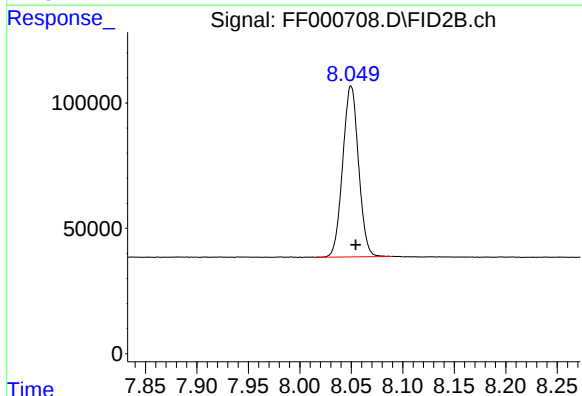


#4 N-TETRADECANE

R.T.: 8.050 min
Delta R.T.: -0.004 min
Response: 730279
Conc: 5.25 ug/ml

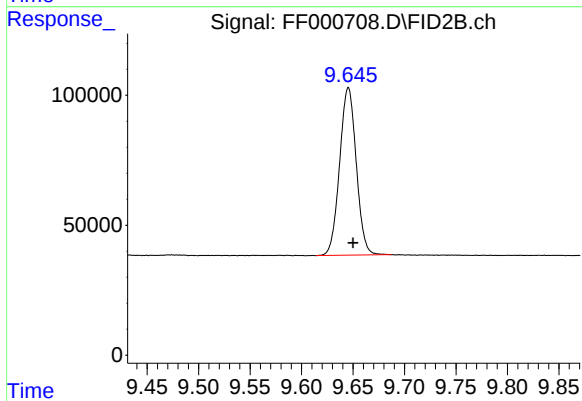

#5 N-HEXADECANE


R.T.: 9.646 min
Delta R.T.: -0.005 min
Response: 725066
Conc: 5.26 ug/ml

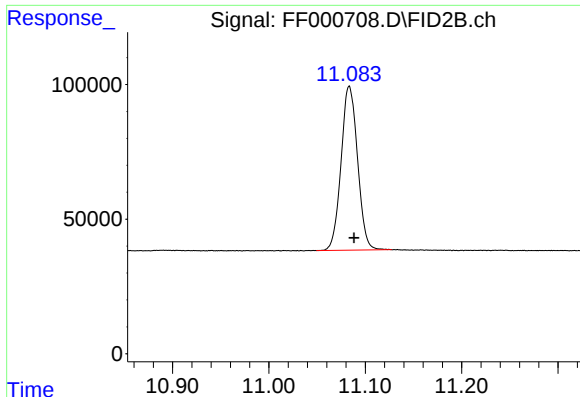

#6 N-OCTADECANE


R.T.: 11.083 min
Delta R.T.: -0.005 min
Response: 720694
Conc: 5.28 ug/ml

Instrument :
FID_F
ClientSampleId :

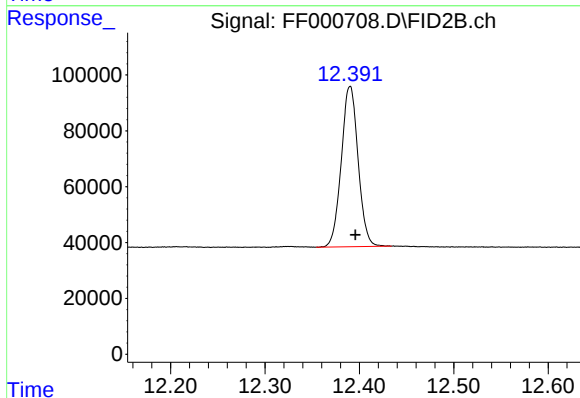


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: -0.006 min
Response: 710105
Conc: 5.30 ug/ml

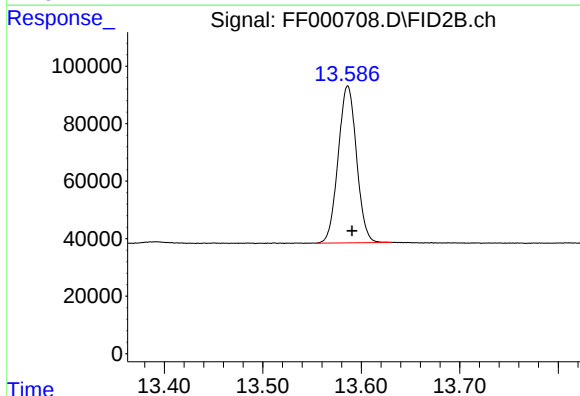


#8 N-DOCOSANE

R.T.: 13.586 min
Delta R.T.: -0.004 min
Response: 706914
Conc: 5.35 ug/ml

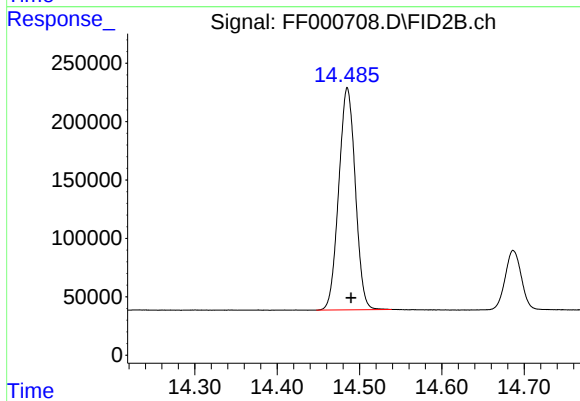

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.485 min
Delta R.T.: -0.005 min
Response: 2656968
Conc: 23.04 ug/ml

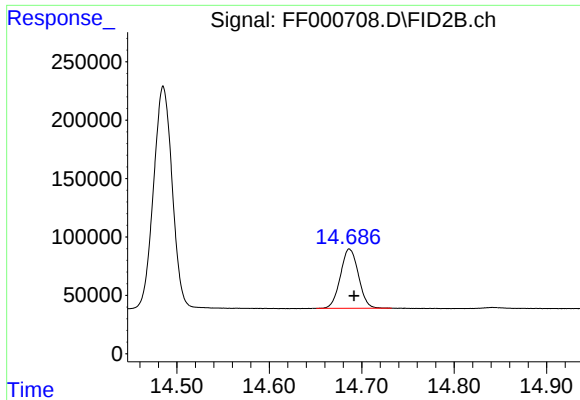

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 686595
Conc: 5.29 ug/ml

Instrument :
FID_F
ClientSampleId :

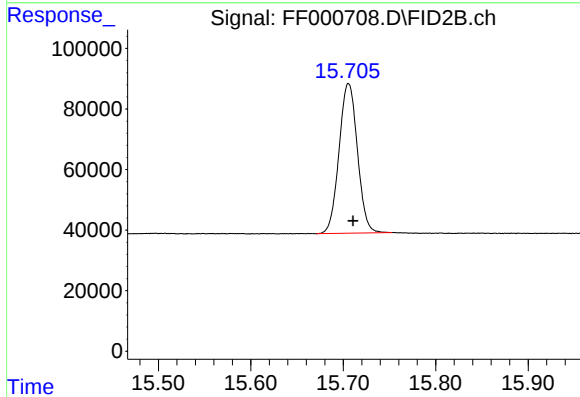

#11 N-HEXACOSANE

R.T.: 15.706 min
Delta R.T.: -0.005 min
Response: 683669
Conc: 5.32 ug/ml

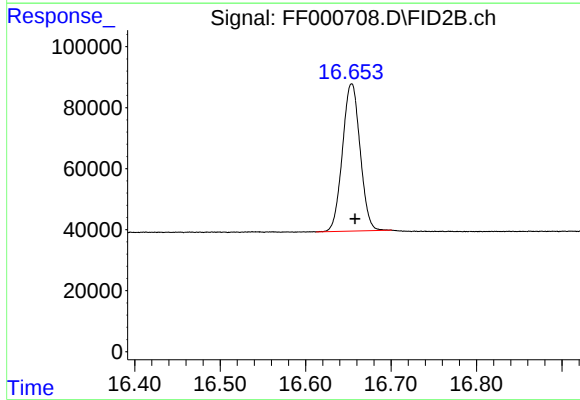

#12 N-OCTACOSANE

R.T.: 16.654 min
Delta R.T.: -0.004 min
Response: 692046
Conc: 5.44 ug/ml