

Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
 Data File : FF000710.D
 Signal(s) : FID2B.ch
 Acq On : 01 Jun 2018 19:38
 Operator : UA\AJ
 Sample : J2923-08
 Misc : Precision Bias study water 04
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 02 05:27:46 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
 Quant Title :
 QLast Update : Fri Jun 01 16:01:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.486	2595132	22.503 ug/ml
Target Compounds			
2) N-DECANE	4.248	717926	5.124 ug/ml
3) N-DODECANE	6.262	717403	5.119 ug/ml
4) N-TETRADECANE	8.050	714673	5.133 ug/ml
5) N-HEXADECANE	9.645	708426	5.138 ug/ml
6) N-OCTADECANE	11.083	704745	5.161 ug/ml
7) N-EICOSANE	12.390	692444	5.168 ug/ml
8) N-DOCOSANE	13.585	687248	5.197 ug/ml
10) N-TETRACOSANE	14.687	669280	5.160 ug/ml
11) N-HEXACOSANE	15.706	665917	5.184 ug/ml
12) N-OCTACOSANE	16.654	660379	5.193 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF060118\
Data File : FF000710.D
Signal(s) : FID2B.ch
Acq On : 01 Jun 2018 19:38
Operator : UA\AJ
Sample : J2923-08
Misc : Precision Bias study water 04
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 02 05:27:46 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF060118.M
Quant Title :
QLast Update : Fri Jun 01 16:01:51 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

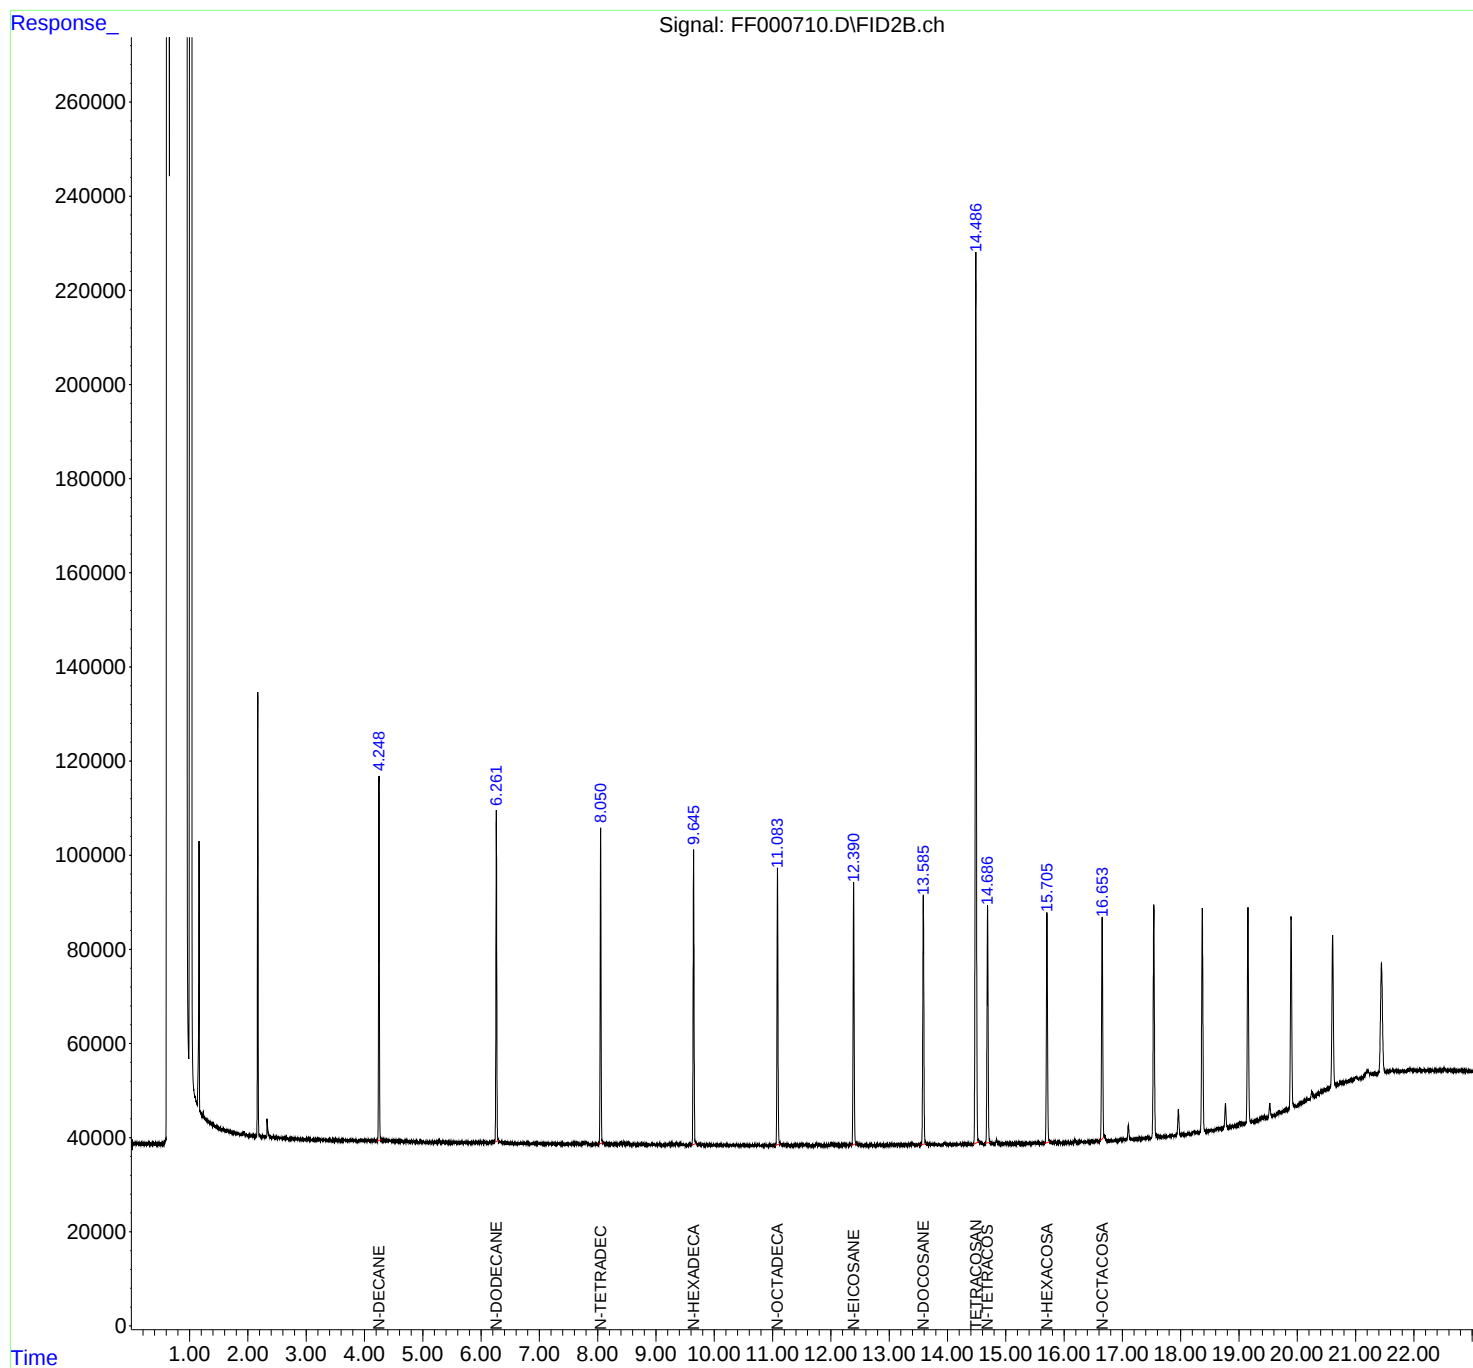


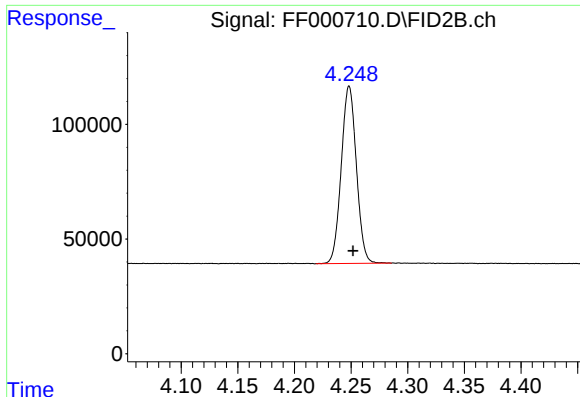

#2 N-DECANE


R.T.: 4.248 min
Delta R.T.: -0.003 min
Response: 717926
Conc: 5.12 ug/ml

Instrument :
FID_F
ClientSampleId :

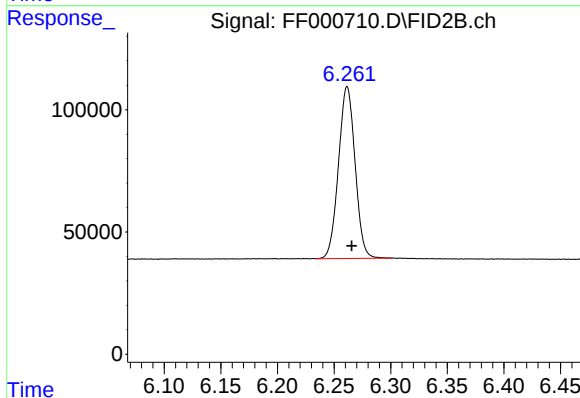


#3 N-DODECANE

R.T.: 6.262 min
Delta R.T.: -0.004 min
Response: 717403
Conc: 5.12 ug/ml

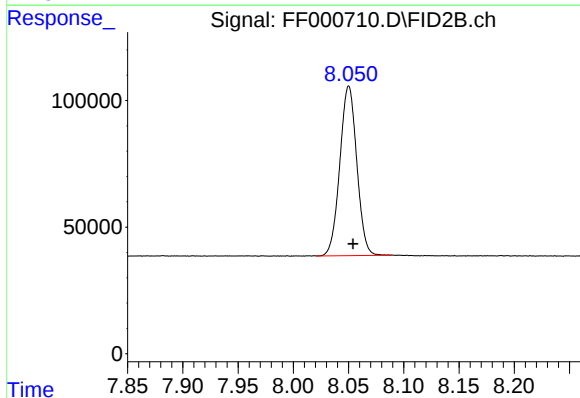


#4 N-TETRADECANE

R.T.: 8.050 min
Delta R.T.: -0.004 min
Response: 714673
Conc: 5.13 ug/ml

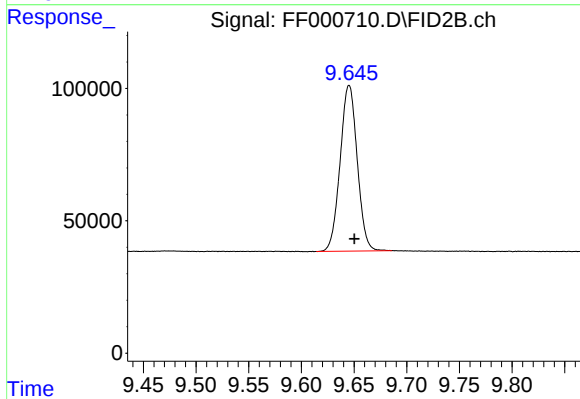

#5 N-HEXADECANE


R.T.: 9.645 min
Delta R.T.: -0.005 min
Response: 708426
Conc: 5.14 ug/ml

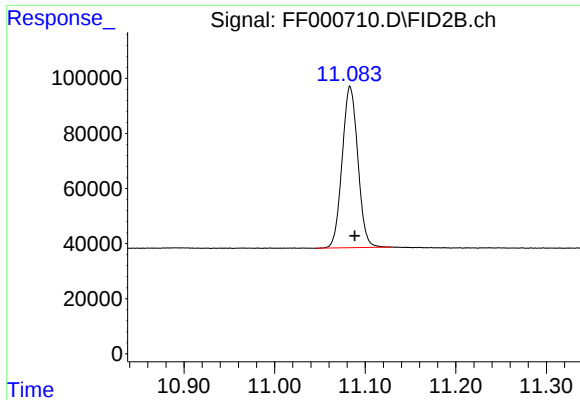

#6 N-OCTADECANE


R.T.: 11.083 min
Delta R.T.: -0.005 min
Response: 704745
Conc: 5.16 ug/ml

Instrument :
FID_F
ClientSampleId :

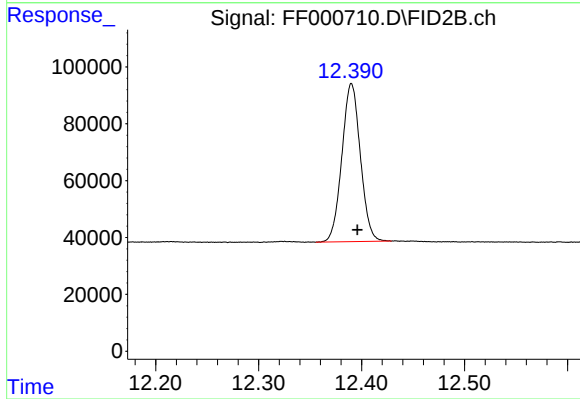


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: -0.006 min
Response: 692444
Conc: 5.17 ug/ml

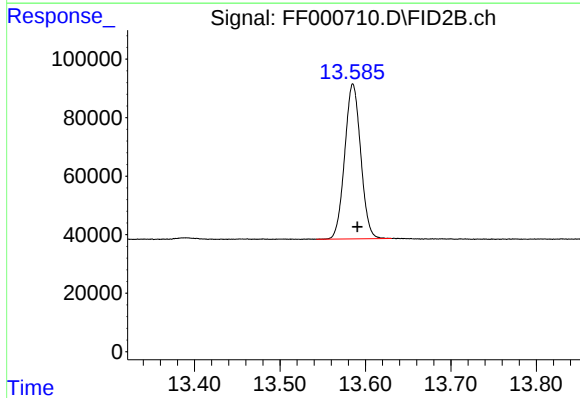


#8 N-DOCOSANE

R.T.: 13.585 min
Delta R.T.: -0.005 min
Response: 687248
Conc: 5.20 ug/ml

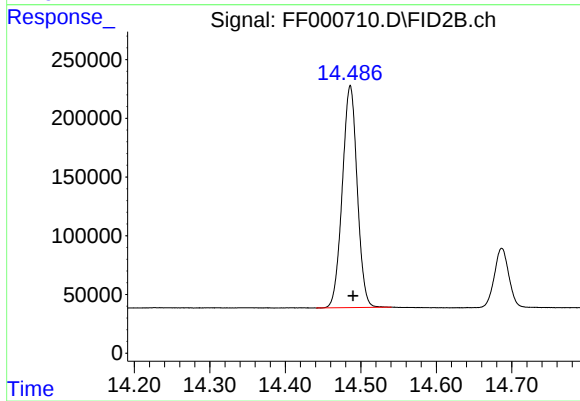

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.486 min
Delta R.T.: -0.004 min
Response: 2595132
Conc: 22.50 ug/ml

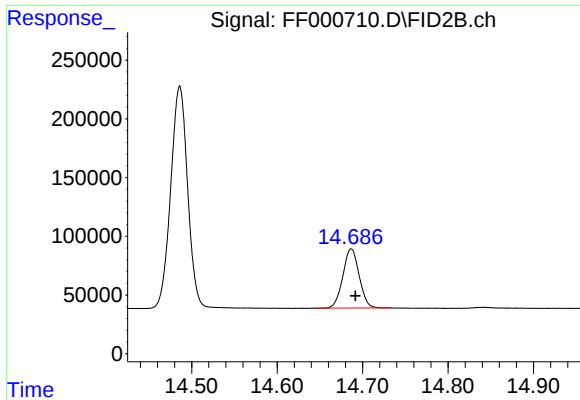

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.005 min
Response: 669280
Conc: 5.16 ug/ml

Instrument :
FID_F
ClientSampleId :

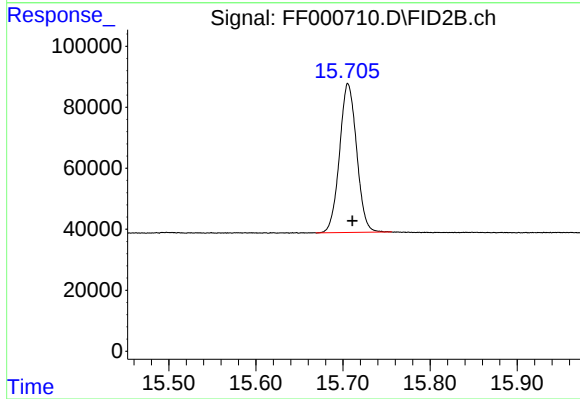

#11 N-HEXACOSANE

R.T.: 15.706 min
Delta R.T.: -0.005 min
Response: 665917
Conc: 5.18 ug/ml

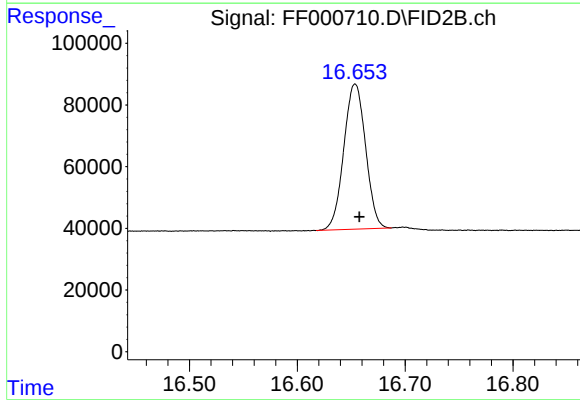

#12 N-OCTACOSANE

R.T.: 16.654 min
Delta R.T.: -0.004 min
Response: 660379
Conc: 5.19 ug/ml