

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060123\  
Data File : FF012801.D  
Signal(s) : FID2B.ch  
Acq On : 01 Jun 2023 10:52  
Operator : YP\AJ  
Sample : 02983-09 5X  
Misc :  
ALS Vial : 62 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 01 17:37:11 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF050523.M  
Quant Title :  
QLast Update : Fri May 05 16:23:08 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.984  | 340914   | 2.824 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 12.968f | 892256   | 6.445 ug/ml |
| 10) N-TETRACOSANE             | 15.189  | 581221   | 4.356 ug/ml |
| 12) N-OCTACOSANE              | 17.196  | 206083   | 1.626 ug/ml |
| 14) N-DOTRIACONTANE           | 18.873  | 271675   | 2.274 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF060123\  
Data File : FF012801.D  
Signal(s) : FID2B.ch  
Acq On : 01 Jun 2023 10:52  
Operator : YP\AJ  
Sample : 02983-09 5X  
Misc :  
ALS Vial : 62 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 01 17:37:11 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF050523.M  
Quant Title :  
QLast Update : Fri May 05 16:23:08 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

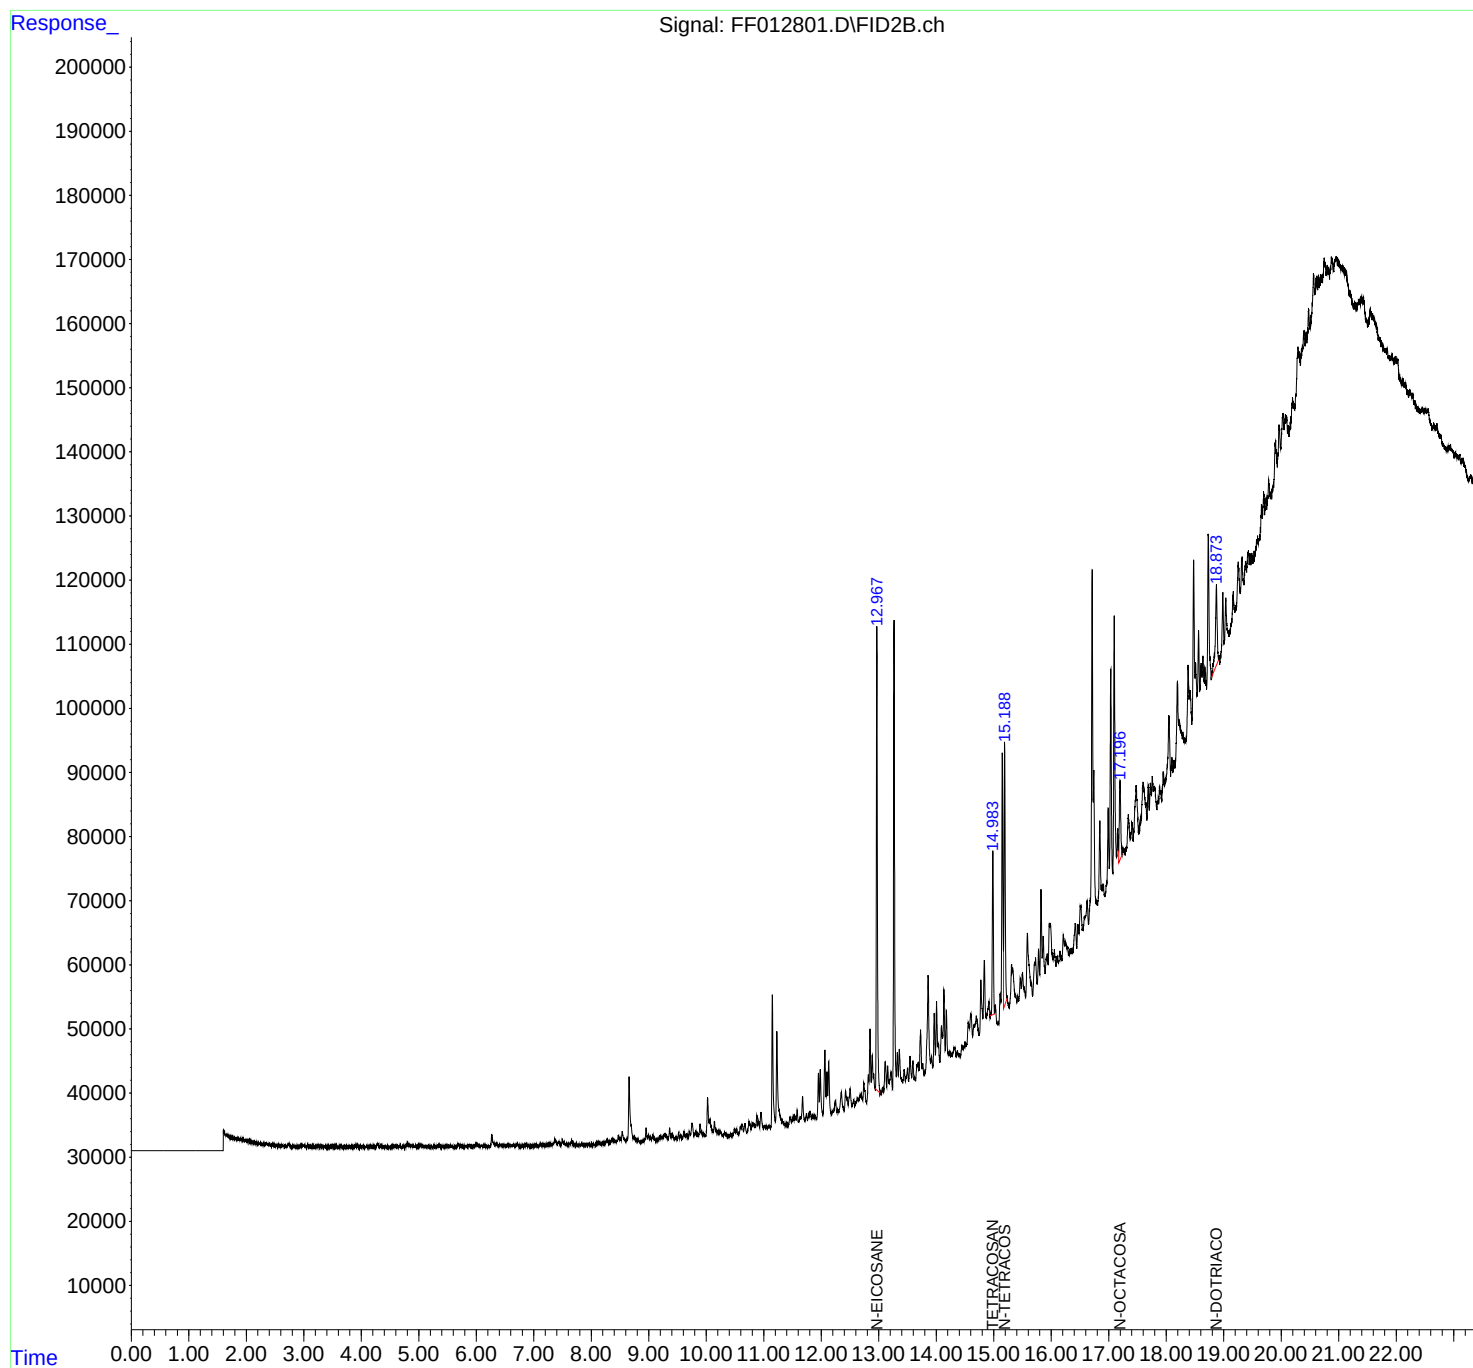


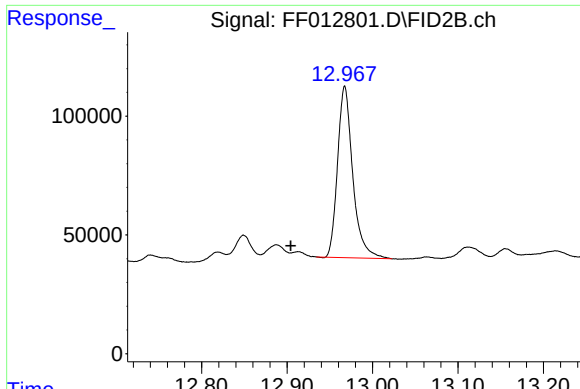

#7 N-EICOSANE


R.T.: 12.968 min  
Delta R.T.: 0.063 min  
Response: 892256  
Conc: 6.45 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

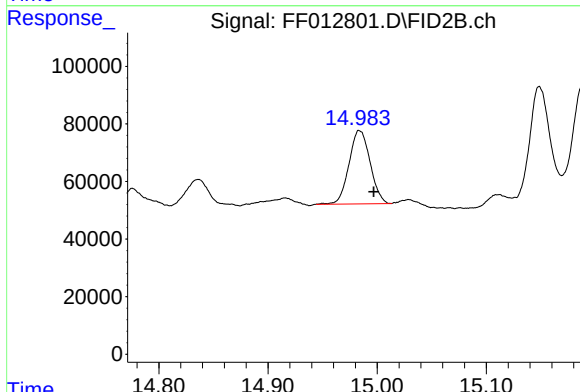


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.984 min  
Delta R.T.: -0.013 min  
Response: 340914  
Conc: 2.82 ug/ml

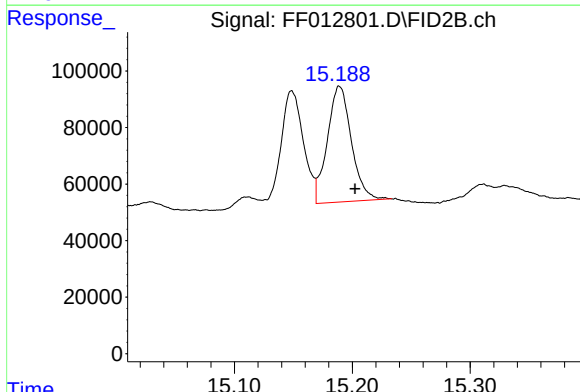


#10 N-TETRACOSANE

R.T.: 15.189 min  
Delta R.T.: -0.013 min  
Response: 581221  
Conc: 4.36 ug/ml

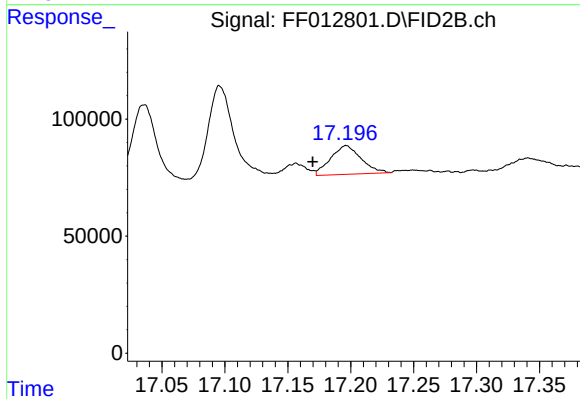

#12 N-OCTACOSANE

R.T.: 17.196 min  
Delta R.T.: 0.027 min  
Response: 206083  
Conc: 1.63 ug/ml

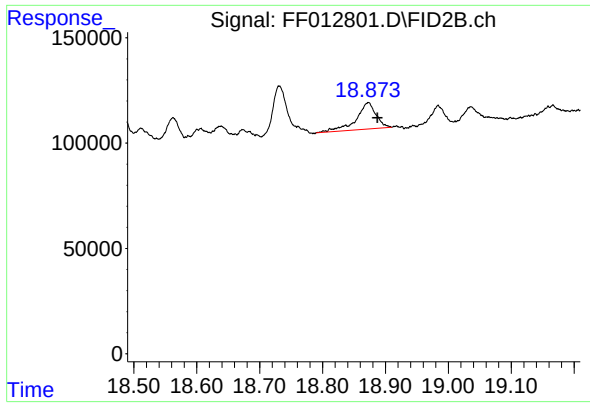

#14 N-DOTRIACONTANE

R.T.: 18.873 min  
Delta R.T.: -0.014 min  
Response: 271675  
Conc: 2.27 ug/ml

Instrument :  
FID\_F  
ClientSampleId :