

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060319\
 Data File : FF004704.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2019 20:54
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jun 04 09:29:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	7992166	65.450 ug/ml
Target Compounds			
2) N-DECANE	4.426	10353652	70.707 ug/ml
3) N-DODECANE	6.449	10104973	68.285 ug/ml
4) N-TETRADECANE	8.246	9778006	66.567 ug/ml
5) N-HEXADECANE	9.850	9610604	65.092 ug/ml
6) N-OCTADECANE	11.296	9320984	64.202 ug/ml
7) N-EICOSANE	12.611	9256045	63.911 ug/ml
8) N-DOCOSANE	13.814	9115480	64.509 ug/ml
10) N-TETRACOSANE	14.922	9109313	65.730 ug/ml
11) N-HEXACOSANE	15.947	9164793	67.263 ug/ml
12) N-OCTACOSANE	16.902	9357681	68.827 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060319\
Data File : FF004704.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2019 20:54
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jun 04 09:29:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

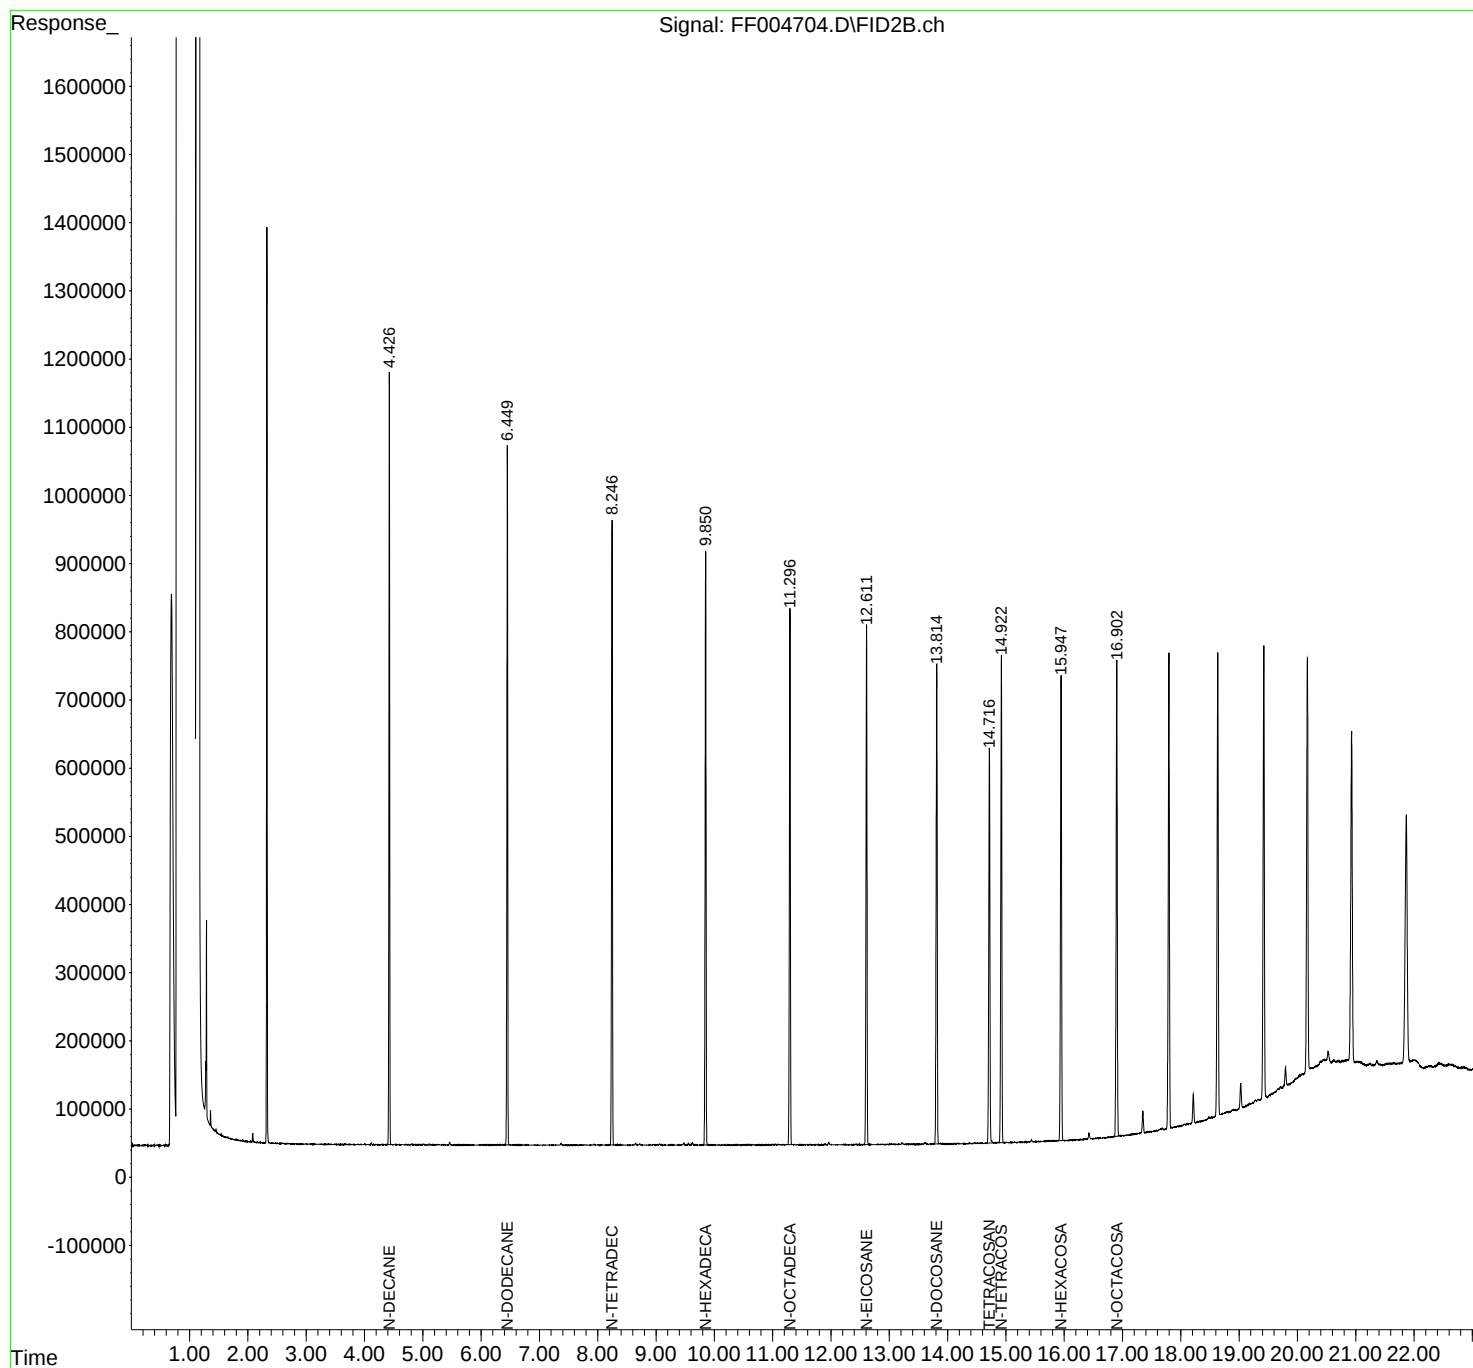

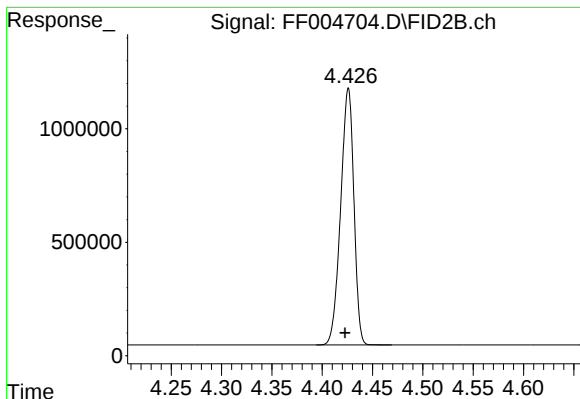


#2 N-DECANE

R.T.: 4.426 min
Delta R.T.: 0.003 min
Response: 10353652
Conc: 70.71 ug/ml

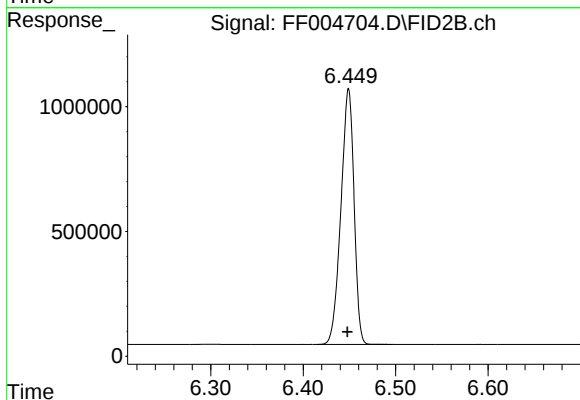


#3 N-DODECANE

R.T.: 6.449 min
Delta R.T.: 0.001 min
Response: 10104973
Conc: 68.29 ug/ml

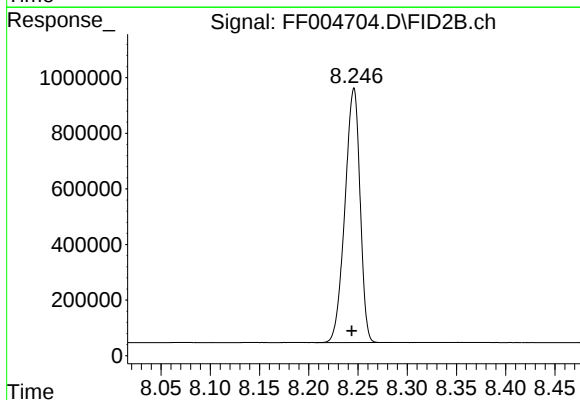


#4 N-TETRADECANE

R.T.: 8.246 min
Delta R.T.: 0.002 min
Response: 9778006
Conc: 66.57 ug/ml

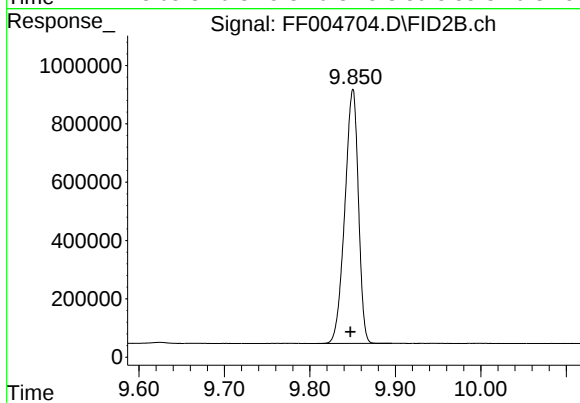


#5 N-HEXADECANE

R.T.: 9.850 min
Delta R.T.: 0.003 min
Response: 9610604
Conc: 65.09 ug/ml

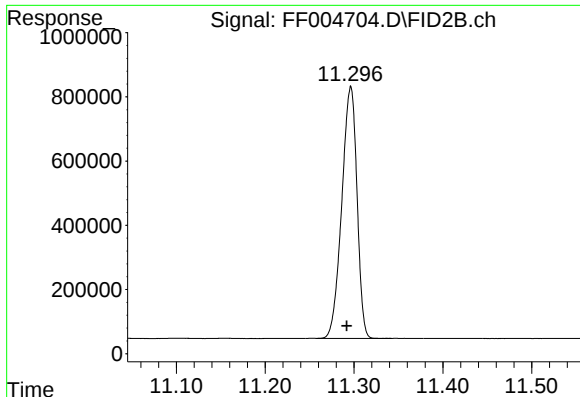


#6 N-OCTADECANE

R.T.: 11.296 min
Delta R.T.: 0.005 min
Response: 9320984
Conc: 64.20 ug/ml

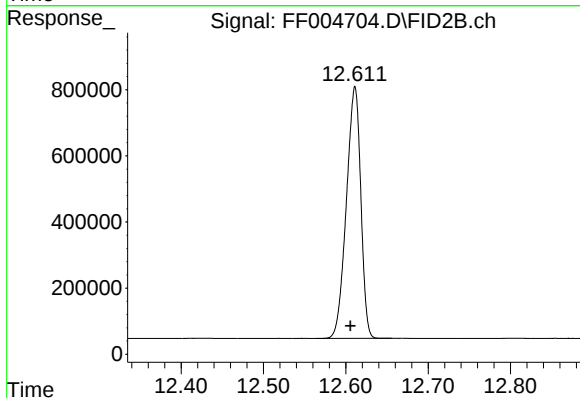


#7 N-EICOSANE

R.T.: 12.611 min
Delta R.T.: 0.005 min
Response: 9256045
Conc: 63.91 ug/ml

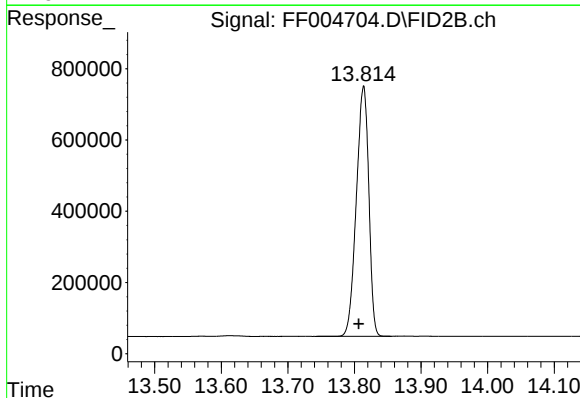


#8 N-DOCOSANE

R.T.: 13.814 min
Delta R.T.: 0.007 min
Response: 9115480
Conc: 64.51 ug/ml

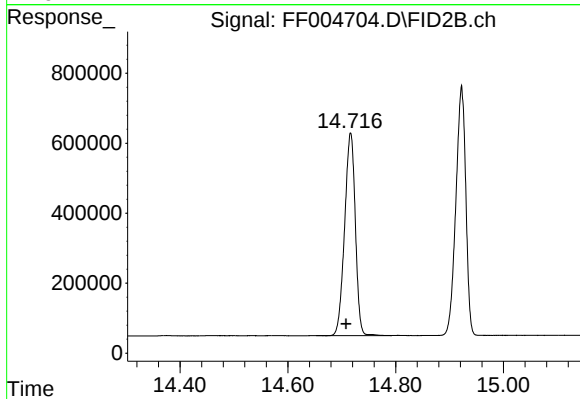


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.717 min
Delta R.T.: 0.008 min
Response: 7992166
Conc: 65.45 ug/ml

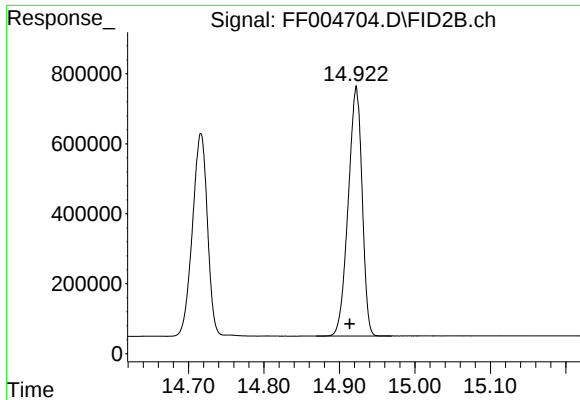


#10 N-TETRACOSANE

R.T.: 14.922 min
Delta R.T.: 0.009 min
Response: 9109313
Conc: 65.73 ug/ml

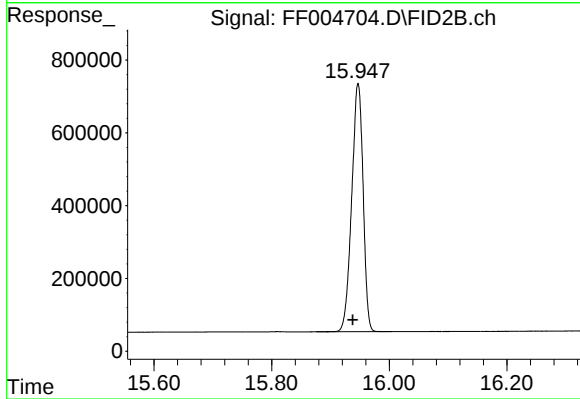

#11 N-HEXACOSANE

R.T.: 15.947 min
Delta R.T.: 0.009 min
Response: 9164793
Conc: 67.26 ug/ml

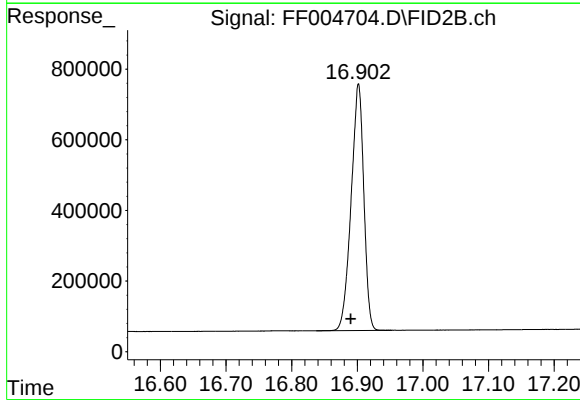

#12 N-OCTACOSANE

R.T.: 16.902 min
Delta R.T.: 0.012 min
Response: 9357681
Conc: 68.83 ug/ml