

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
 Data File : FF008462.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2021 08:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 02:54:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.770	1993227	15.964 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.671	181830	1.342 ug/ml
16) N-HEXATRIACONTANE	20.209	499645	4.186 ug/ml
18) N-TETRACONTANE	21.892	813199	7.153 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008462.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 08:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:54:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

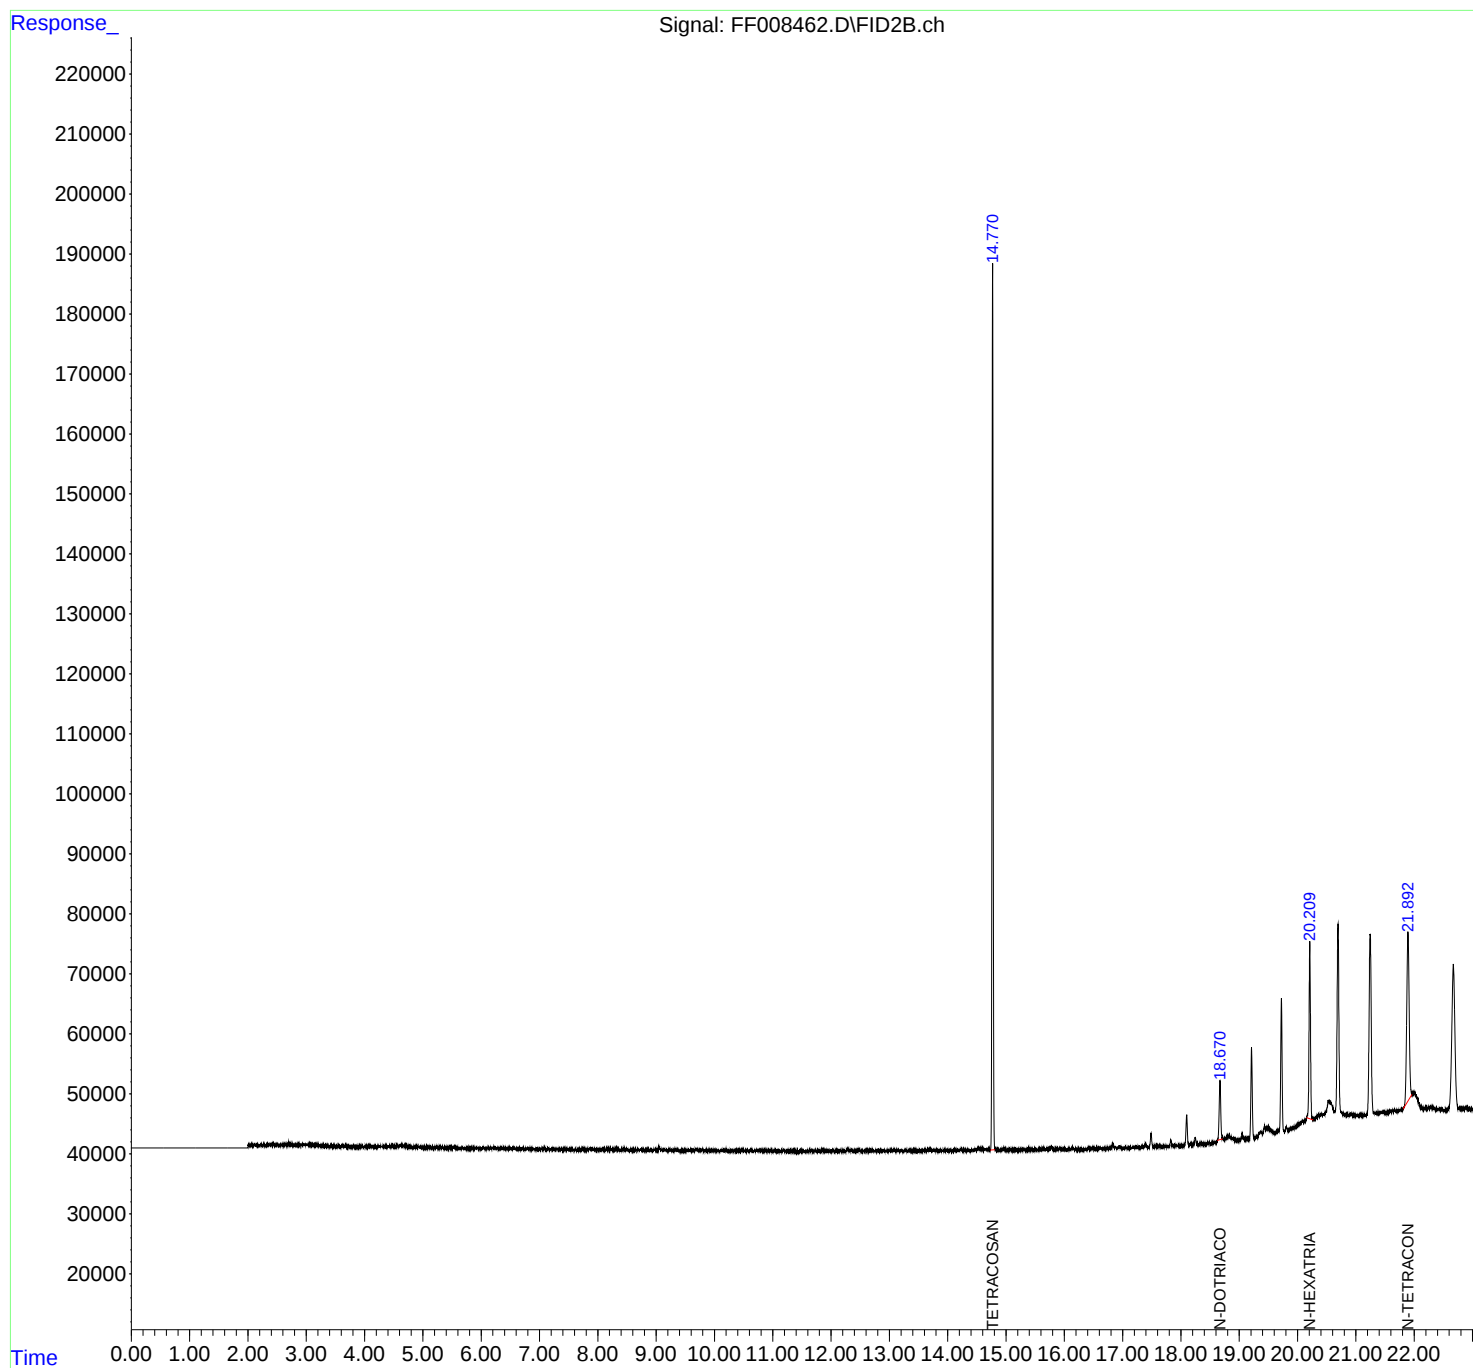


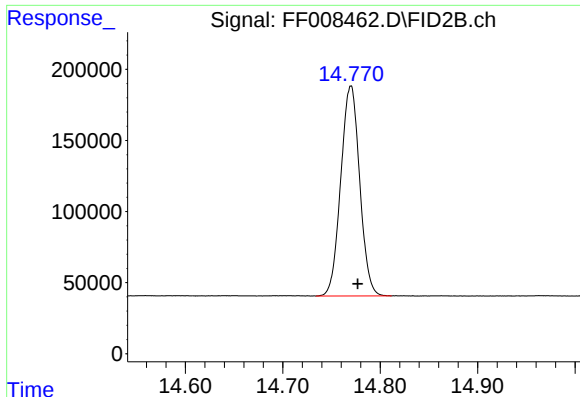

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.770 min
Delta R.T.: -0.007 min
Response: 1993227
Conc: 15.96 ug/ml

Instrument :
FID_F
ClientSampleId :

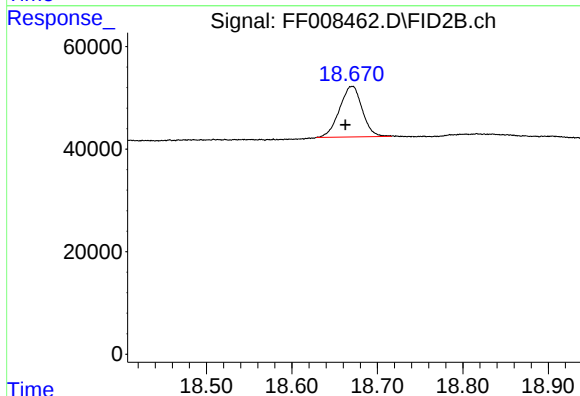


#14 N-DOTRIACONTANE

R.T.: 18.671 min
Delta R.T.: 0.008 min
Response: 181830
Conc: 1.34 ug/ml

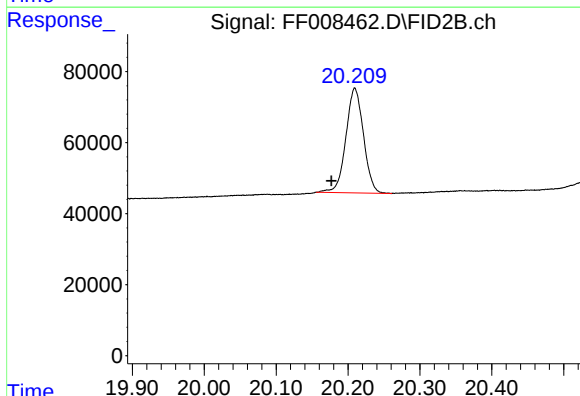

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.032 min
Response: 499645
Conc: 4.19 ug/ml

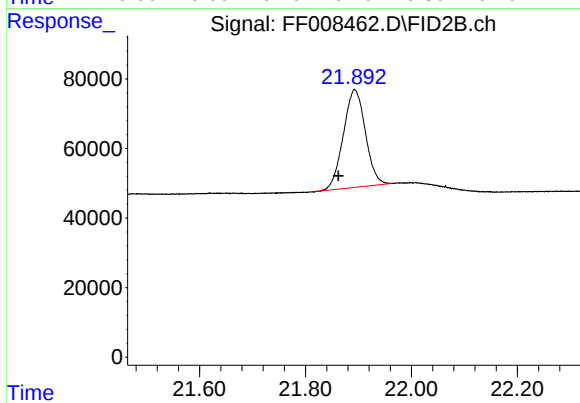

#18 N-TETRACONTANE

R.T.: 21.892 min
Delta R.T.: 0.030 min
Response: 813199
Conc: 7.15 ug/ml