

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
 Data File : FF008464.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2021 09:46
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 02:54:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.545	4858086	35.533	ug/ml
12) N-OCTACOSANE	16.945	4178484	29.779	ug/ml
13) N-TRIACONTANE	17.824	324201	2.340	ug/ml
14) N-DOTRIACONTANE	18.656	449424	3.317	ug/ml
15) N-TETRATRIACONTANE	19.435	298019	2.337	ug/ml
16) N-HEXATRIACONTANE	20.171	213286	1.787	ug/ml
17) N-OCTATRIACONTANE	20.918	156019	1.449	ug/ml
18) N-TETRACONTANE	21.859	43548	0.383	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008464.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 09:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:54:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

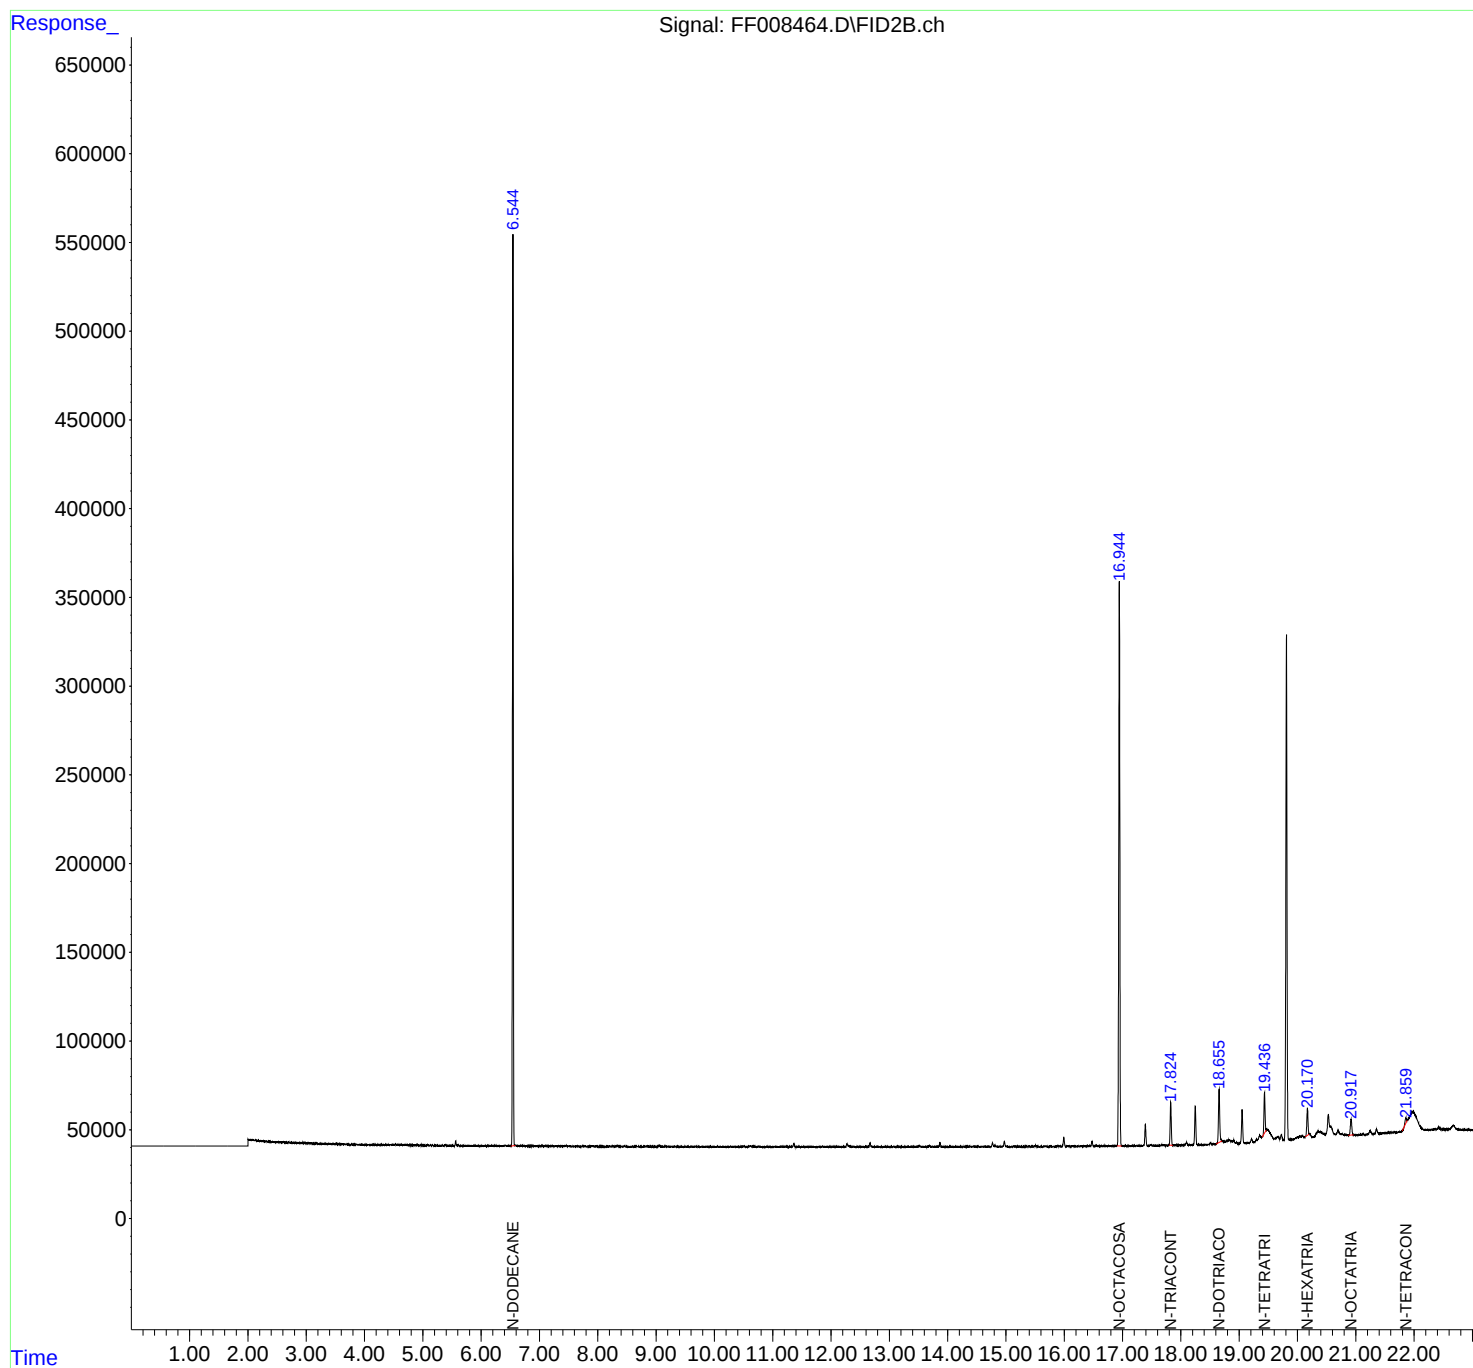


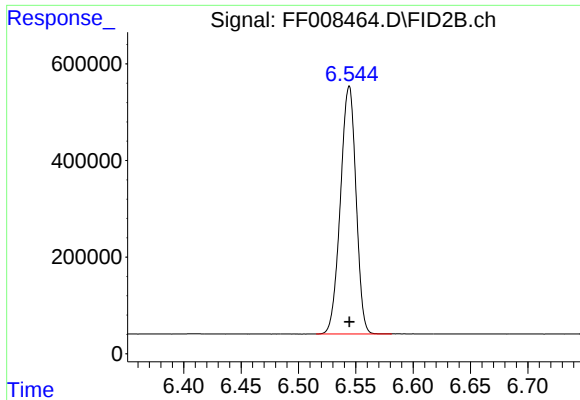

#3 N-DODECANE


R.T.: 6.545 min
Delta R.T.: 0.000 min
Response: 4858086
Conc: 35.53 ug/ml

Instrument :
FID_F
ClientSampleId :

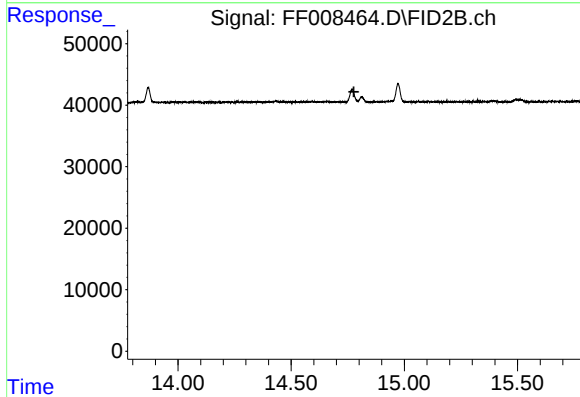


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

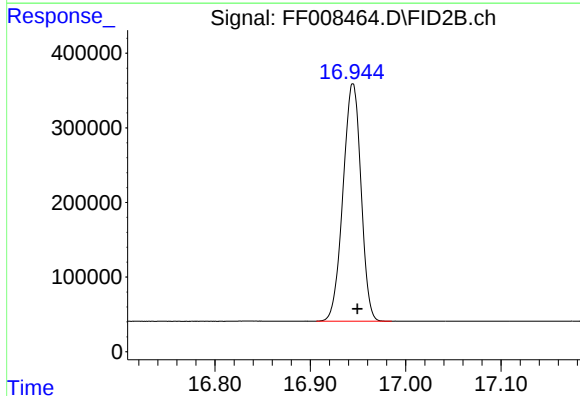


#12 N-OCTACOSANE

R.T.: 16.945 min
Delta R.T.: -0.004 min
Response: 4178484
Conc: 29.78 ug/ml

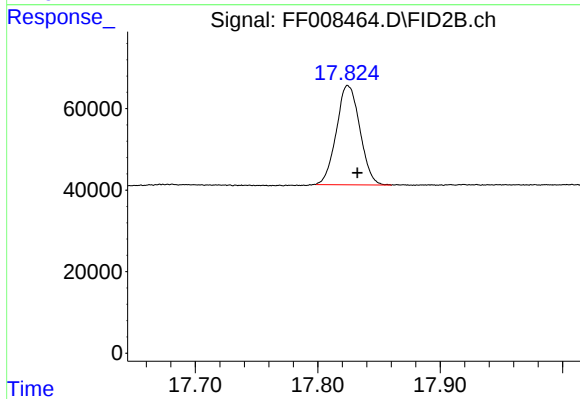

#13 N-TRIACONTANE


R.T.: 17.824 min
Delta R.T.: -0.008 min
Response: 324201
Conc: 2.34 ug/ml

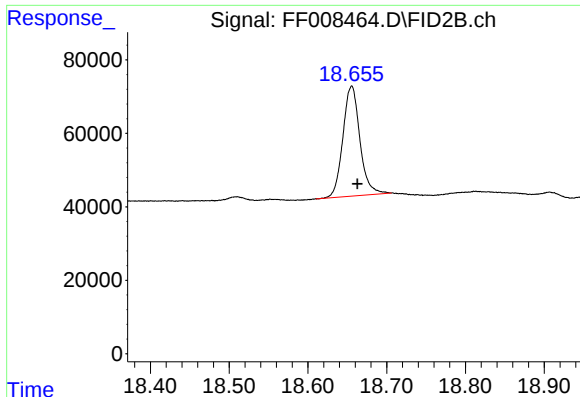

#14 N-DOTRIACONTANE


R.T.: 18.656 min
Delta R.T.: -0.007 min
Response: 449424
Conc: 3.32 ug/ml

Instrument :
FID_F
ClientSampleId :

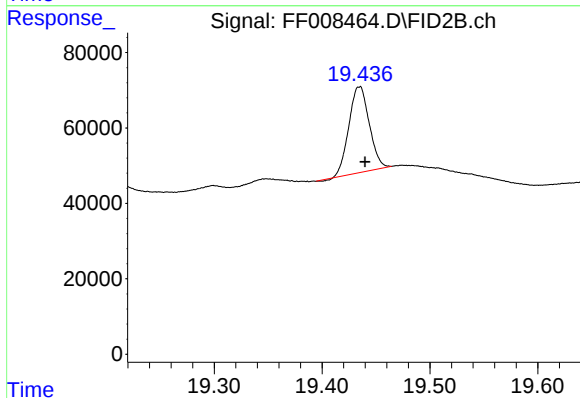


#15 N-TETRATRIACONTANE

R.T.: 19.435 min
Delta R.T.: -0.005 min
Response: 298019
Conc: 2.34 ug/ml

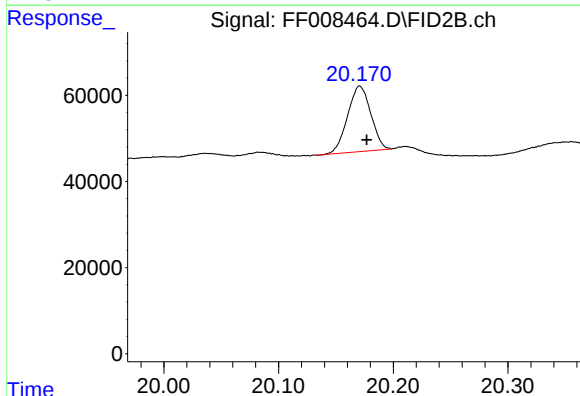


#16 N-HEXATRIACONTANE

R.T.: 20.171 min
Delta R.T.: -0.006 min
Response: 213286
Conc: 1.79 ug/ml

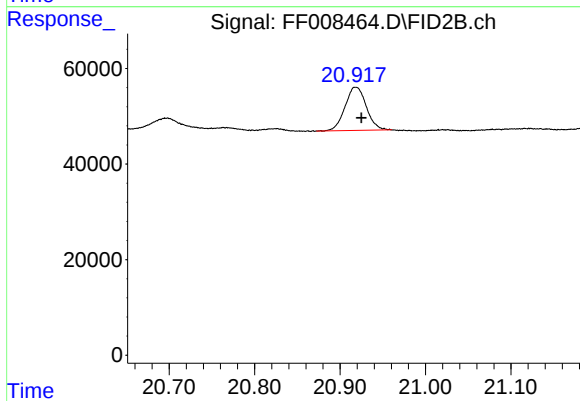

#17 N-OCTATRIACONTANE

R.T.: 20.918 min
Delta R.T.: -0.007 min
Response: 156019
Conc: 1.45 ug/ml

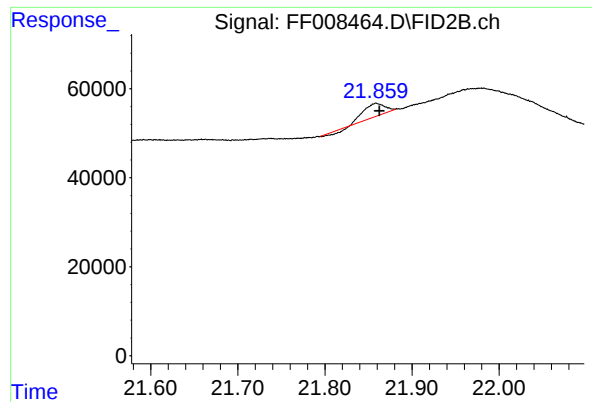

#18 N-TETRACONTANE

R.T.: 21.859 min
Delta R.T.: -0.003 min
Response: 43548
Conc: 0.38 ug/ml

Instrument :
FID_F
ClientSampleId :