

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
 Data File : FF008465.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2021 10:17
 Operator : DD\AJ
 Sample : M2580-10 10X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 02:55:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.771	101220	0.811 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.988	44847	0.320 ug/ml
13) N-TRIACONTANE	17.829	82683	0.597 ug/ml
14) N-DOTRIACONTANE	18.665	49051	0.362 ug/ml
16) N-HEXATRIACONTANE	20.215	11863	0.099 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008465.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 10:17
Operator : DD\AJ
Sample : M2580-10 10X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:55:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

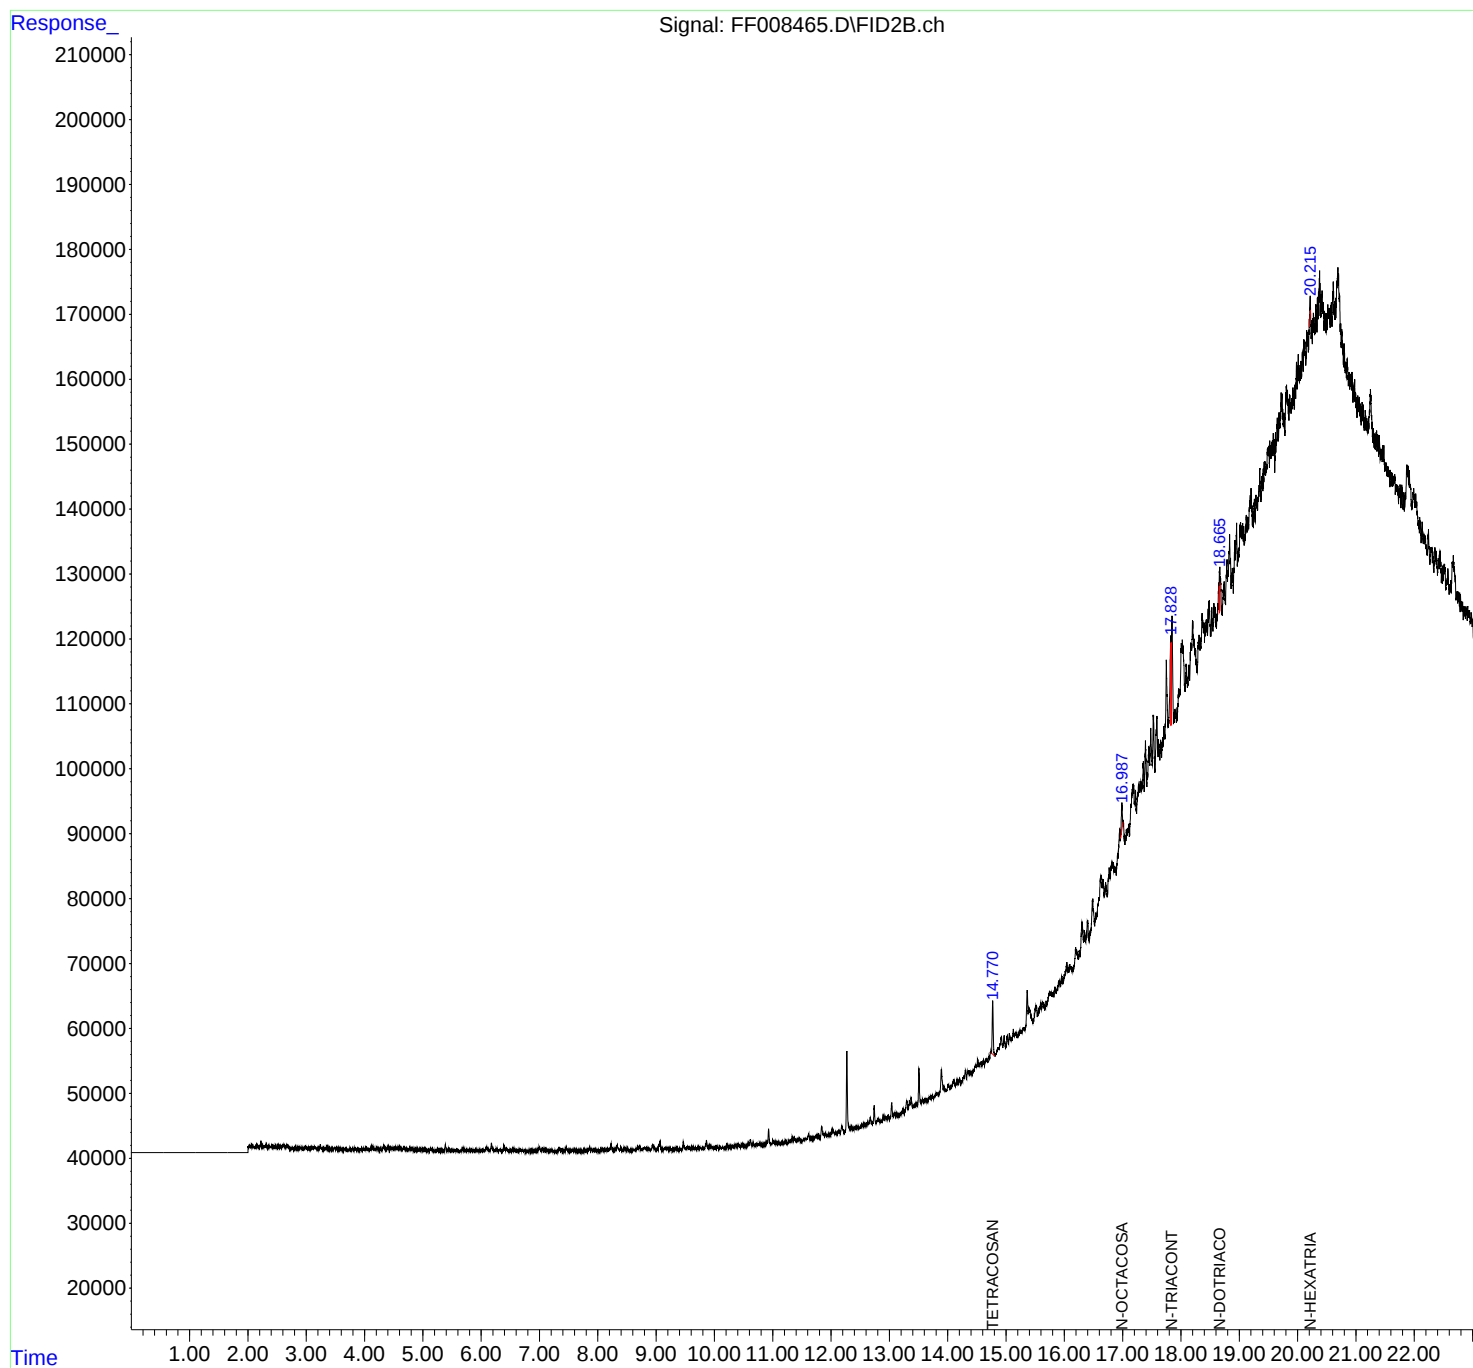


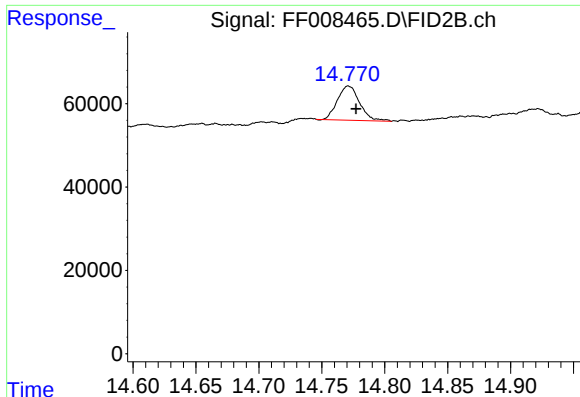

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.771 min
Delta R.T.: -0.006 min
Response: 101220
Conc: 0.81 ug/ml

Instrument :
FID_F
ClientSampleId :

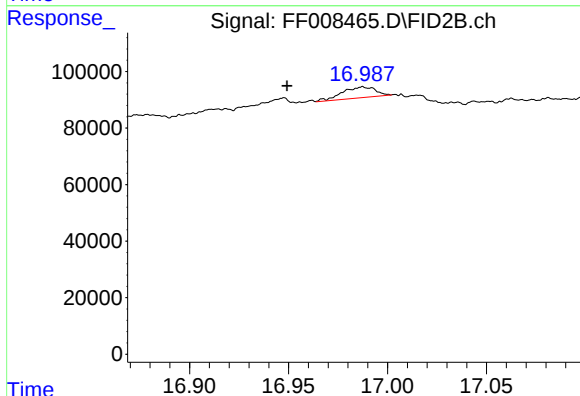


#12 N-OCTACOSANE

R.T.: 16.988 min
Delta R.T.: 0.038 min
Response: 44847
Conc: 0.32 ug/ml

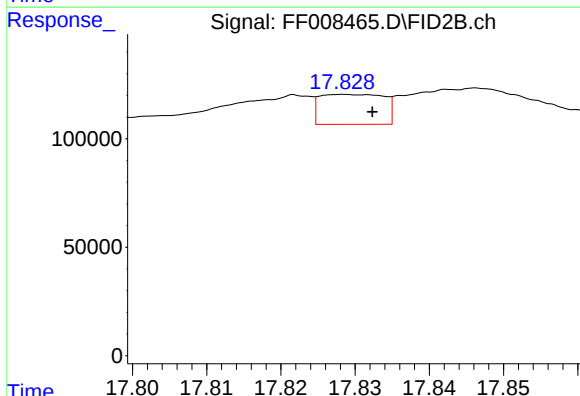


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: -0.004 min
Response: 82683
Conc: 0.60 ug/ml

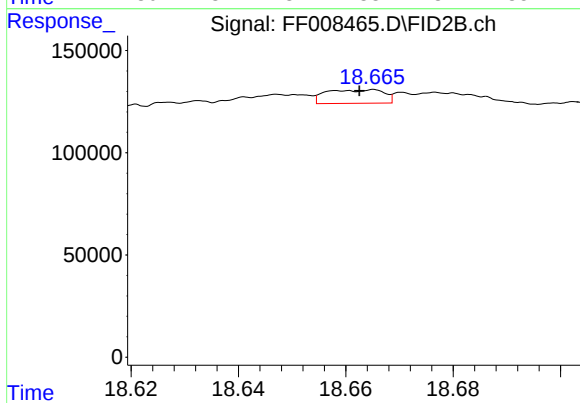

#14 N-DOTRIACONTANE

R.T.: 18.665 min
Delta R.T.: 0.003 min
Response: 49051
Conc: 0.36 ug/ml

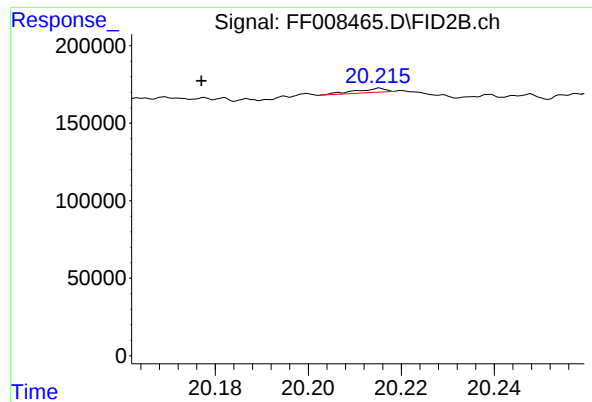

#16 N-HEXATRIACONTANE

R.T.: 20.215 min
Delta R.T.: 0.038 min
Response: 11863
Conc: 0.10 ug/ml

Instrument :
FID_F
ClientSampleId :