

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
 Data File : FF008468.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2021 11:50
 Operator : DD\AJ
 Sample : M2580-01 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 02:55:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.775	438548	3.512 ug/ml
Target Compounds			
4) N-TETRADECANE	8.300	140539	1.006 ug/ml
7) N-EICOSANE	12.672	140553	0.989 ug/ml
10) N-TETRACOSANE	14.971	541223	3.795 ug/ml
11) N-HEXACOSANE	16.000	91636	0.650 ug/ml
12) N-OCTACOSANE	16.952	140555	1.002 ug/ml
13) N-TRIACONTANE	17.832	299783	2.164 ug/ml
14) N-DOTRIACONTANE	18.660	231539	1.709 ug/ml
15) N-TETRATRIACONTANE	19.447	317451	2.490 ug/ml
16) N-HEXATRIACONTANE	20.179	472887	3.962 ug/ml
17) N-OCTATRIACONTANE	20.927	130214	1.209 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008468.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 11:50
Operator : DD\AJ
Sample : M2580-01 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:55:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

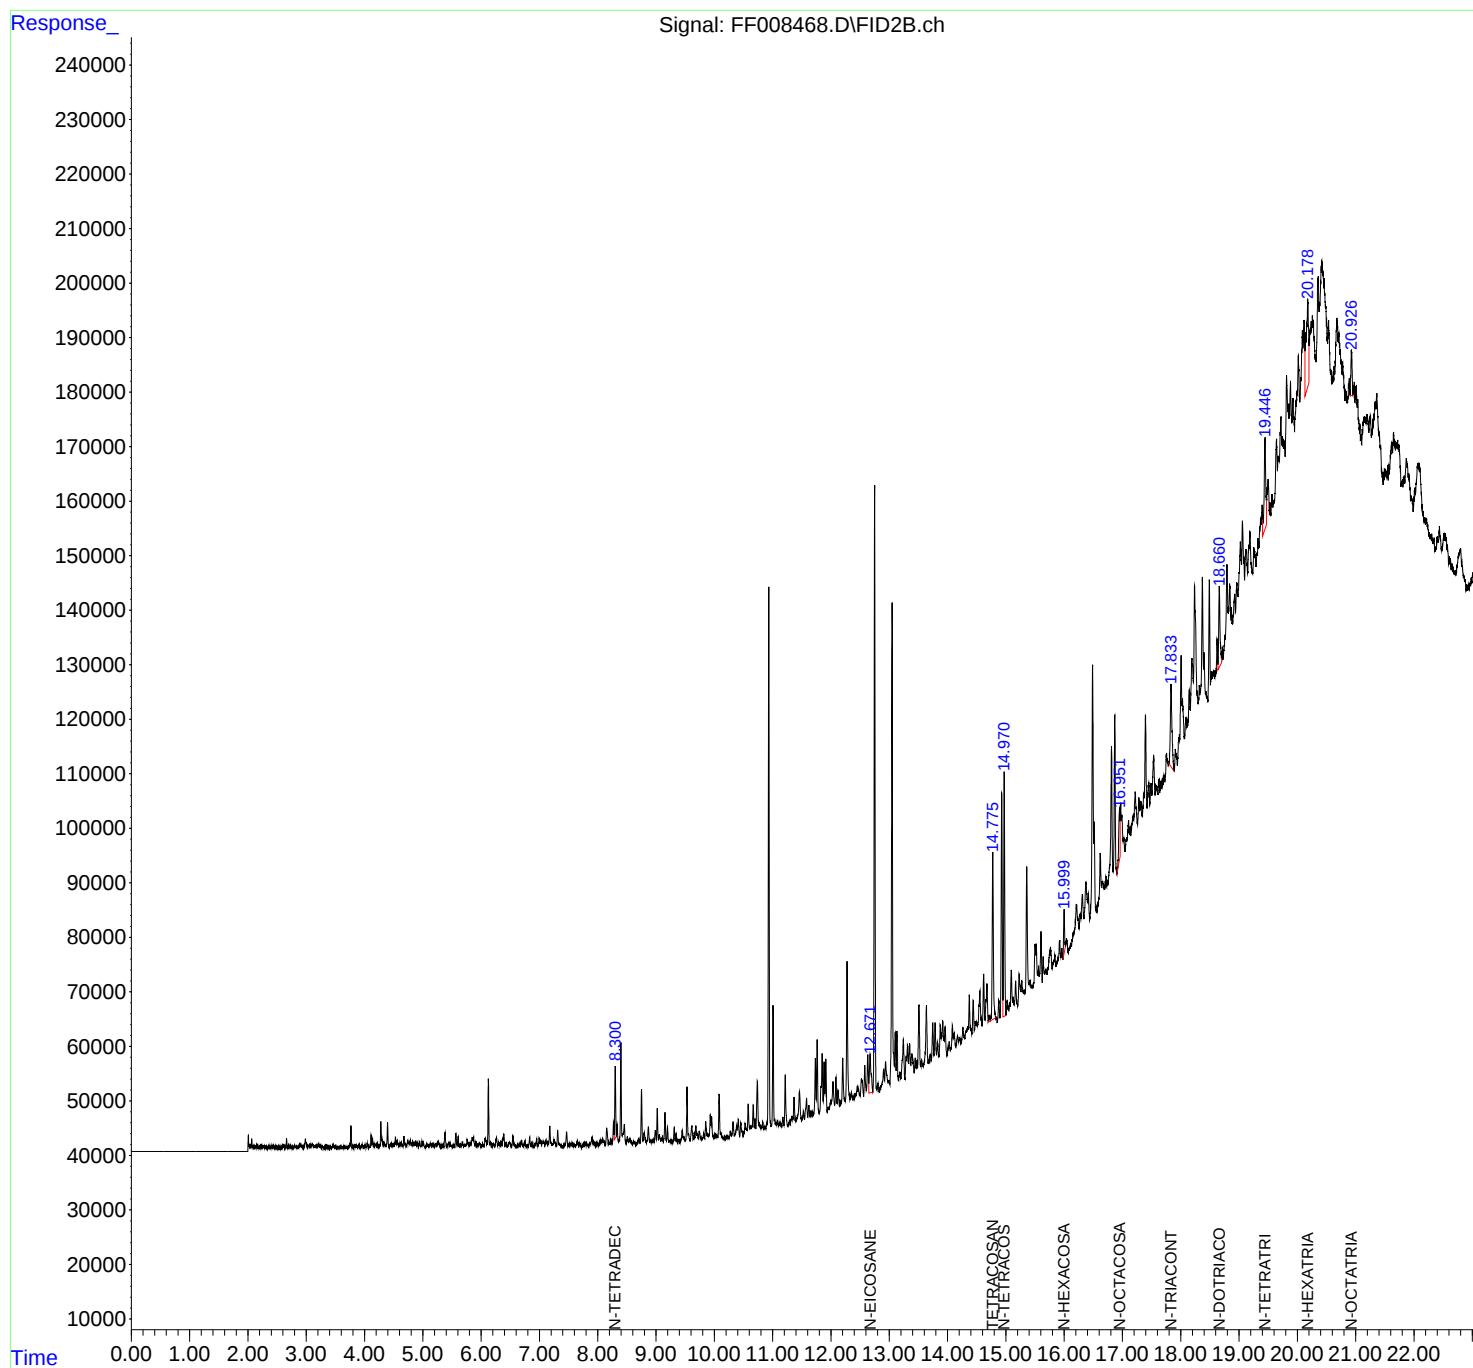


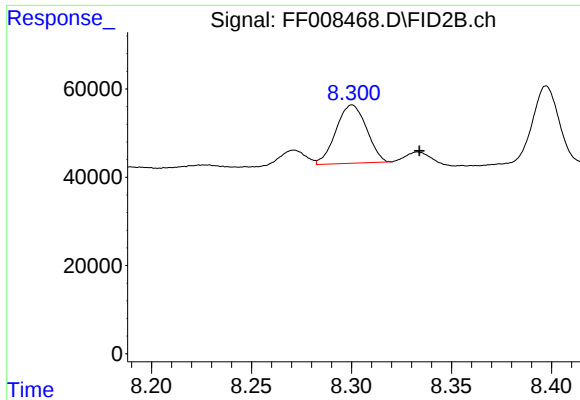

#4 N-TETRADECANE


R.T.: 8.300 min
Delta R.T.: -0.034 min
Response: 140539
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :

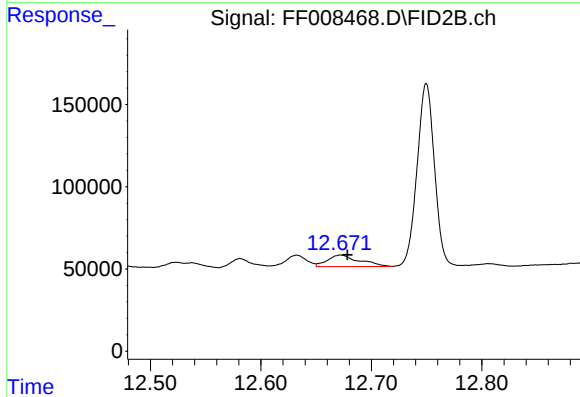


#7 N-EICOSANE

R.T.: 12.672 min
Delta R.T.: -0.006 min
Response: 140553
Conc: 0.99 ug/ml

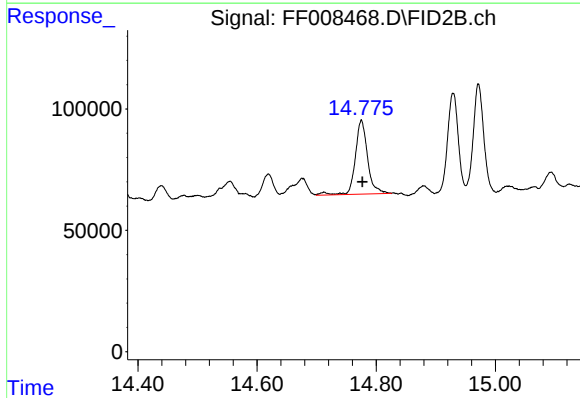


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.775 min
Delta R.T.: -0.002 min
Response: 438548
Conc: 3.51 ug/ml

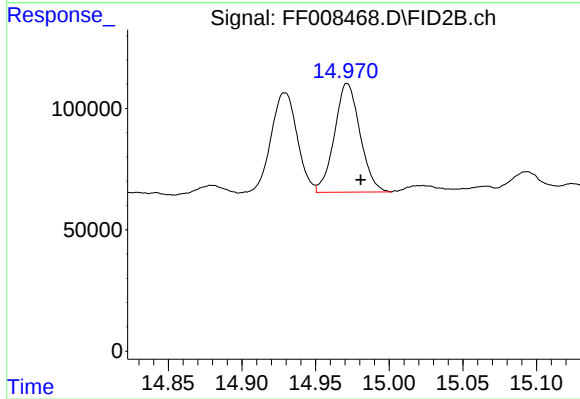

#10 N-TETRACOSANE


R.T.: 14.971 min
Delta R.T.: -0.009 min
Response: 541223
Conc: 3.79 ug/ml

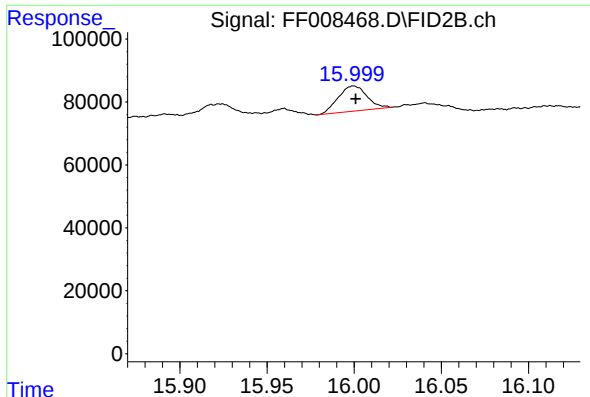

#11 N-HEXACOSANE


R.T.: 16.000 min
Delta R.T.: -0.001 min
Response: 91636
Conc: 0.65 ug/ml

Instrument :
FID_F
ClientSampleId :

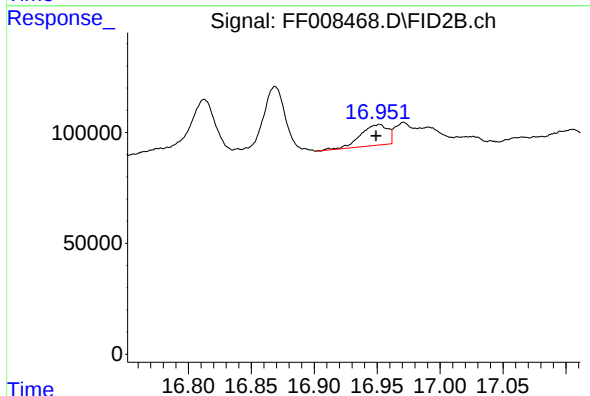


#12 N-OCTACOSANE

R.T.: 16.952 min
Delta R.T.: 0.003 min
Response: 140555
Conc: 1.00 ug/ml

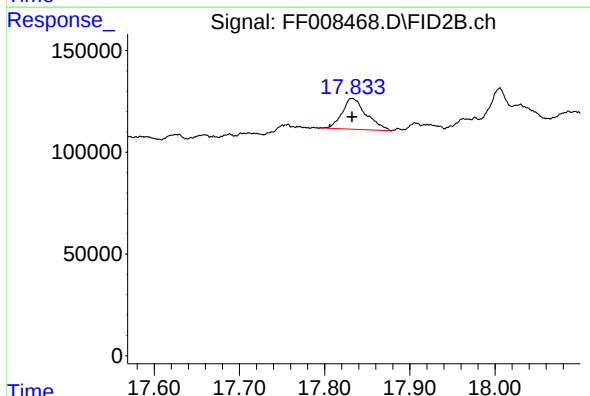


#13 N-TRIACONTANE

R.T.: 17.832 min
Delta R.T.: 0.000 min
Response: 299783
Conc: 2.16 ug/ml

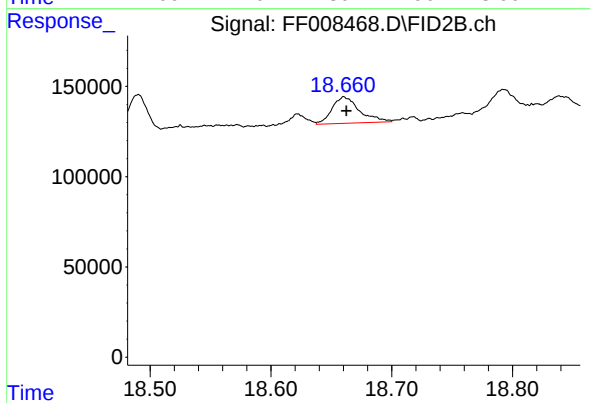

#14 N-DOTRIACONTANE


R.T.: 18.660 min
Delta R.T.: -0.002 min
Response: 231539
Conc: 1.71 ug/ml

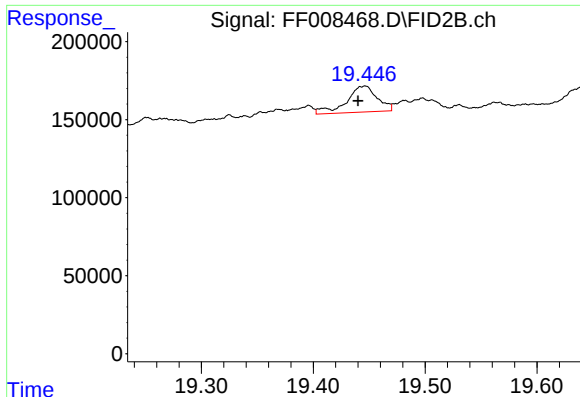

#15 N-TETRATRIACONTANE


R.T.: 19.447 min
Delta R.T.: 0.006 min
Response: 317451
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

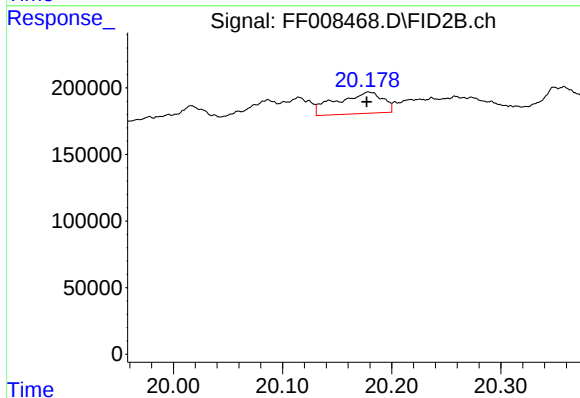

#16 N-HEXATRIACONTANE

R.T.: 20.179 min
Delta R.T.: 0.002 min
Response: 472887
Conc: 3.96 ug/ml

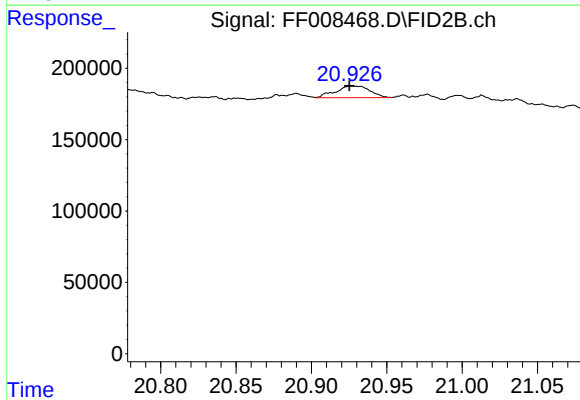

#17 N-OCTATRIACONTANE

R.T.: 20.927 min
Delta R.T.: 0.002 min
Response: 130214
Conc: 1.21 ug/ml