

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
 Data File : FF008469.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2021 12:21
 Operator : DD\AJ
 Sample : M2580-14 5X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 04 02:56:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.773	179203	1.435 ug/ml
Target Compounds			
7) N-EICOSANE	12.748f	614977	4.329 ug/ml
10) N-TETRACOSANE	14.971	370428	2.597 ug/ml
12) N-OCTACOSANE	16.969	117856	0.840 ug/ml
14) N-DOTRIACONTANE	18.663	81430	0.601 ug/ml
15) N-TETRATRIACONTANE	19.445	209961	1.647 ug/ml
16) N-HEXATRIACONTANE	20.189	928944	7.782 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008469.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 12:21
Operator : DD\AJ
Sample : M2580-14 5X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 04 02:56:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

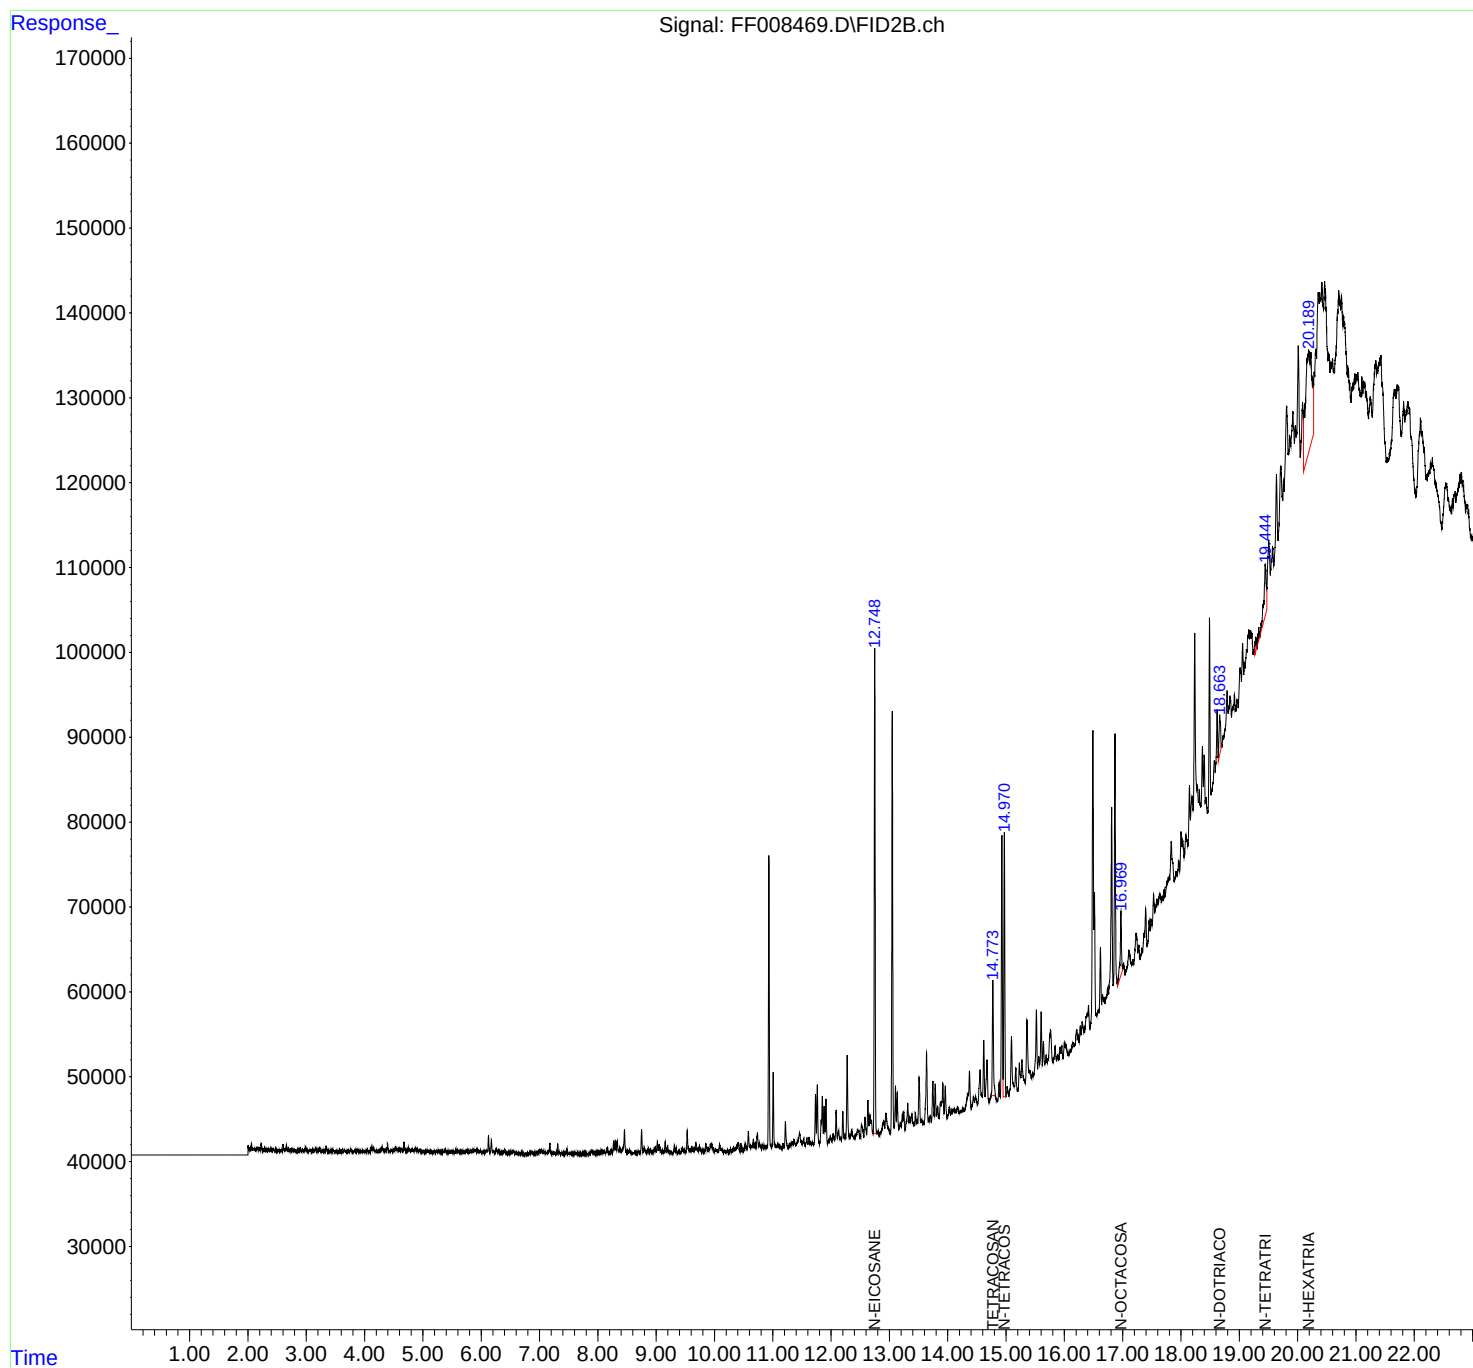


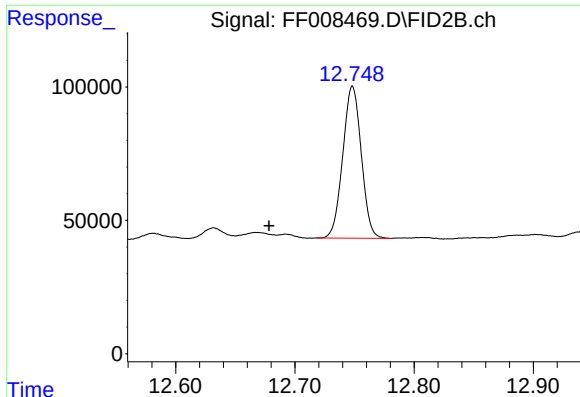

#7 N-EICOSANE


R.T.: 12.748 min
Delta R.T.: 0.070 min
Response: 614977
Conc: 4.33 ug/ml

Instrument :
FID_F
ClientSampleId :

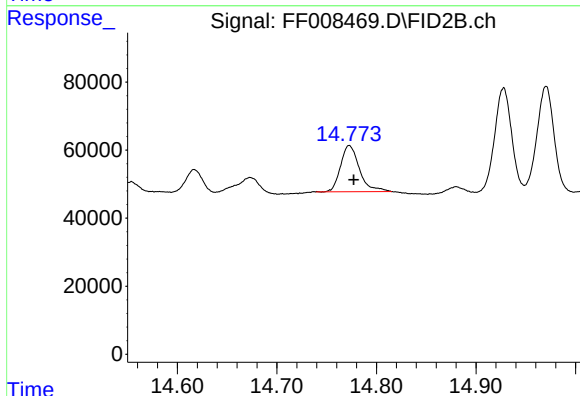


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.773 min
Delta R.T.: -0.004 min
Response: 179203
Conc: 1.44 ug/ml

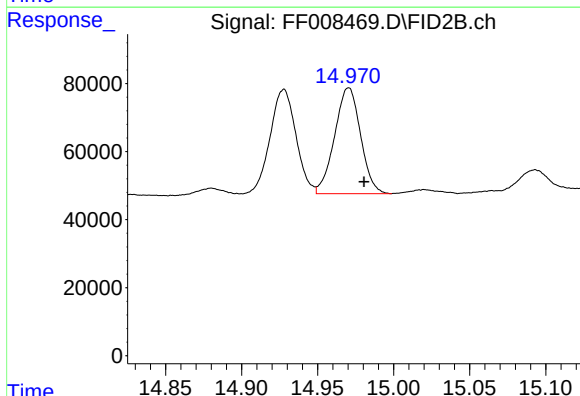


#10 N-TETRACOSANE

R.T.: 14.971 min
Delta R.T.: -0.010 min
Response: 370428
Conc: 2.60 ug/ml

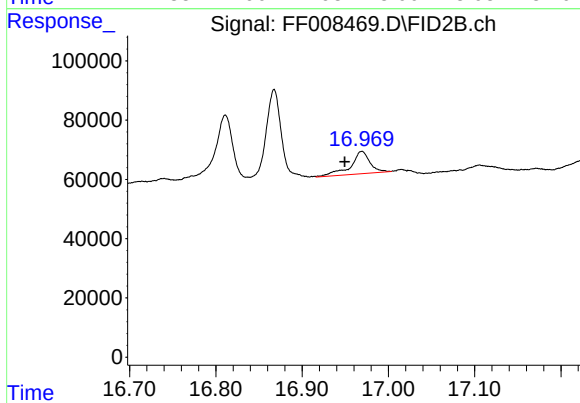

#12 N-OCTACOSANE


R.T.: 16.969 min
Delta R.T.: 0.020 min
Response: 117856
Conc: 0.84 ug/ml

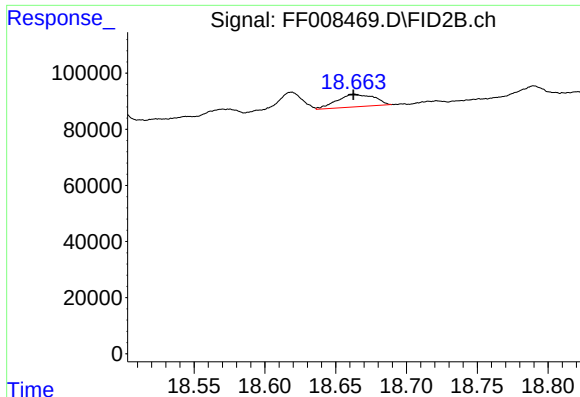

#14 N-DOTRIACONTANE


R.T.: 18.663 min
Delta R.T.: 0.000 min
Response: 81430
Conc: 0.60 ug/ml

Instrument :
FID_F
ClientSampleId :

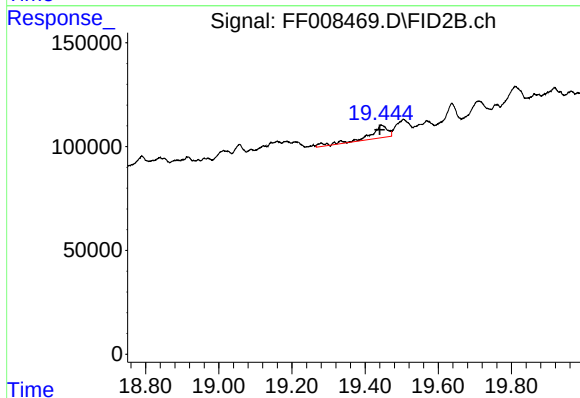

#15 N-TETRATRIACONTANE

R.T.: 19.445 min
Delta R.T.: 0.005 min
Response: 209961
Conc: 1.65 ug/ml

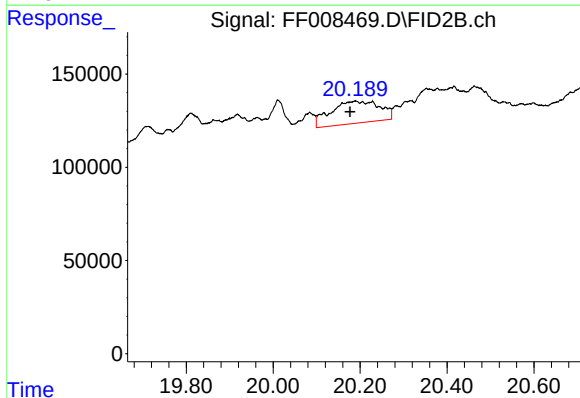

#16 N-HEXATRIACONTANE

R.T.: 20.189 min
Delta R.T.: 0.012 min
Response: 928944
Conc: 7.78 ug/ml