

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008472.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 14:09
Operator : DD\AJ
Sample : M2580-17 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

2)	N-DECANE	4.526	65012	0.482 ug/ml
10)	N-TETRACOSANE	14.973	641186	4.496 ug/ml
12)	N-OCTACOSANE	16.973	168986	1.204 ug/ml
14)	N-DOTRIACONTANE	18.623	95501	0.705 ug/ml
15)	N-TETRATRIACONTANE	19.503f	147606	1.158 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008472.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 14:09
Operator : DD\AJ
Sample : M2580-17 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 02:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

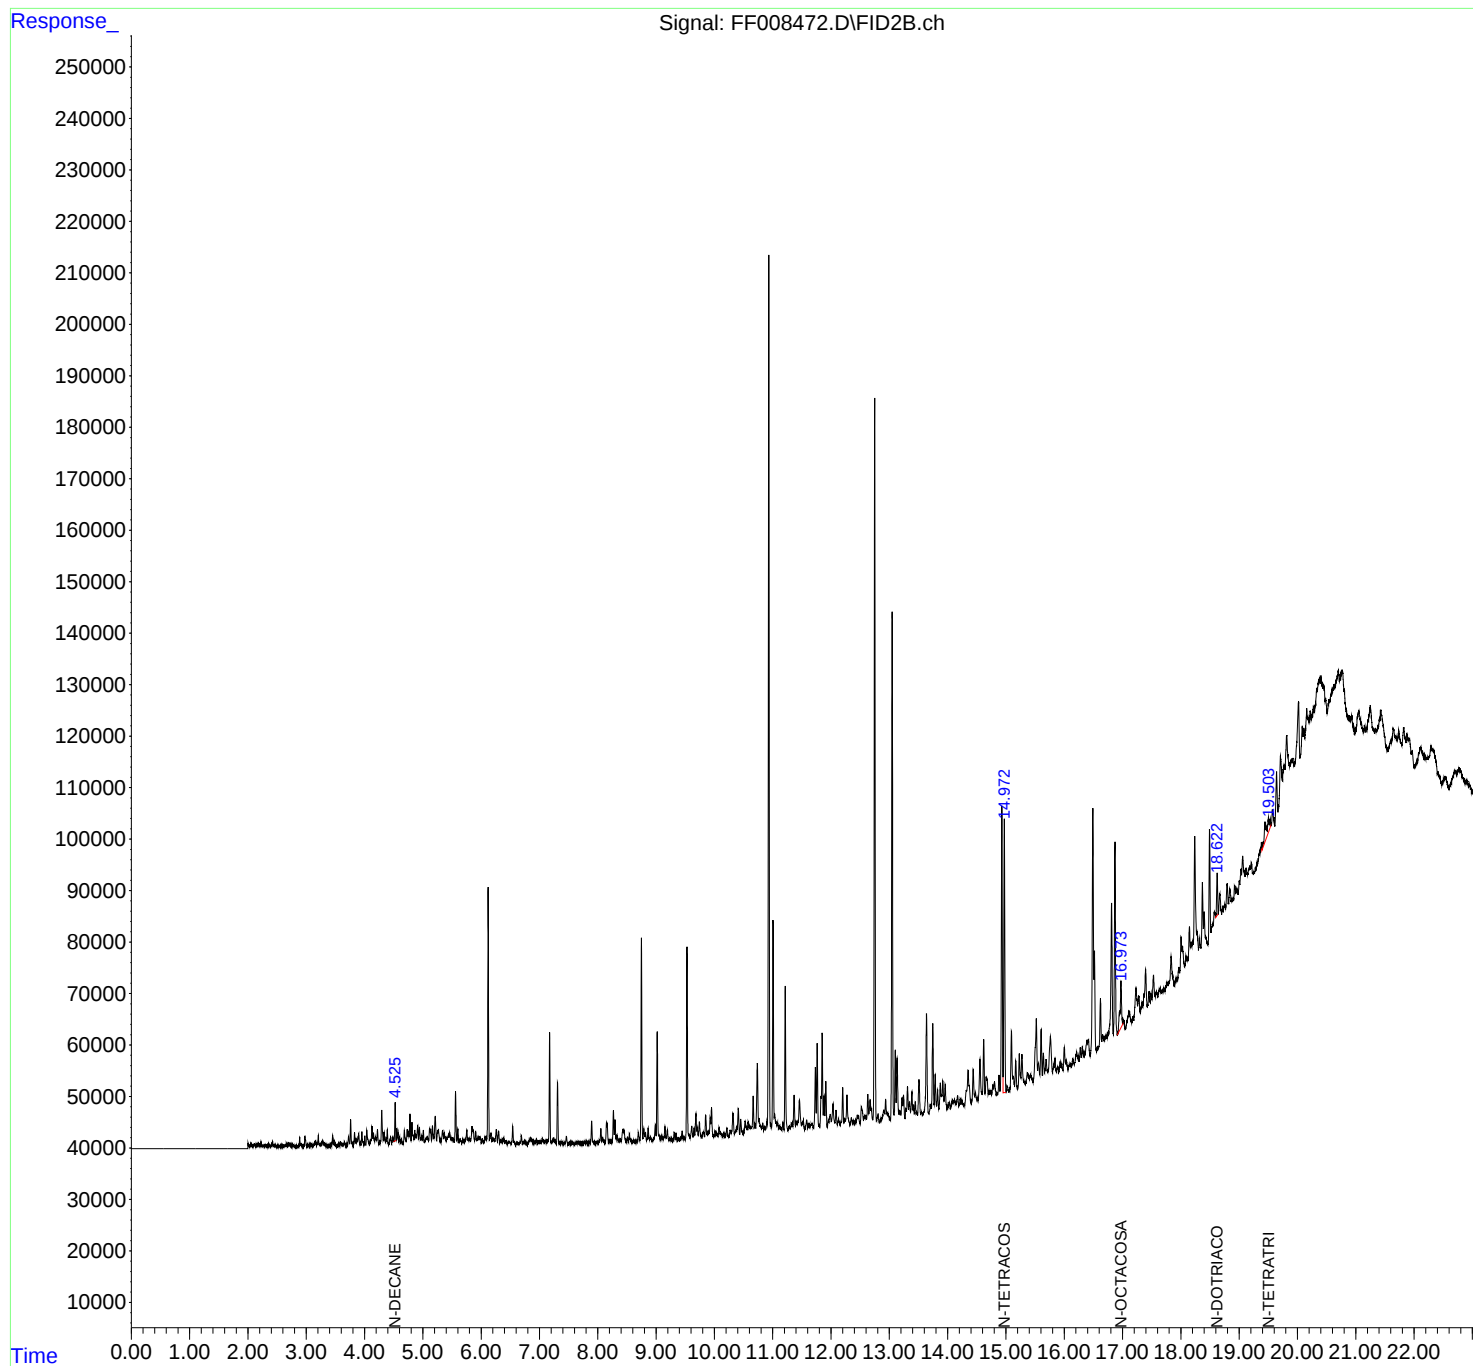


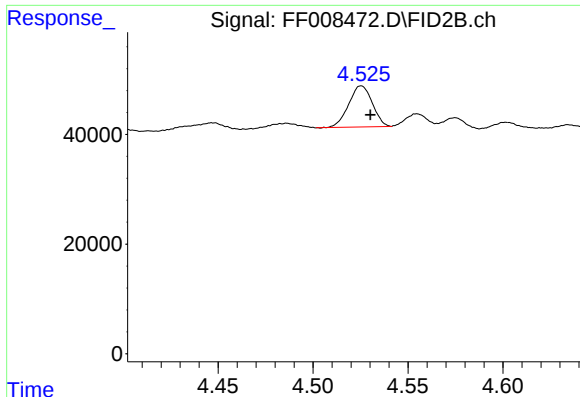

#2 N-DECANE


R.T.: 4.526 min
Delta R.T.: -0.005 min
Response: 65012
Conc: 0.48 ug/ml

Instrument :
FID_F
ClientSampleId :

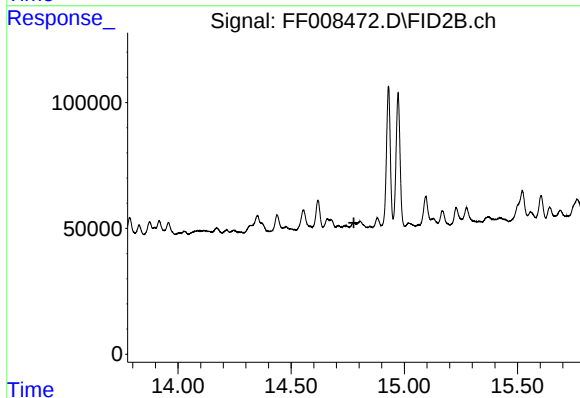


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

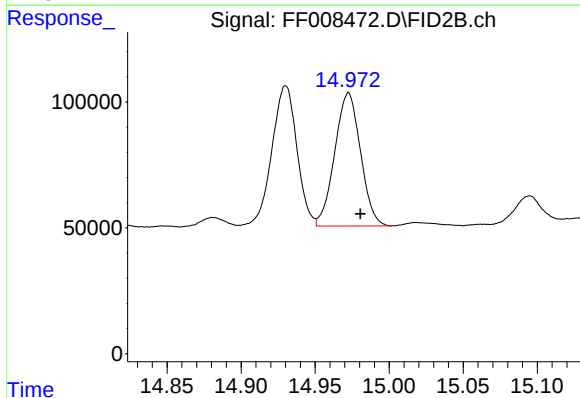


#10 N-TETRACOSANE

R.T.: 14.973 min
Delta R.T.: -0.008 min
Response: 641186
Conc: 4.50 ug/ml

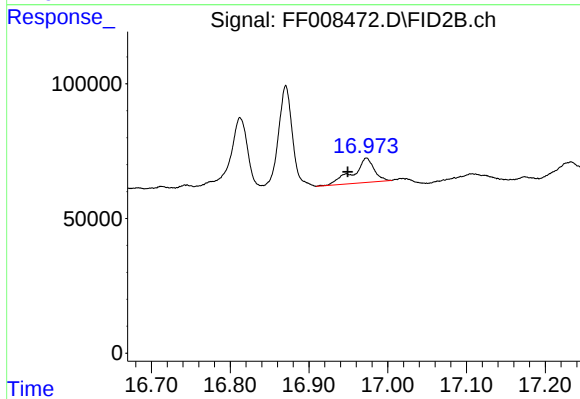

#12 N-OCTACOSANE


R.T.: 16.973 min
Delta R.T.: 0.024 min
Response: 168986
Conc: 1.20 ug/ml

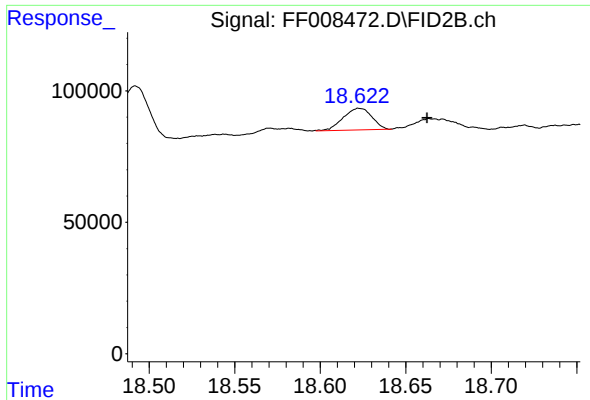

#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: -0.040 min
Response: 95501
Conc: 0.70 ug/ml

Instrument :
FID_F
ClientSampleId :

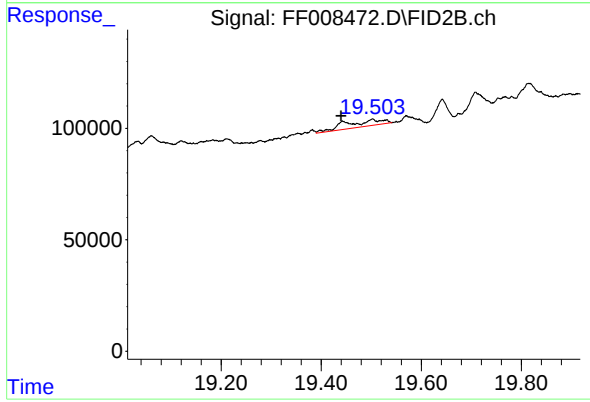

#15 N-TETRATRIACONTANE

R.T.: 19.503 min
Delta R.T.: 0.063 min
Response: 147606
Conc: 1.16 ug/ml