

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008476.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 16:19
Operator : DD\AJ
Sample : M2580-10 30X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:17:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	17.832	171528	1.238 ug/ml
14) N-DOTRIACONTANE	18.664	103713	0.765 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008476.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 16:19
Operator : DD\AJ
Sample : M2580-10 30X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:17:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

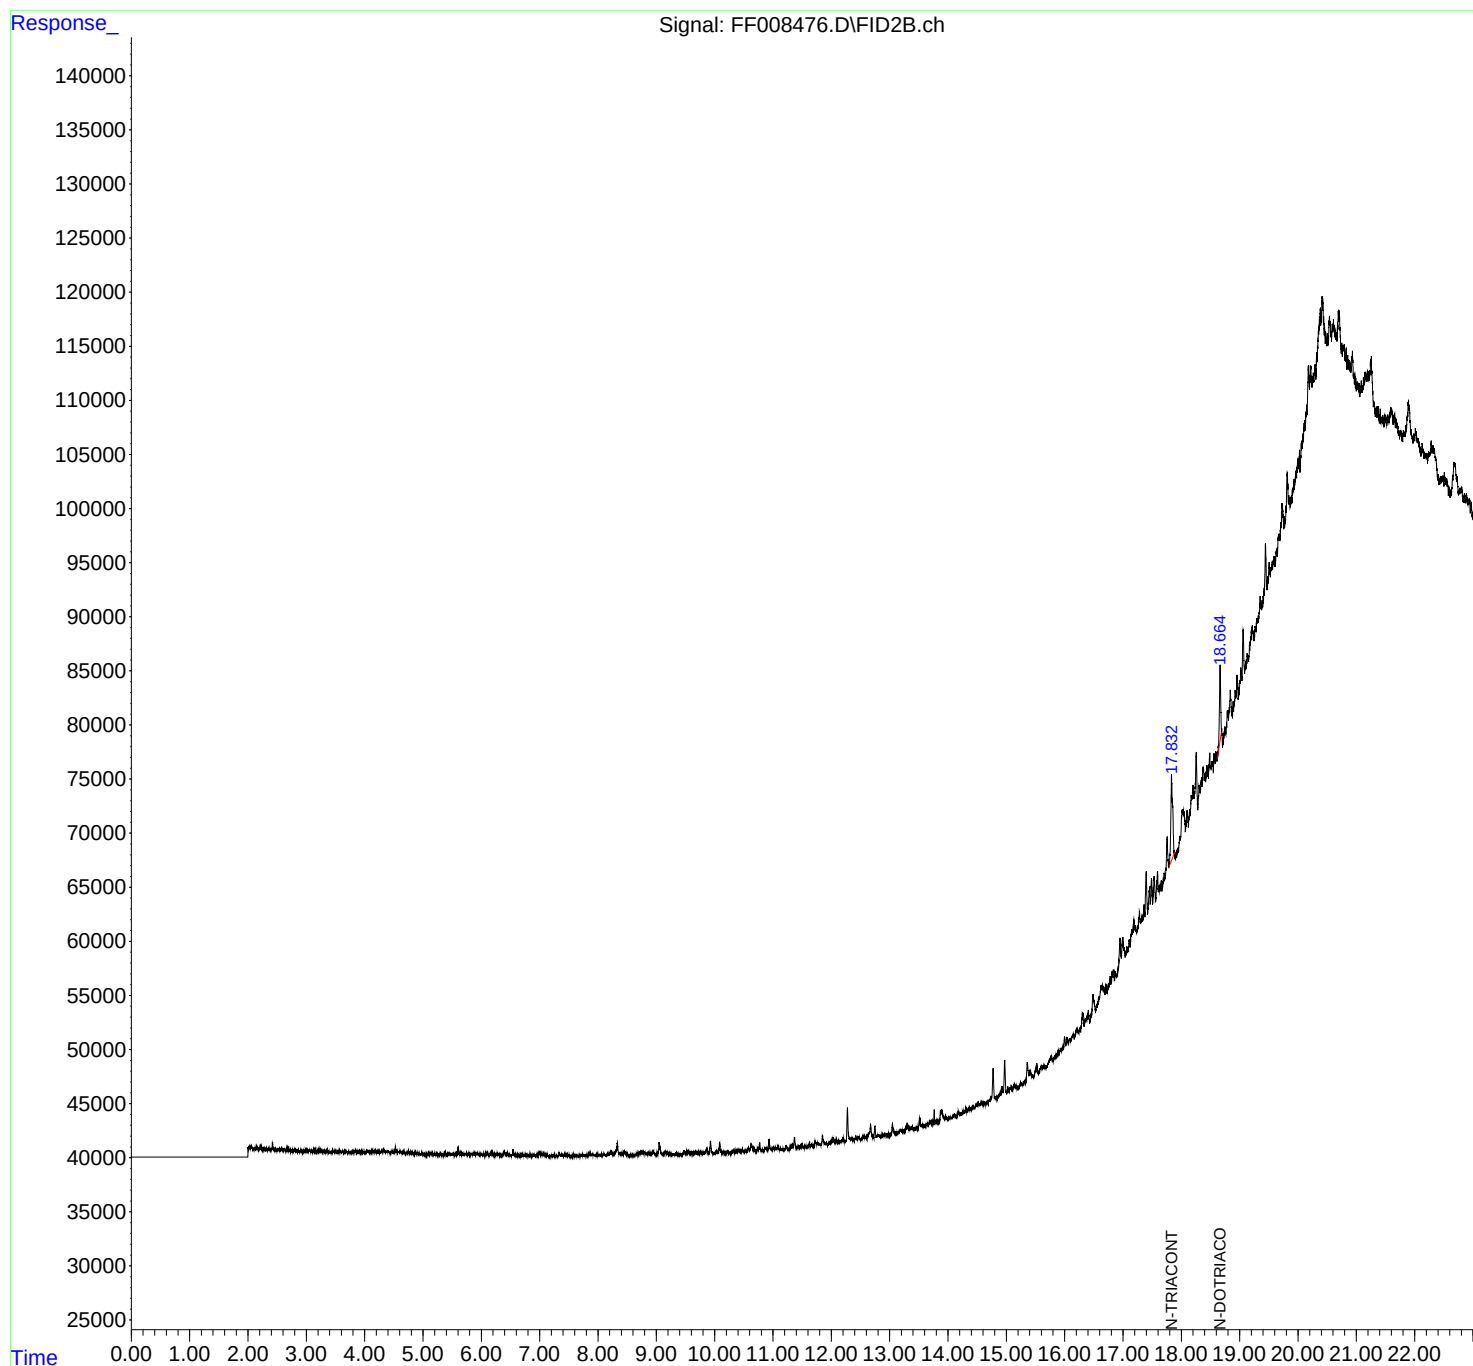


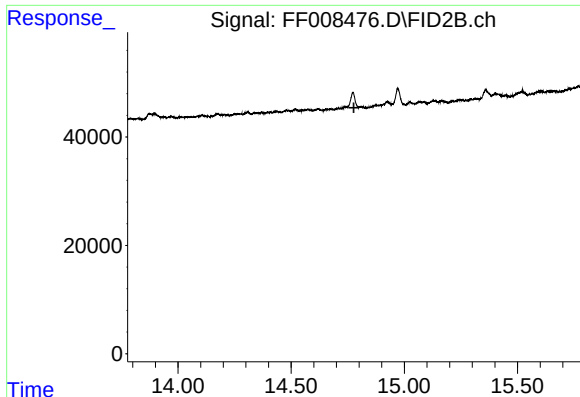

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

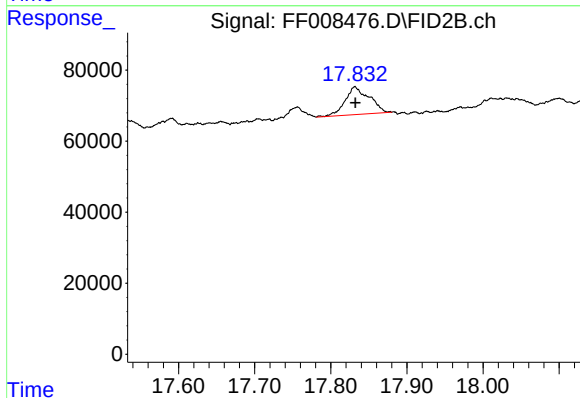

#13 N-TRIACONTANE

R.T.: 17.832 min
Delta R.T.: 0.000 min
Response: 171528
Conc: 1.24 ug/ml

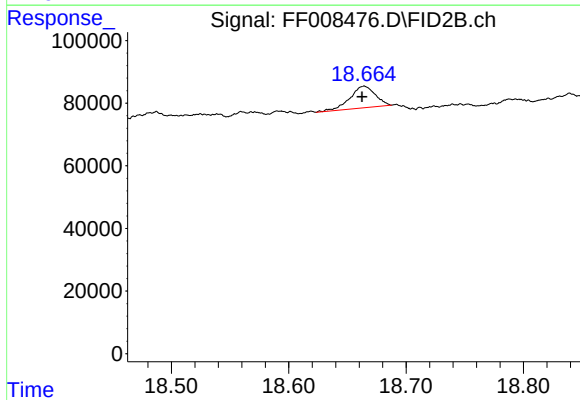

#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: 0.002 min
Response: 103713
Conc: 0.77 ug/ml