

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008478.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 17:22
Operator : DD\AJ
Sample : M2580-17 100X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:17:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	14.972	308442	2.163 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008478.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 17:22
Operator : DD\AJ
Sample : M2580-17 100X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 04 03:17:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

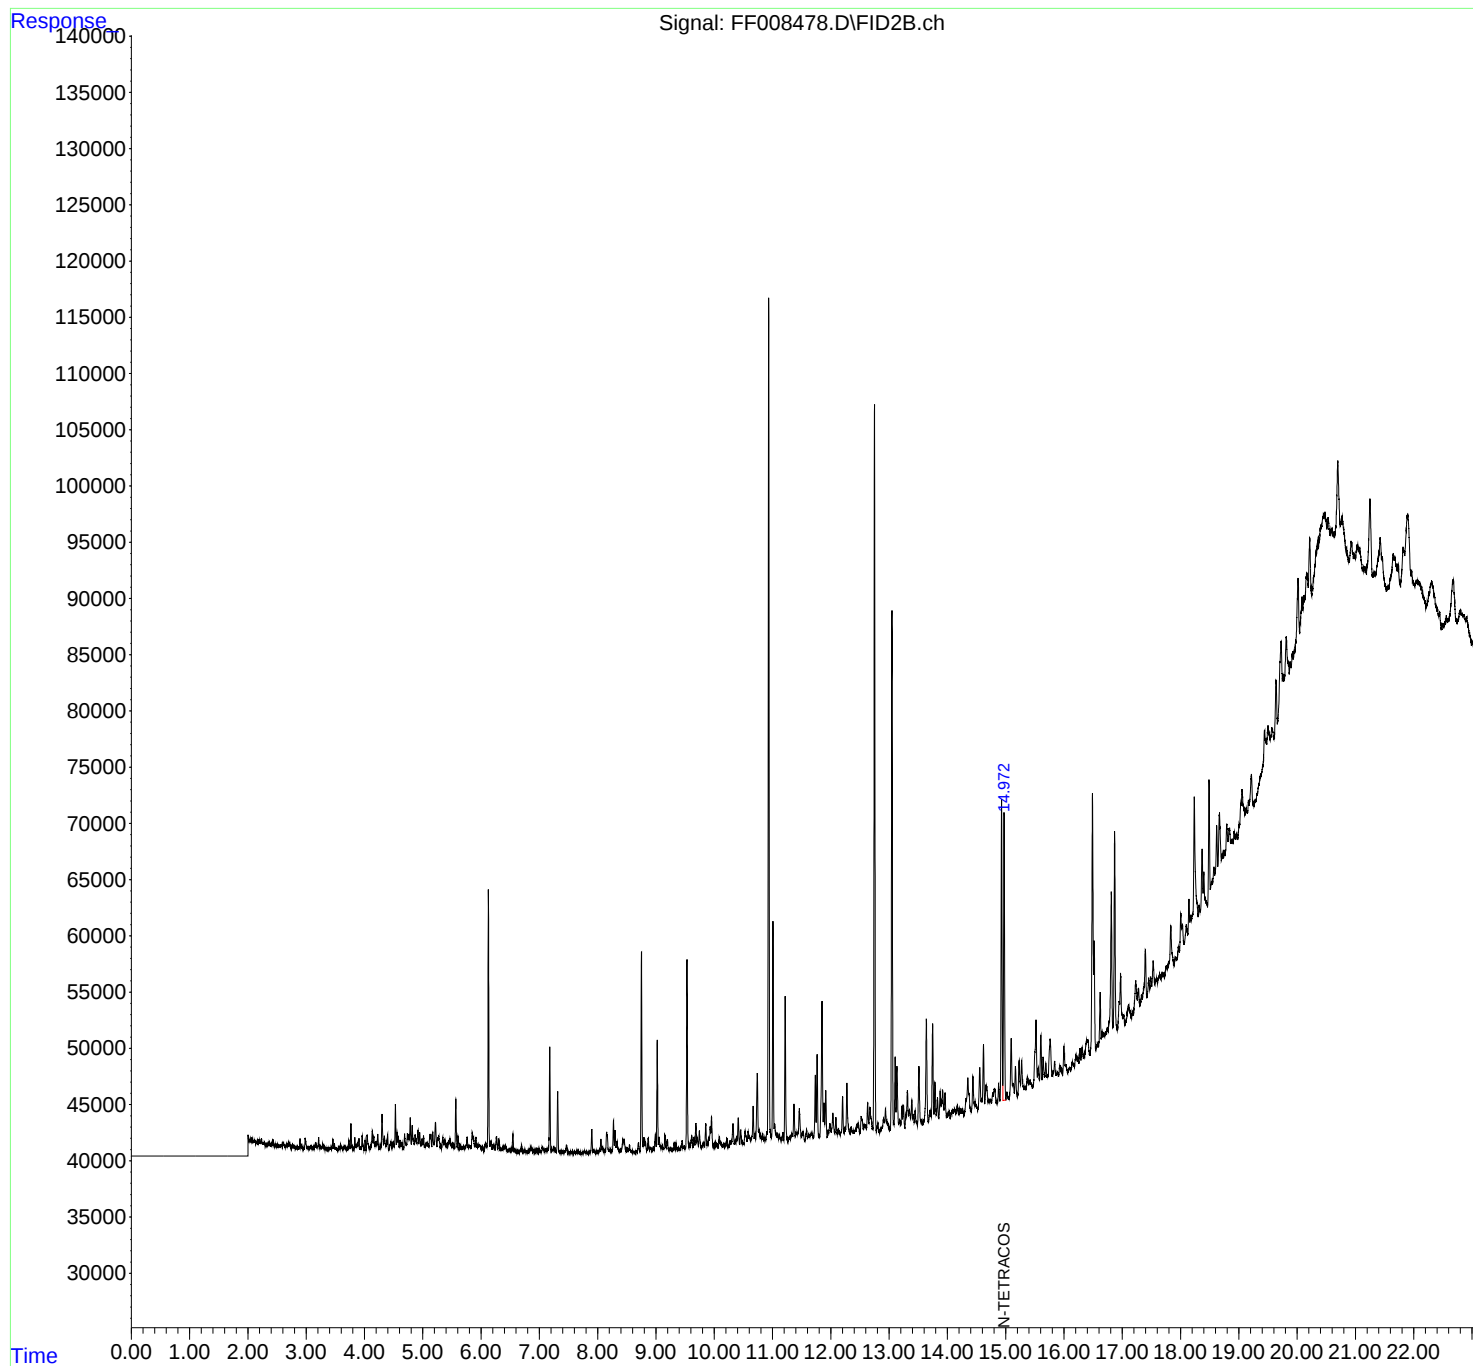


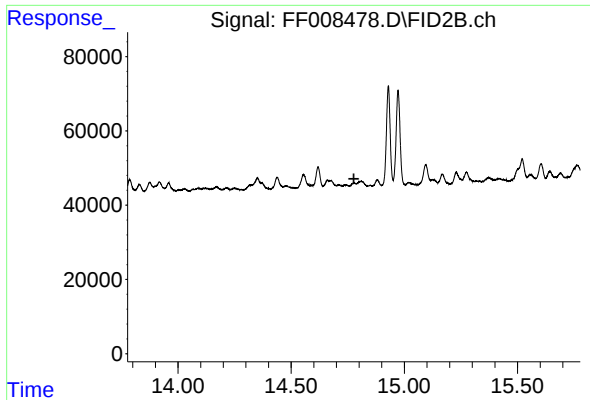

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

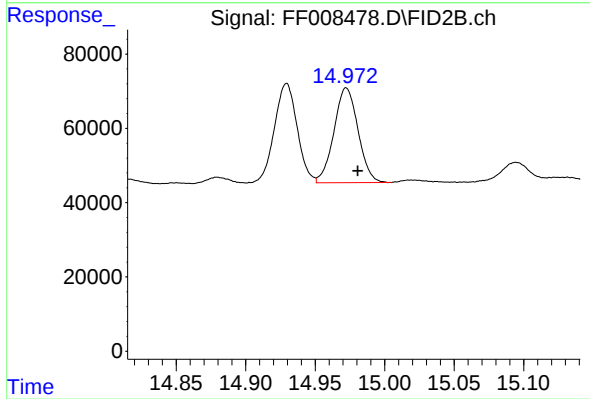

#10 N-TETRACOSANE

R.T.: 14.972 min
Delta R.T.: -0.008 min
Response: 308442
Conc: 2.16 ug/ml