

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008466.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 10:48
Operator : DD\AJ
Sample : M2580-13 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
18-B5(0-2)

Integration File: autoint1.e
Quant Time: Jun 04 02:55:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.773	1098799	8.801 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008466.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 10:48
Operator : DD\AJ
Sample : M2580-13 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
18-B5(0-2)

Integration File: autoint1.e
Quant Time: Jun 04 02:55:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

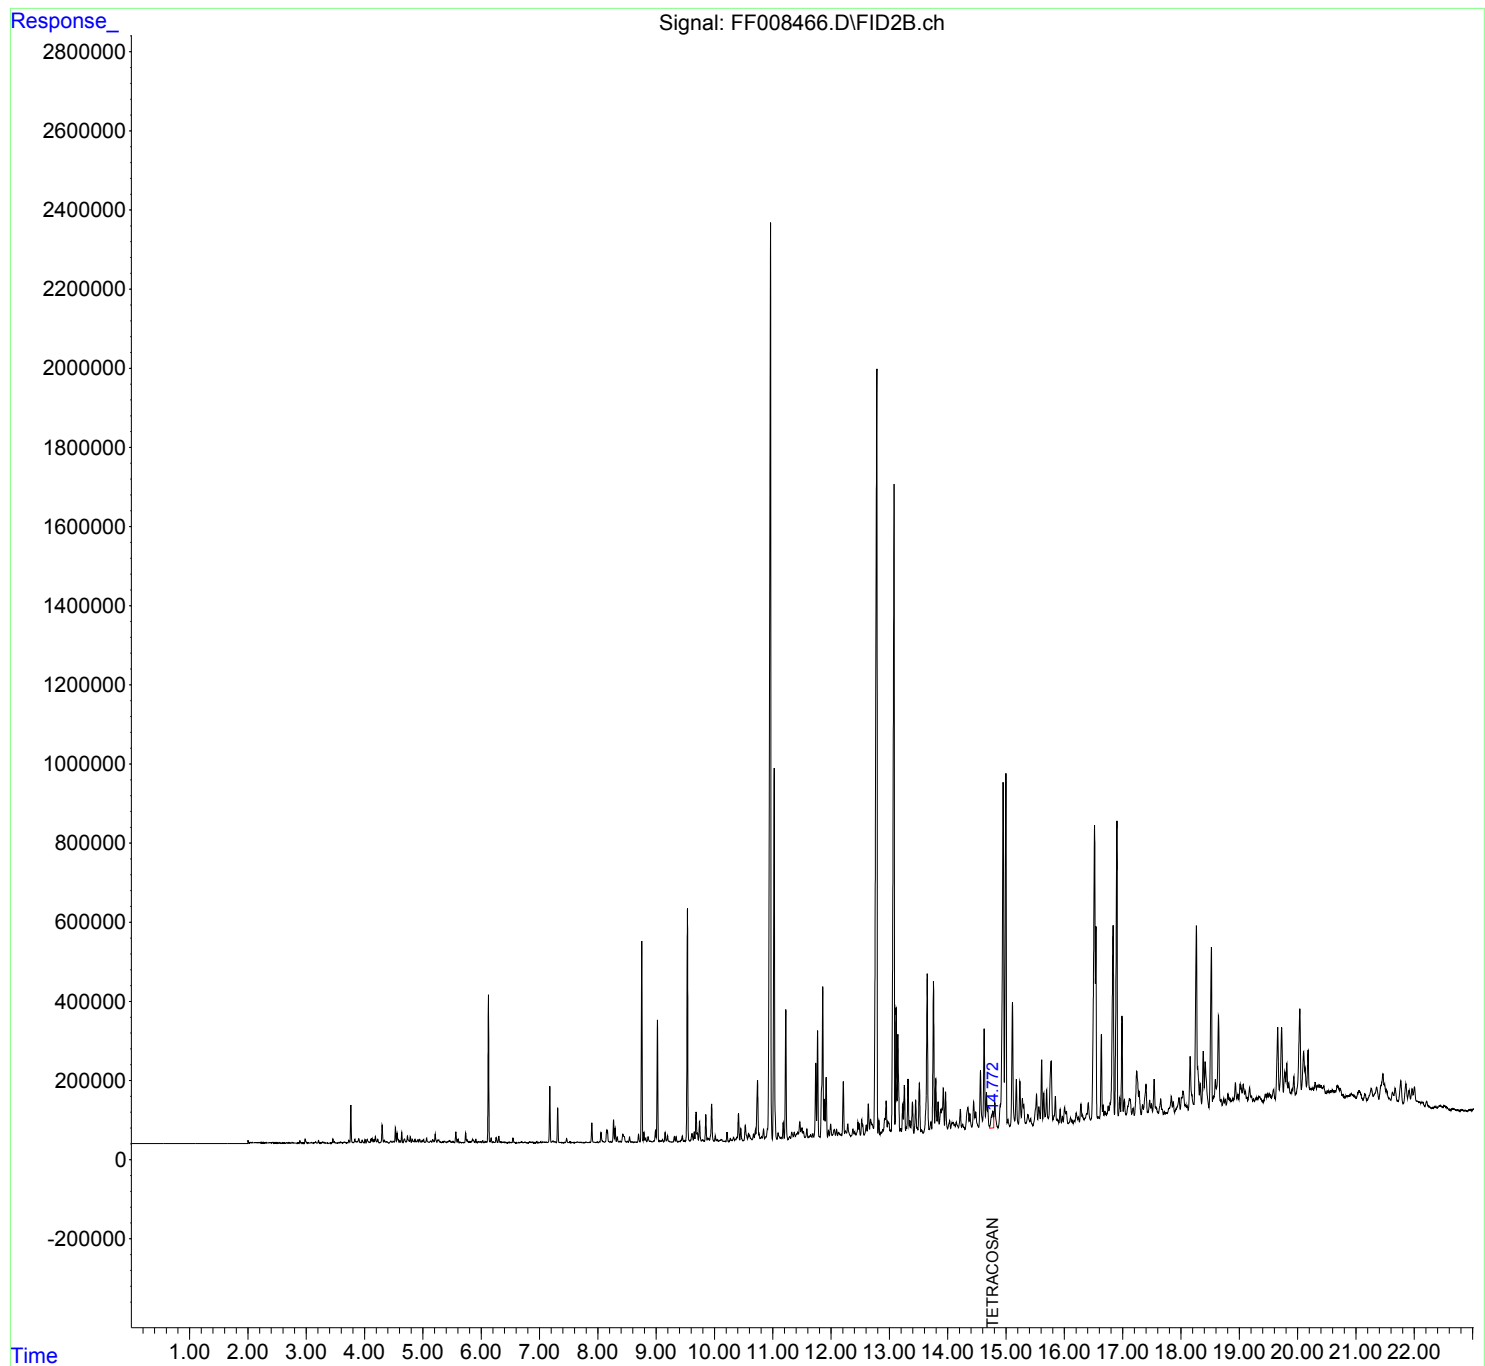

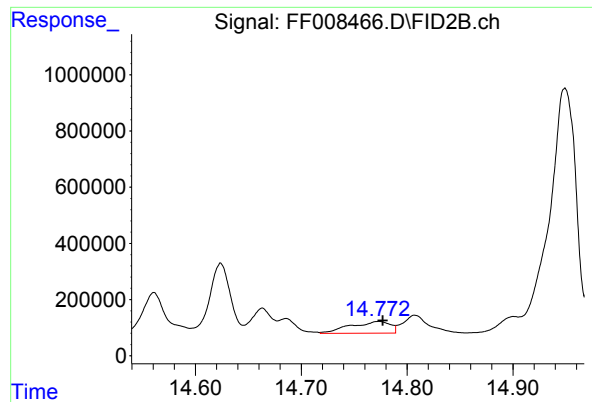

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.773 min
Delta R.T.: -0.004 min
Response: 1098799
Conc: 8.80 ug/ml

Instrument :
FID_F
ClientSampleId :
18-B5(0-2)