

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008472.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 14:09
Operator : DD\AJ
Sample : M2580-17 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
18-B6(6-12)

Manual Integrations
APPROVED

Ankita
6/4/2021 3:30:34 PM

Integration File: autoint1.e
Quant Time: Jun 04 02:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.774	29930	0.240 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060321\
Data File : FF008472.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2021 14:09
Operator : DD\AJ
Sample : M2580-17 50X
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
18-B6(6-12)


Manual Integrations
APPROVED

Ankita
6/4/2021 3:30:34 PM

Integration File: autoint1.e
Quant Time: Jun 04 02:56:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

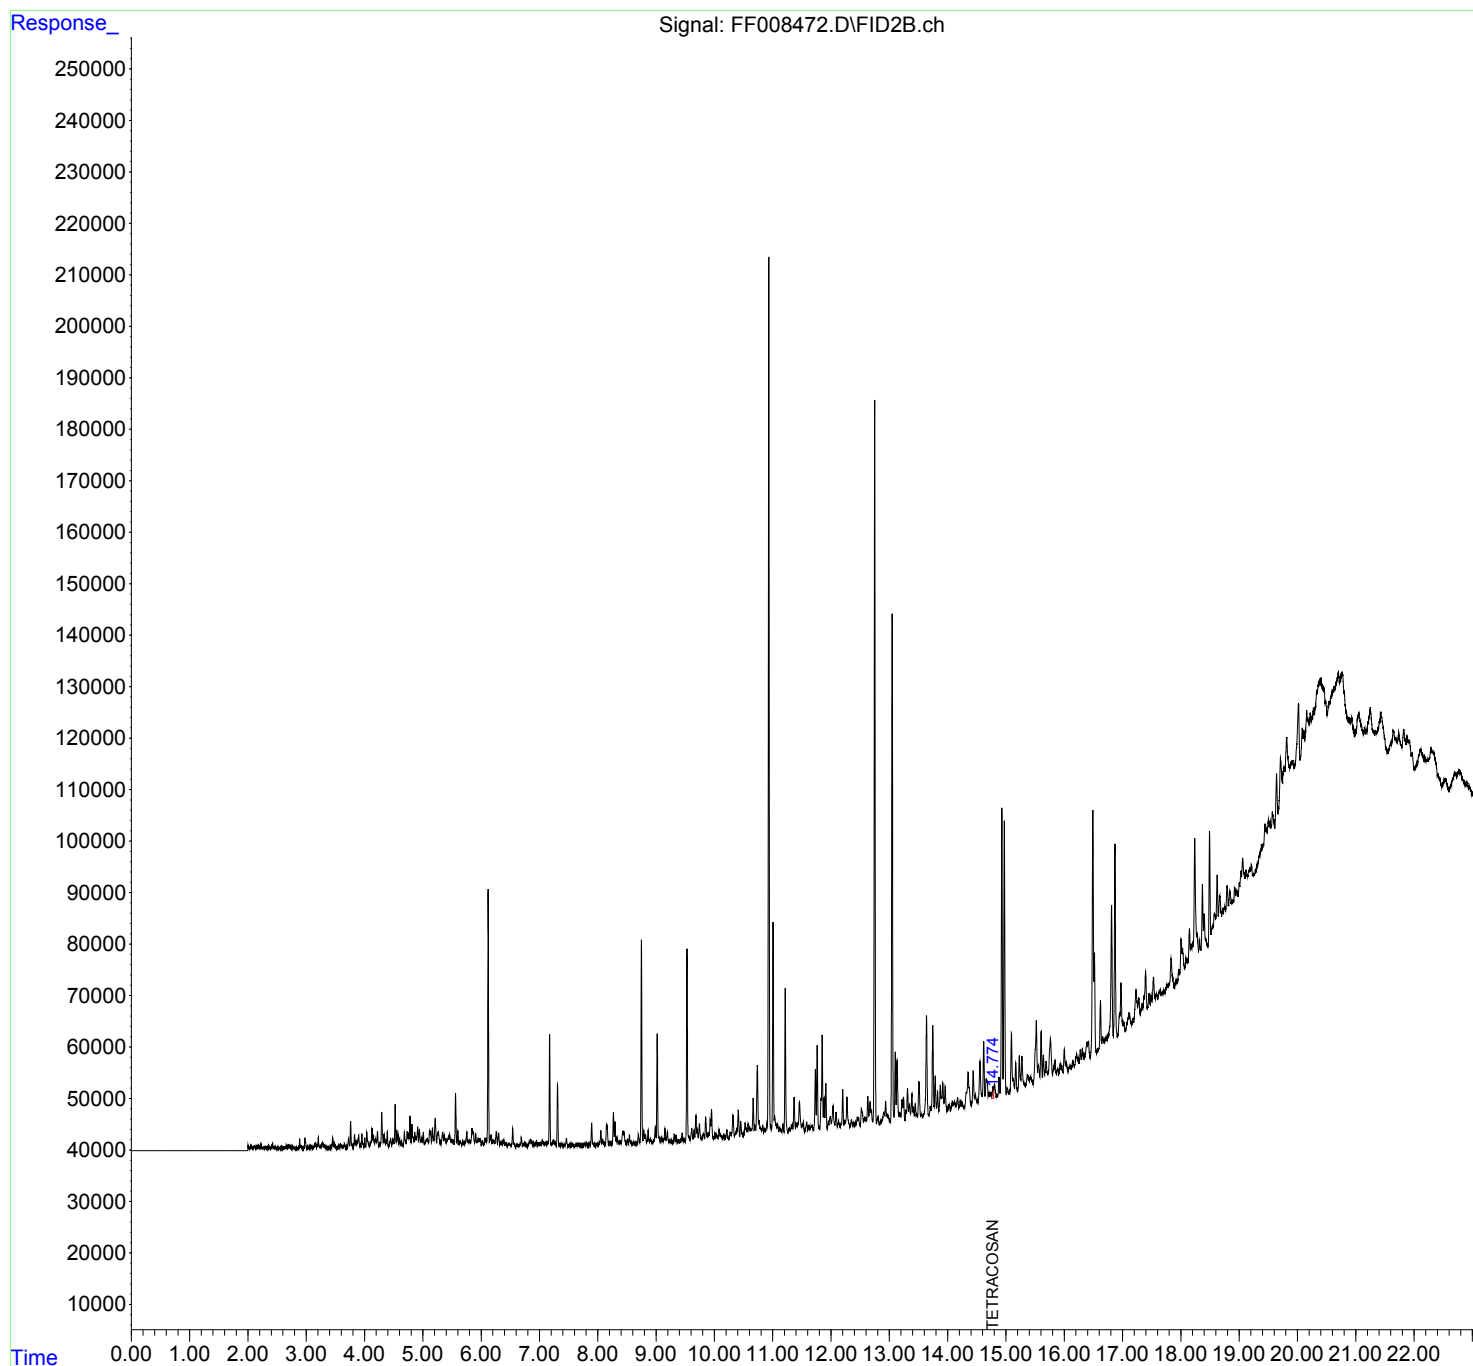

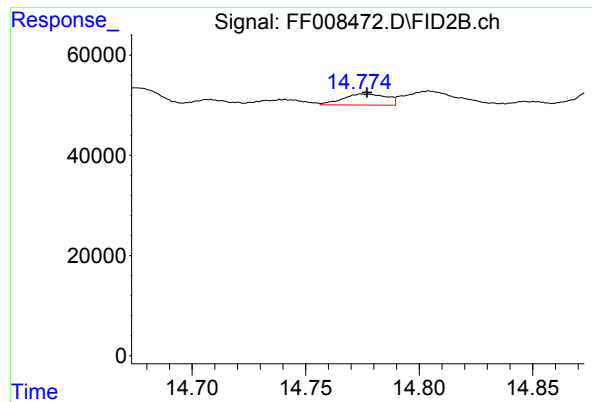

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.774 min
Delta R.T.: -0.003 min
Response: 29930
Conc: 0.24 ug/ml m

Instrument :
FID_F
ClientSampleId :
18-B6(6-12)

Manual Integrations
APPROVED

Ankita
6/4/2021 3:30:34 PM