

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060419\
 Data File : FF004709.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2019 11:05
 Operator : AJ\SJ
 Sample : K2641-13 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 04 14:33:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.715	679231	5.562 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.301f	313976	2.138 ug/ml
7)	N-EICOSANE	12.669f	235924	1.629 ug/ml
10)	N-TETRACOSANE	14.896	153287	1.106 ug/ml
12)	N-OCTACOSANE	16.900	228318	1.679 ug/ml
13)	N-TRIACONTANE	17.794	533098	3.855 ug/ml
14)	N-DOTRIACONTANE	18.634	279632	2.021 ug/ml
15)	N-TETRATRIACONTANE	19.423	71270	0.521 ug/ml
16)	N-HEXATRIACONTANE	20.134	394425	2.996 ug/ml
18)	N-TETRACONTANE	21.875	333722	2.710 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060419\
Data File : FF004709.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2019 11:05
Operator : AJ\SJ
Sample : K2641-13 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 04 14:33:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

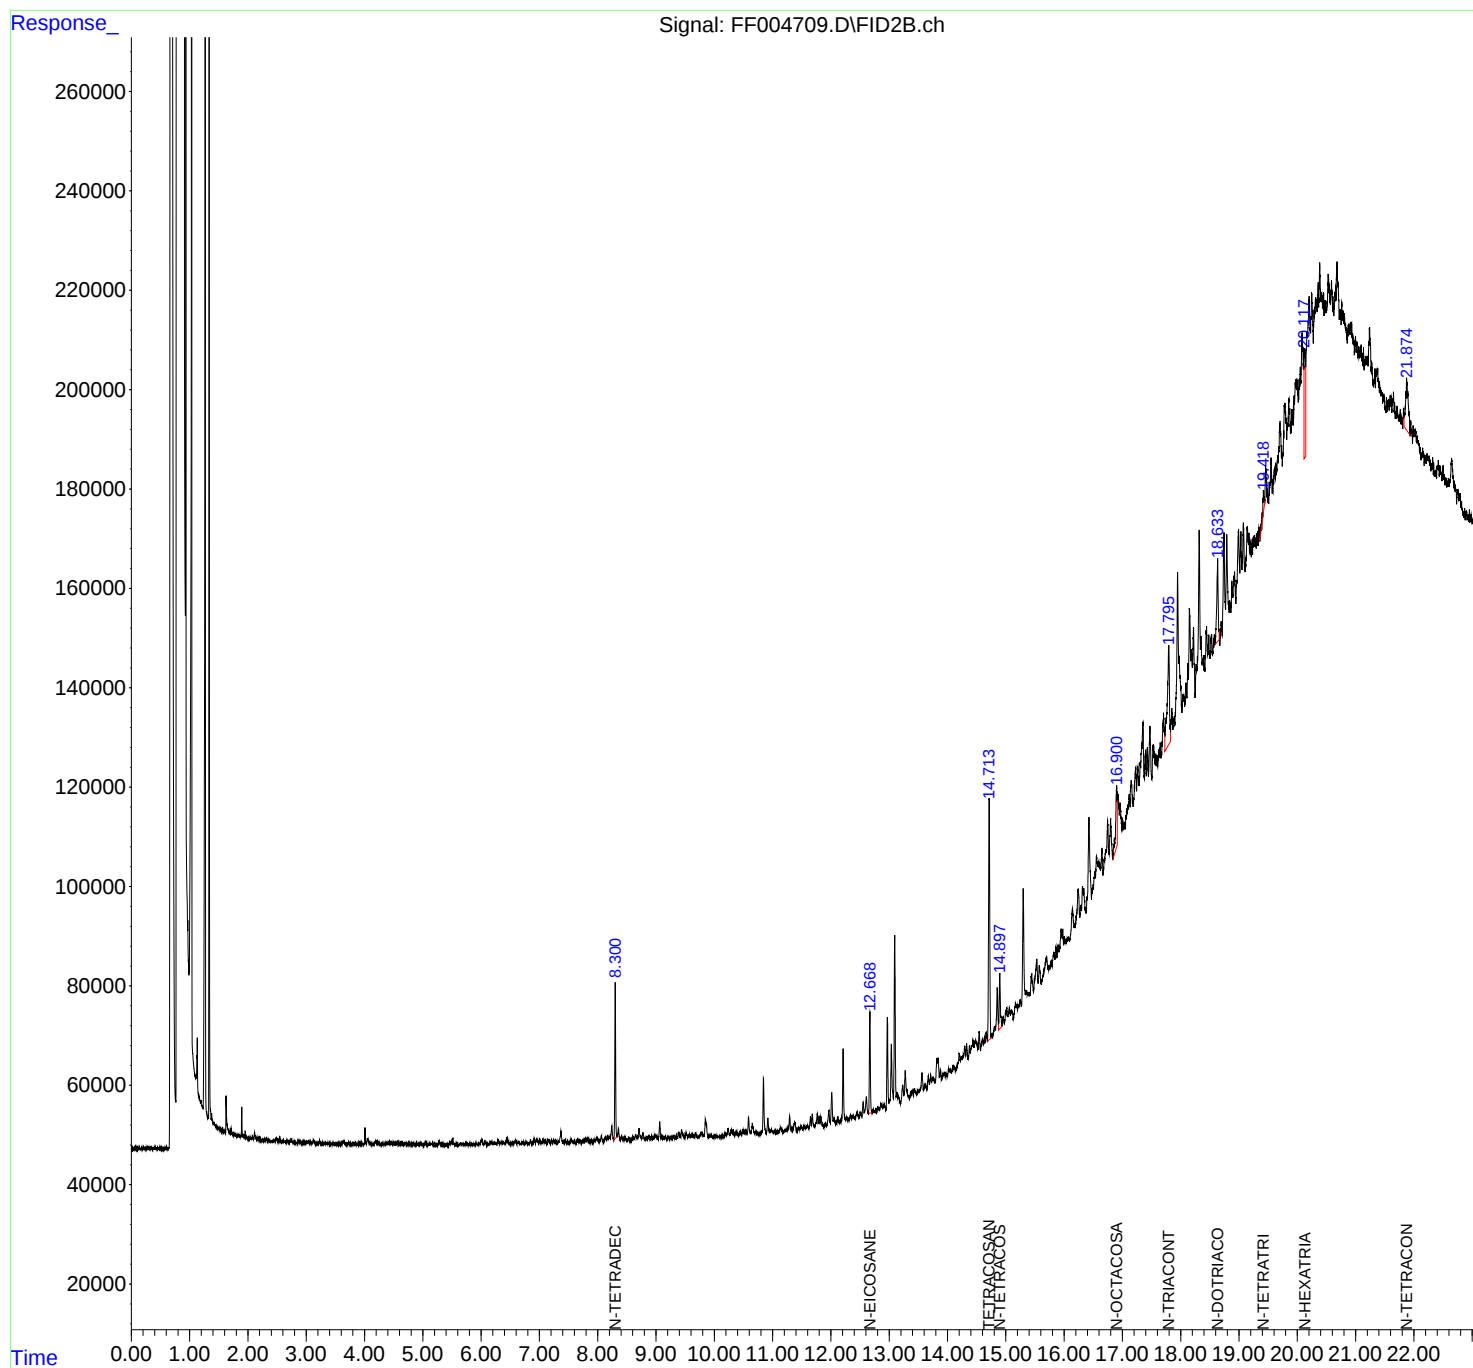

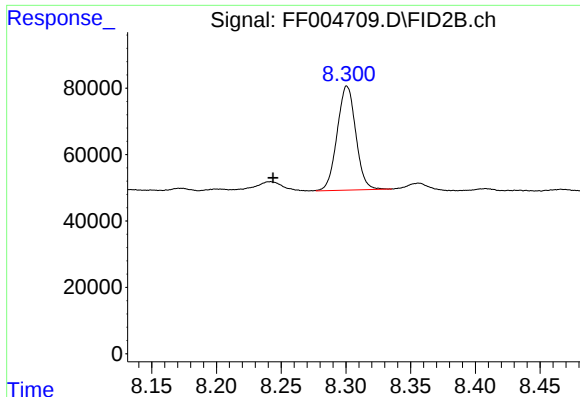


#4 N-TETRADECANE

R.T.: 8.301 min
Delta R.T.: 0.057 min
Response: 313976
Conc: 2.14 ug/ml

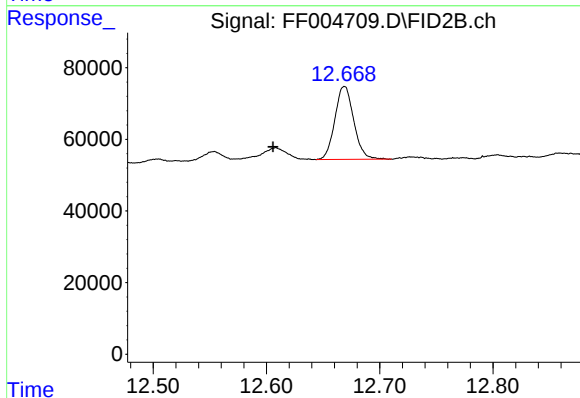


#7 N-EICOSANE

R.T.: 12.669 min
Delta R.T.: 0.063 min
Response: 235924
Conc: 1.63 ug/ml

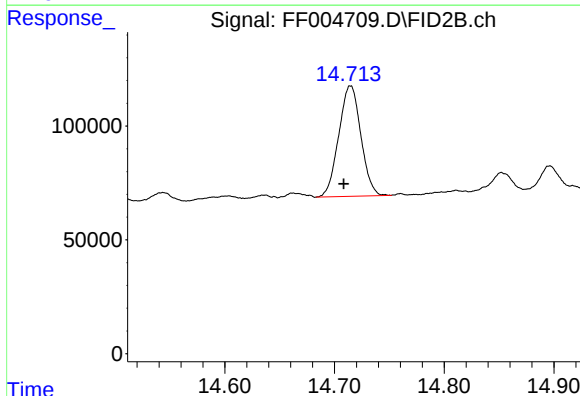


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.715 min
Delta R.T.: 0.006 min
Response: 679231
Conc: 5.56 ug/ml

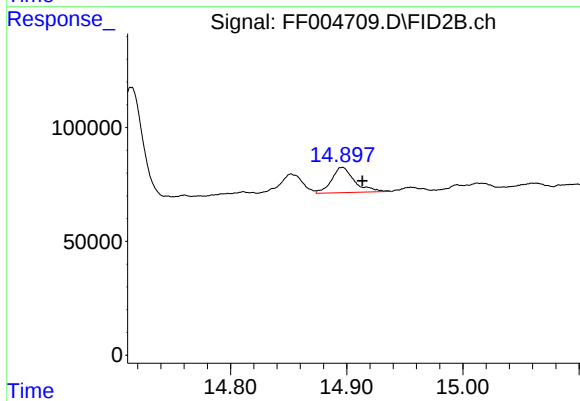


#10 N-TETRACOSANE

R.T.: 14.896 min
Delta R.T.: -0.018 min
Response: 153287
Conc: 1.11 ug/ml

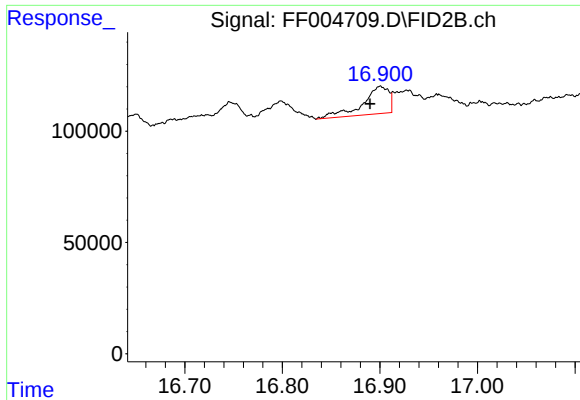


#12 N-OCTACOSANE

R.T.: 16.900 min
Delta R.T.: 0.011 min
Response: 228318
Conc: 1.68 ug/ml

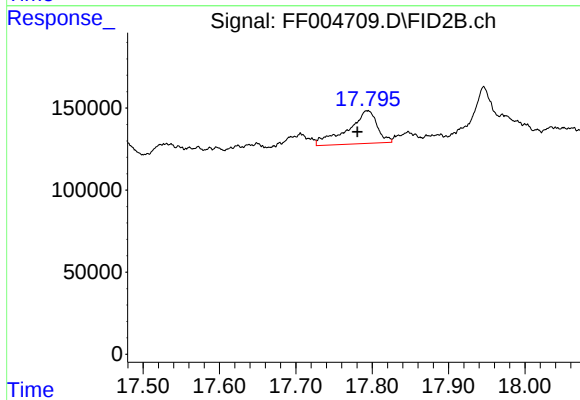


#13 N-TRIACONTANE

R.T.: 17.794 min
Delta R.T.: 0.013 min
Response: 533098
Conc: 3.86 ug/ml

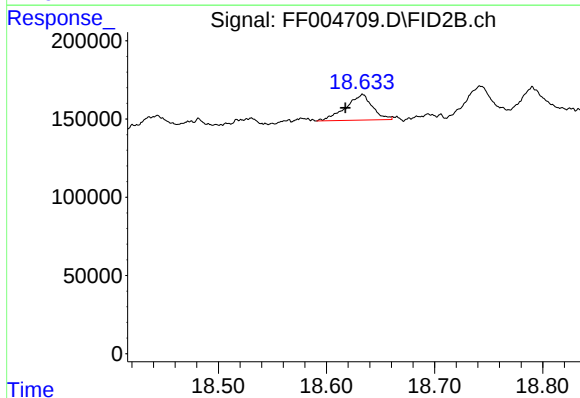


#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: 0.016 min
Response: 279632
Conc: 2.02 ug/ml

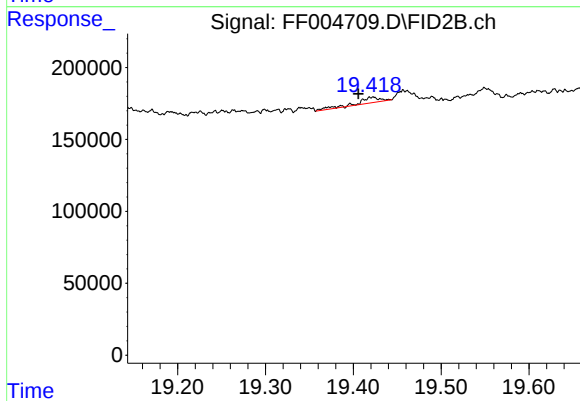


#15 N-TETRATRIACONTANE

R.T.: 19.423 min
Delta R.T.: 0.017 min
Response: 71270
Conc: 0.52 ug/ml

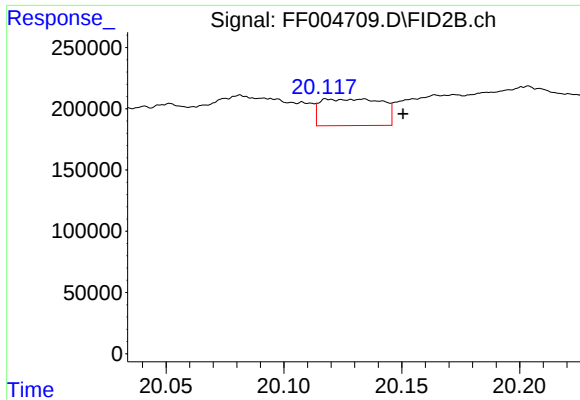

#16 N-HEXATRIACONTANE

R.T.: 20.134 min
Delta R.T.: -0.017 min
Response: 394425
Conc: 3.00 ug/ml

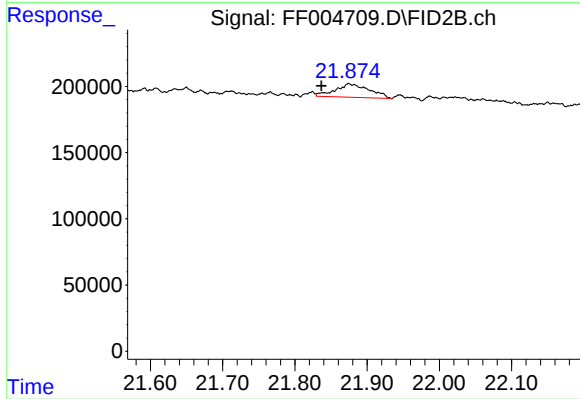

#18 N-TETRACONTANE

R.T.: 21.875 min
Delta R.T.: 0.038 min
Response: 333722
Conc: 2.71 ug/ml