

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060419\
 Data File : FF004707.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2019 10:00
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 04 14:33:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	6251941	51.199 ug/ml
Target Compounds			
2) N-DECANE	4.420	8234690	56.236 ug/ml
3) N-DODECANE	6.447	8060070	54.466 ug/ml
4) N-TETRADECANE	8.245	7807570	53.153 ug/ml
5) N-HEXADECANE	9.850	7661941	51.894 ug/ml
6) N-OCTADECANE	11.297	7407535	51.022 ug/ml
7) N-EICOSANE	12.612	7323011	50.564 ug/ml
8) N-DOCOSANE	13.815	7180067	50.812 ug/ml
10) N-TETRACOSANE	14.923	7164799	51.699 ug/ml
11) N-HEXACOSANE	15.949	7188497	52.758 ug/ml
12) N-OCTACOSANE	16.902	7238074	53.237 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060419\
Data File : FF004707.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2019 10:00
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 04 14:33:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

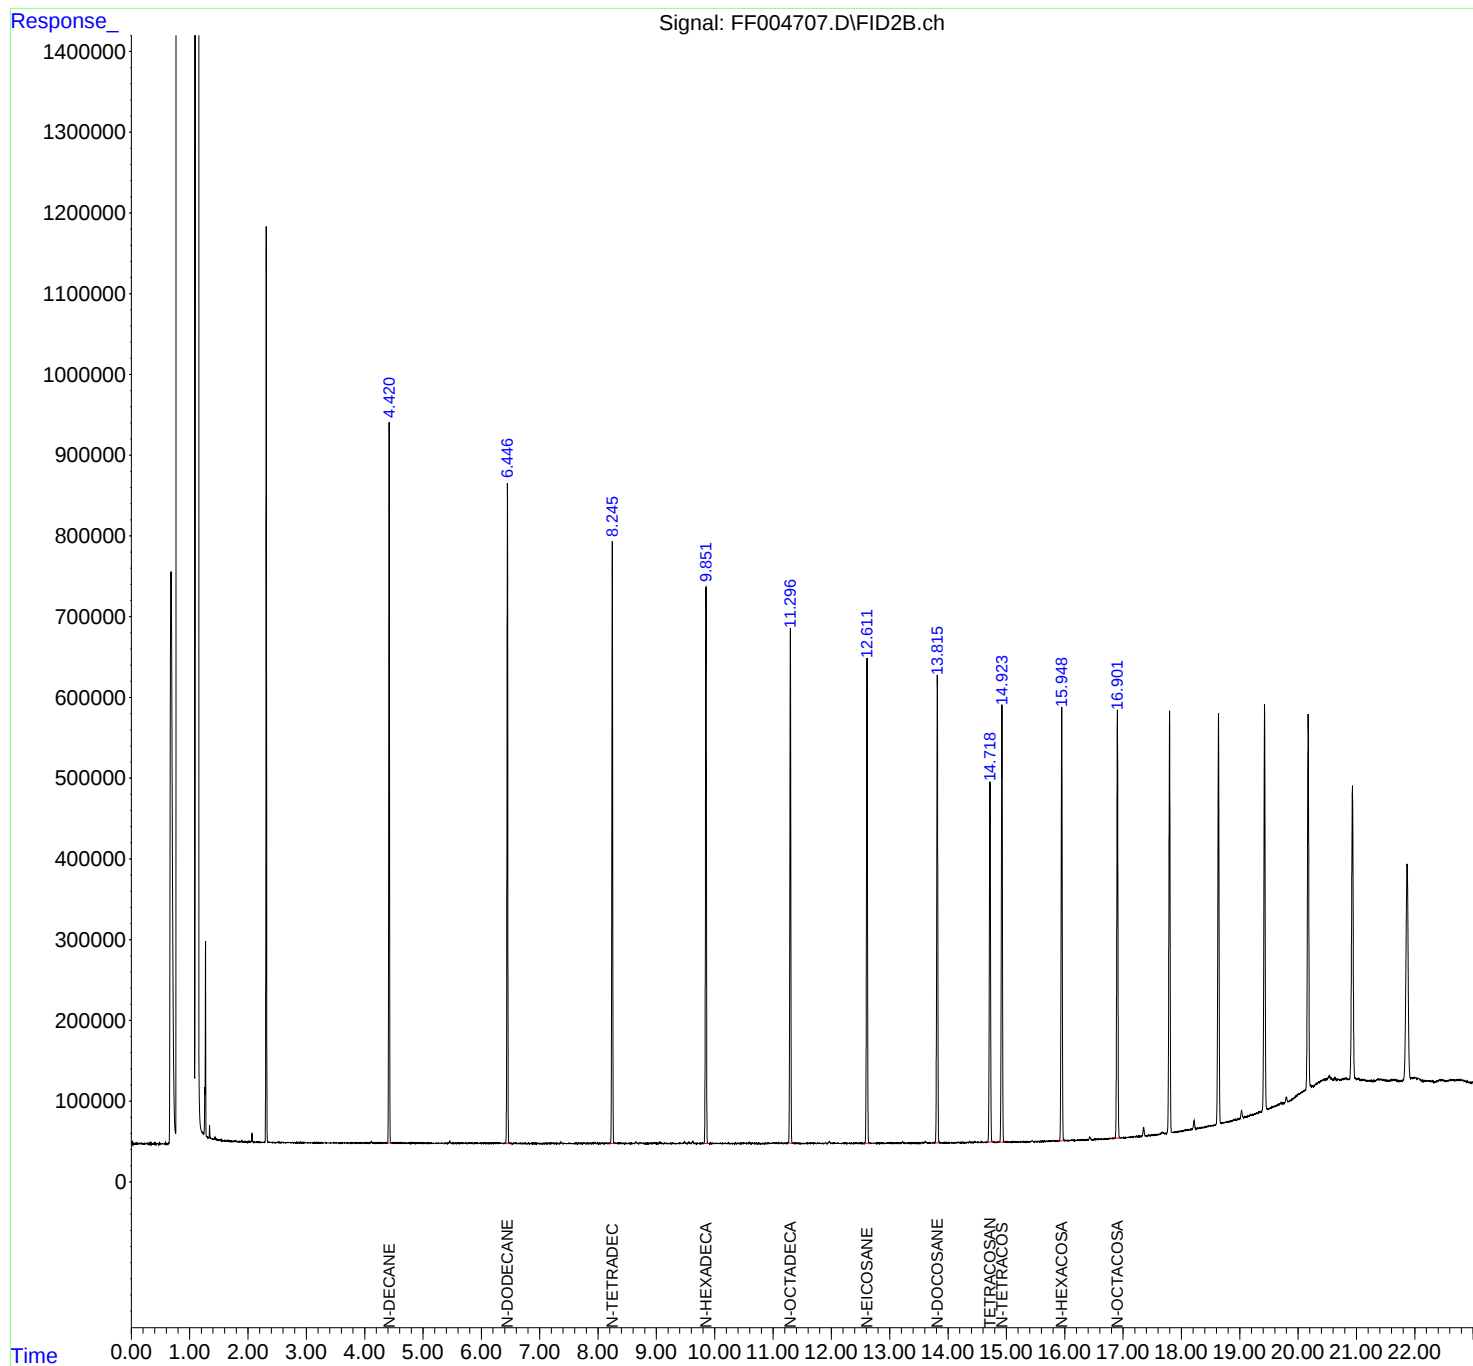

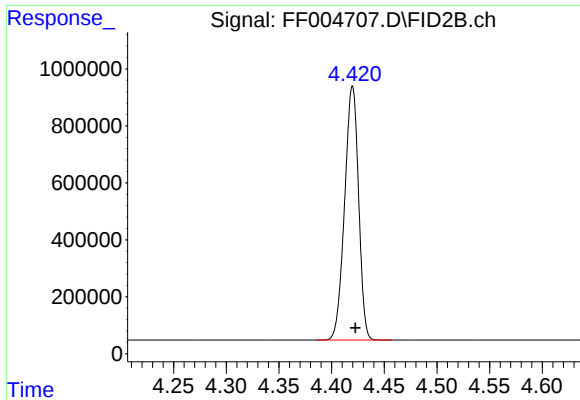


#2 N-DECANE

R.T.: 4.420 min
Delta R.T.: -0.003 min
Response: 8234690
Conc: 56.24 ug/ml

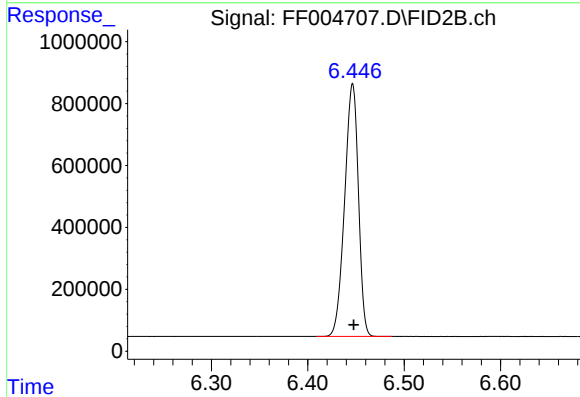


#3 N-DODECANE

R.T.: 6.447 min
Delta R.T.: -0.001 min
Response: 8060070
Conc: 54.47 ug/ml

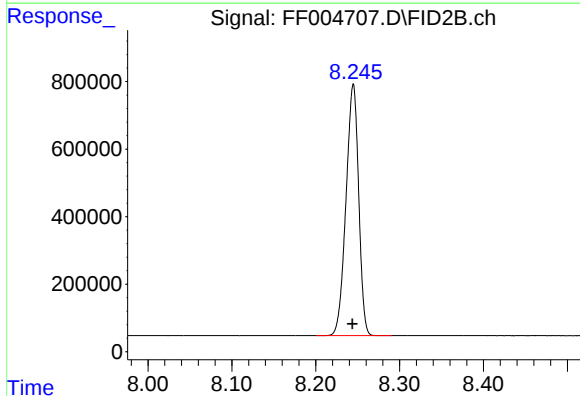


#4 N-TETRADECANE

R.T.: 8.245 min
Delta R.T.: 0.001 min
Response: 7807570
Conc: 53.15 ug/ml

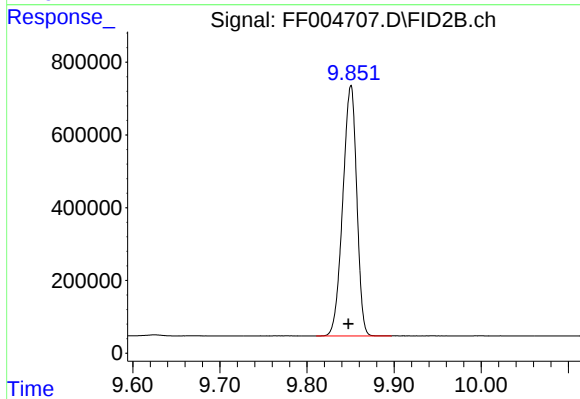


#5 N-HEXADECANE

R.T.: 9.850 min
Delta R.T.: 0.003 min
Response: 7661941
Conc: 51.89 ug/ml

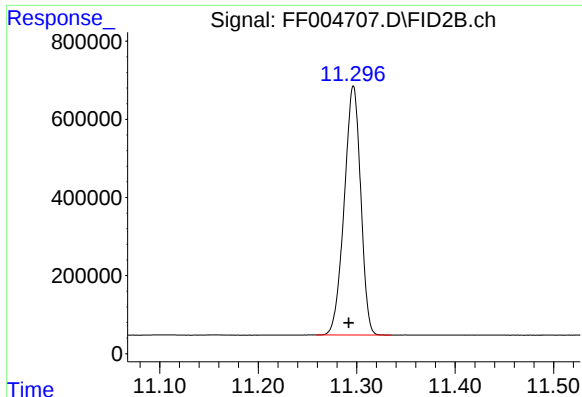


#6 N-OCTADECANE

R.T.: 11.297 min
Delta R.T.: 0.005 min
Response: 7407535
Conc: 51.02 ug/ml

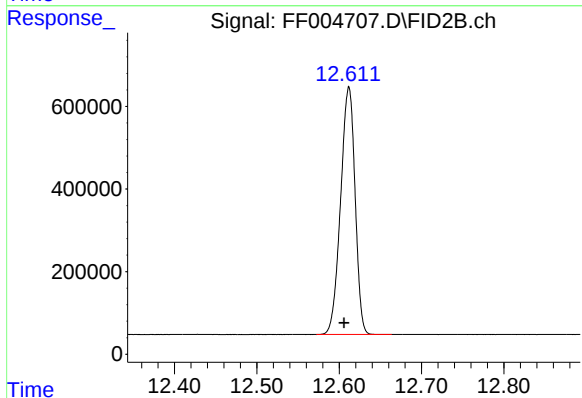


#7 N-EICOSANE

R.T.: 12.612 min
Delta R.T.: 0.006 min
Response: 7323011
Conc: 50.56 ug/ml

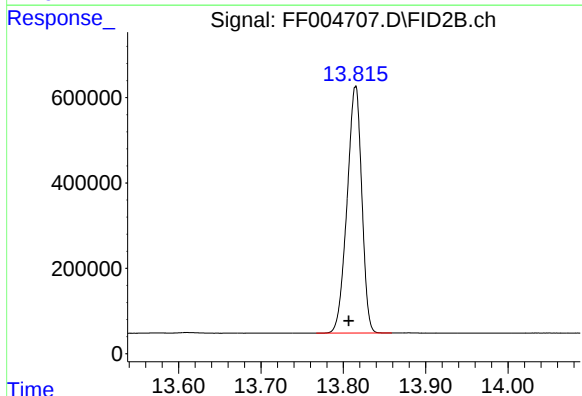


#8 N-DOCOSANE

R.T.: 13.815 min
Delta R.T.: 0.008 min
Response: 7180067
Conc: 50.81 ug/ml

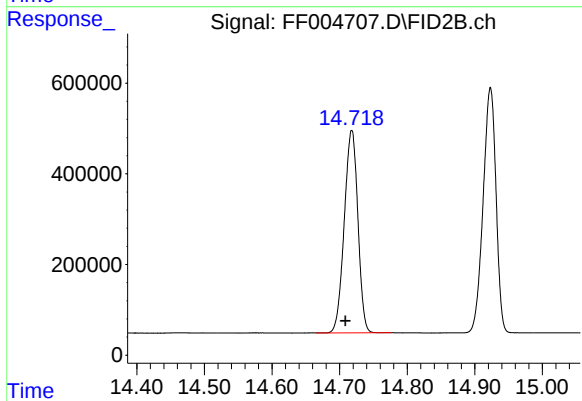


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.718 min
Delta R.T.: 0.010 min
Response: 6251941
Conc: 51.20 ug/ml

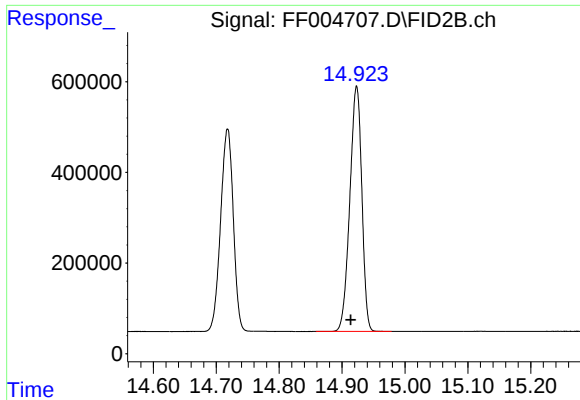


#10 N-TETRACOSANE

R.T.: 14.923 min
Delta R.T.: 0.010 min
Response: 7164799
Conc: 51.70 ug/ml

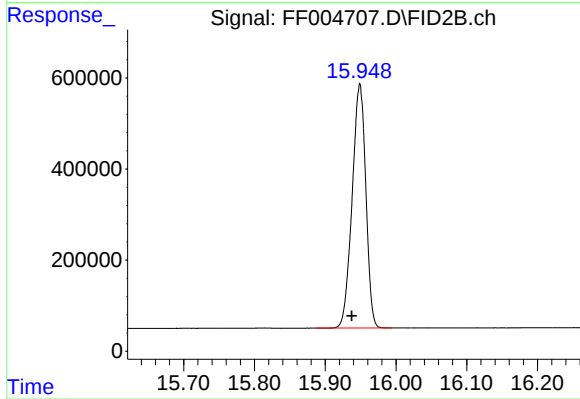

#11 N-HEXACOSANE

R.T.: 15.949 min
Delta R.T.: 0.011 min
Response: 7188497
Conc: 52.76 ug/ml

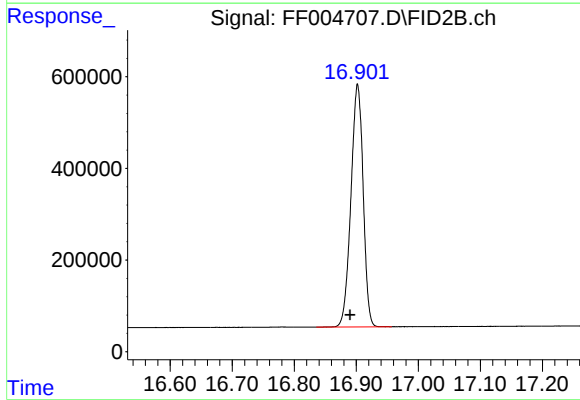

#12 N-OCTACOSANE

R.T.: 16.902 min
Delta R.T.: 0.012 min
Response: 7238074
Conc: 53.24 ug/ml