

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008482.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 08:05
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:19:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.812	96830	0.776 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.964	473506	3.320 ug/ml
14) N-DOTRIACONTANE	18.666	214256	1.581 ug/ml
16) N-HEXATRIACONTANE	20.211	290023	2.430 ug/ml
18) N-TETRACONTANE	21.894	408771	3.596 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008482.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 08:05
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 05 00:19:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

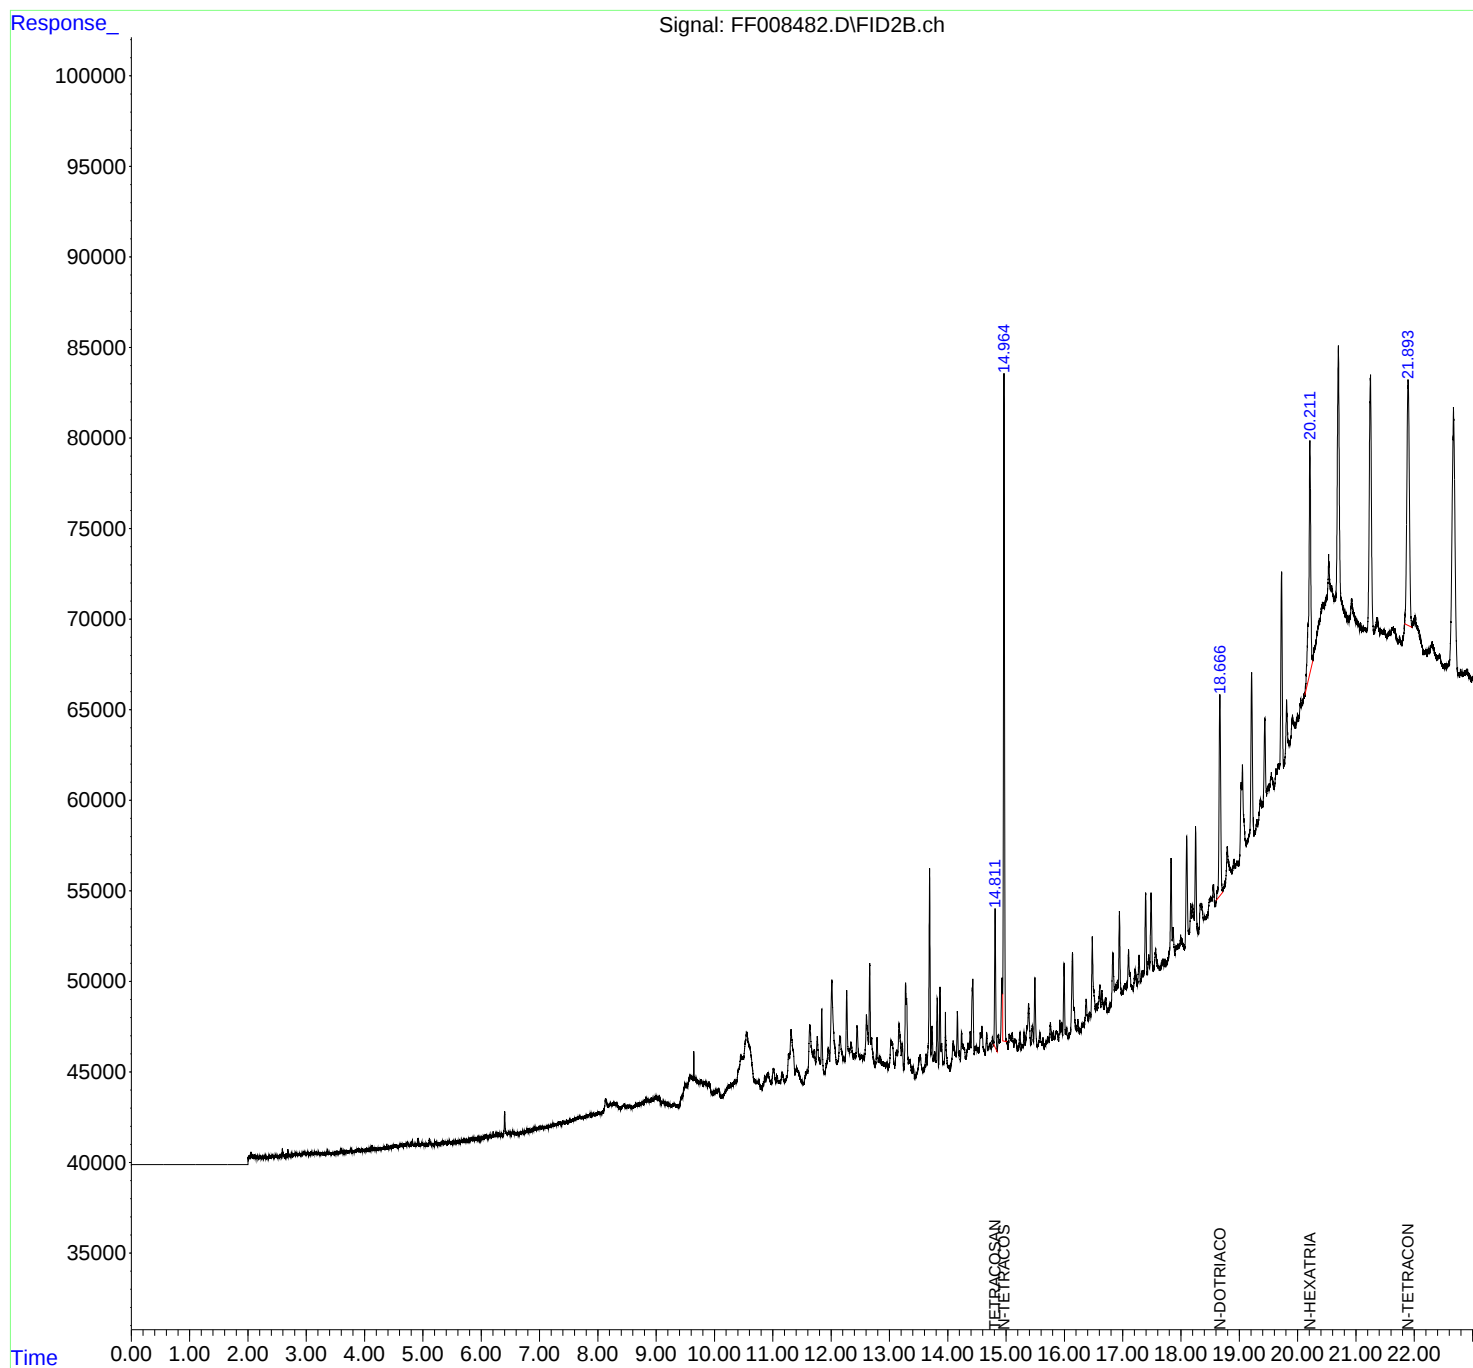


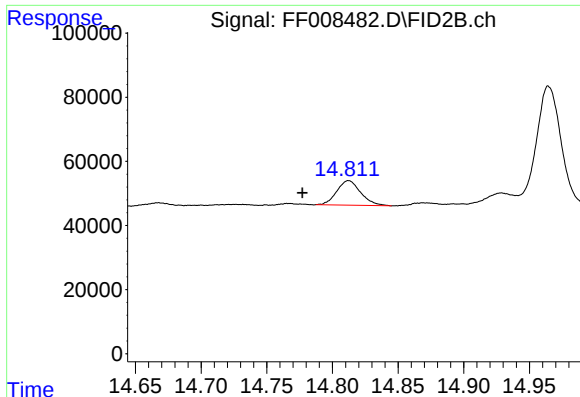

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.812 min
Delta R.T.: 0.035 min
Response: 96830
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

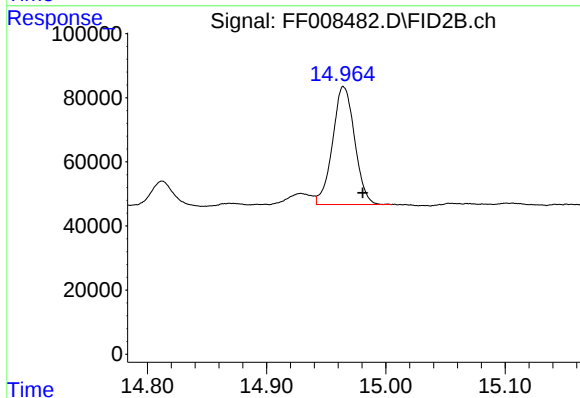


#10 N-TETRACOSANE

R.T.: 14.964 min
Delta R.T.: -0.016 min
Response: 473506
Conc: 3.32 ug/ml

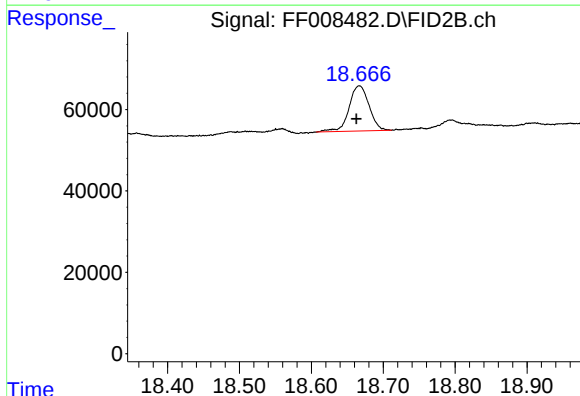


#14 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.004 min
Response: 214256
Conc: 1.58 ug/ml

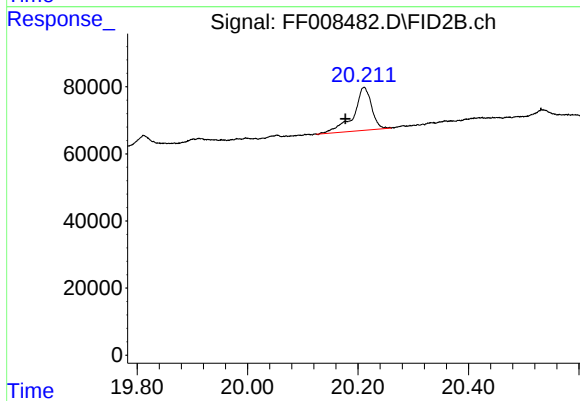

#16 N-HEXATRIACONTANE

R.T.: 20.211 min
Delta R.T.: 0.034 min
Response: 290023
Conc: 2.43 ug/ml

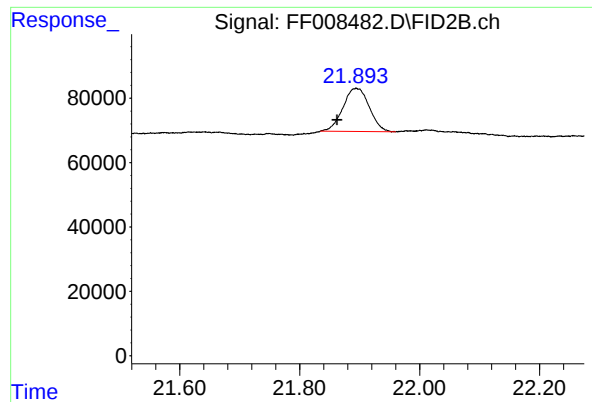

#18 N-TETRACONTANE

R.T.: 21.894 min
Delta R.T.: 0.032 min
Response: 408771
Conc: 3.60 ug/ml

Instrument :
FID_F
ClientSampleId :