

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008487.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 10:55
Operator : DD\AJ
Sample : M2589-13 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:20:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.776	84270	0.675 ug/ml
Target Compounds			
7) N-EICOSANE	12.748f	695478	4.896 ug/ml
10) N-TETRACOSANE	14.972	330414	2.317 ug/ml
13) N-TRIACONTANE	17.835	141982	1.025 ug/ml
14) N-DOTRIACONTANE	18.663	106820	0.788 ug/ml
16) N-HEXATRIACONTANE	20.178	59284	0.497 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008487.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 10:55
Operator : DD\AJ
Sample : M2589-13 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 05 00:20:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

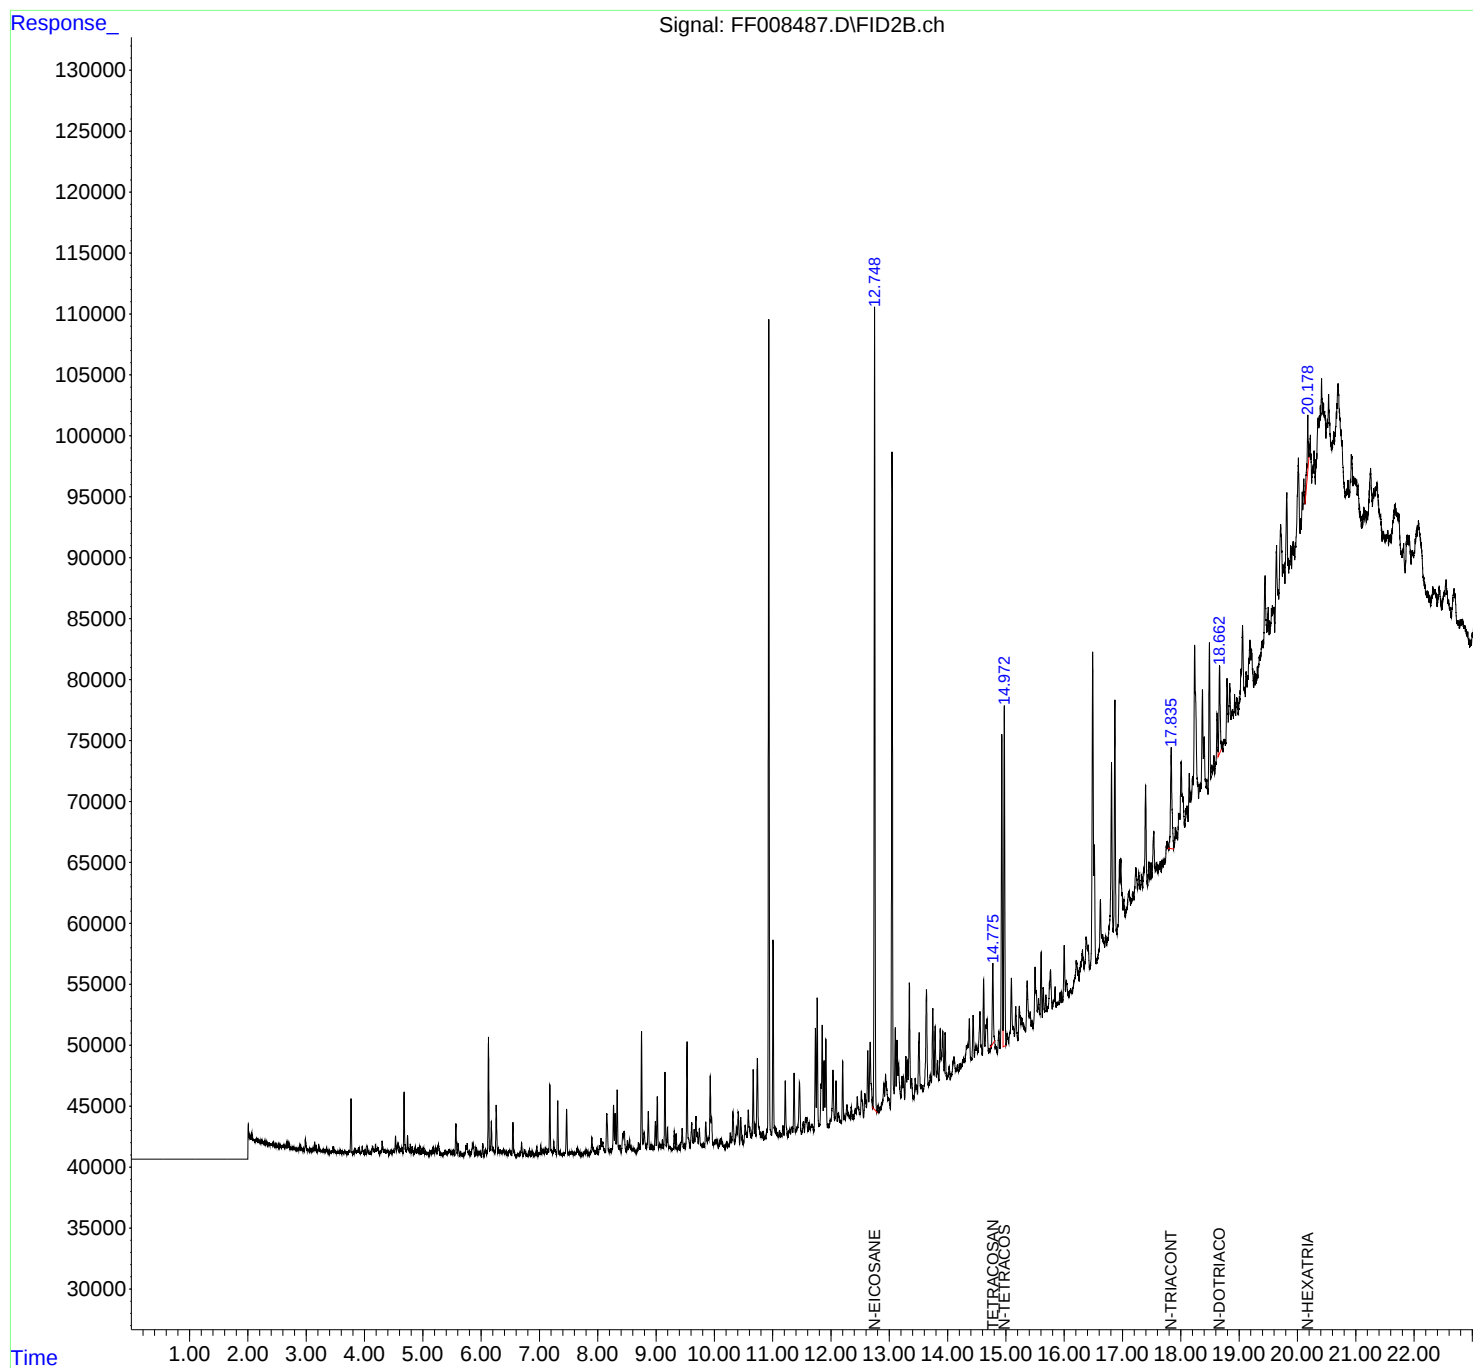


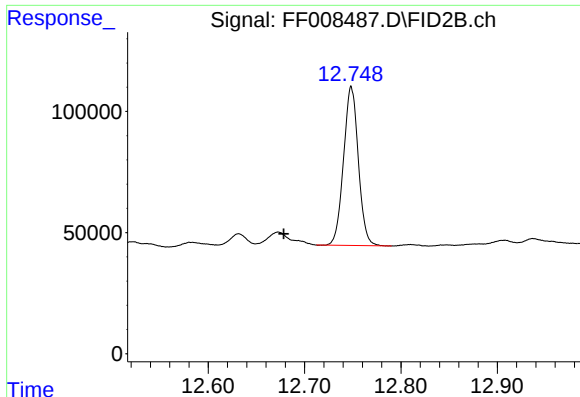

#7 N-EICOSANE


R.T.: 12.748 min
Delta R.T.: 0.070 min
Response: 695478
Conc: 4.90 ug/ml

Instrument :
FID_F
ClientSampleId :

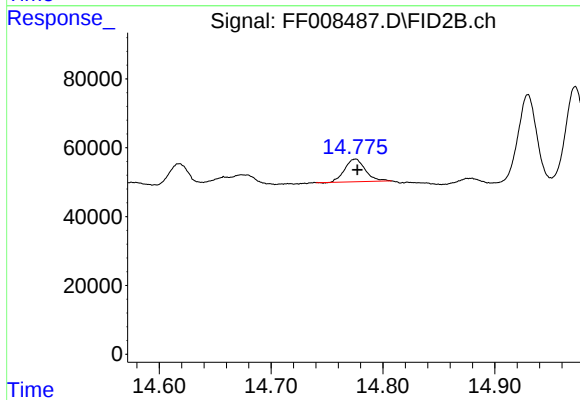


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.776 min
Delta R.T.: -0.001 min
Response: 84270
Conc: 0.67 ug/ml

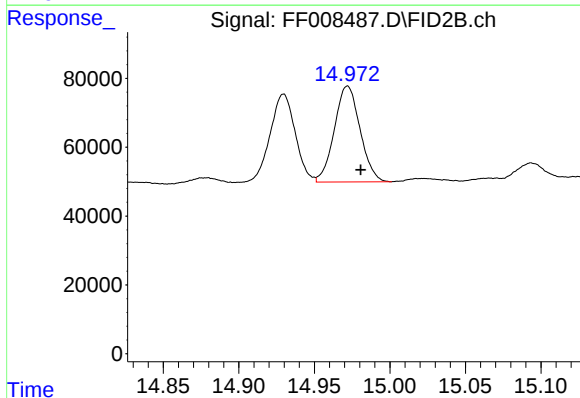


#10 N-TETRACOSANE

R.T.: 14.972 min
Delta R.T.: -0.009 min
Response: 330414
Conc: 2.32 ug/ml

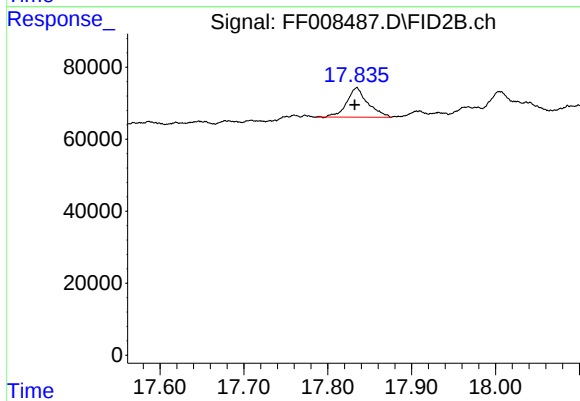

#13 N-TRIACONTANE


R.T.: 17.835 min
Delta R.T.: 0.003 min
Response: 141982
Conc: 1.02 ug/ml

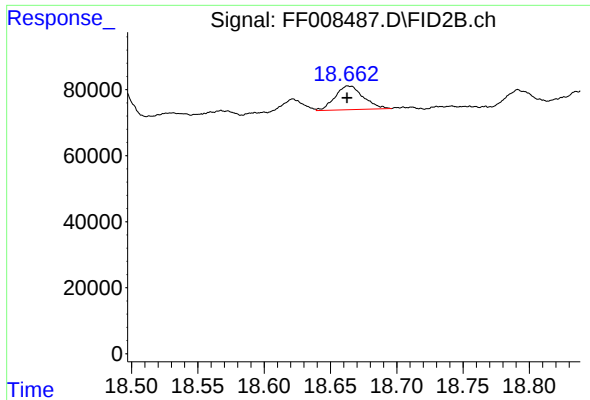

#14 N-DOTRIACONTANE

R.T.: 18.663 min
Delta R.T.: 0.000 min
Response: 106820
Conc: 0.79 ug/ml

Instrument :
FID_F
ClientSampleId :

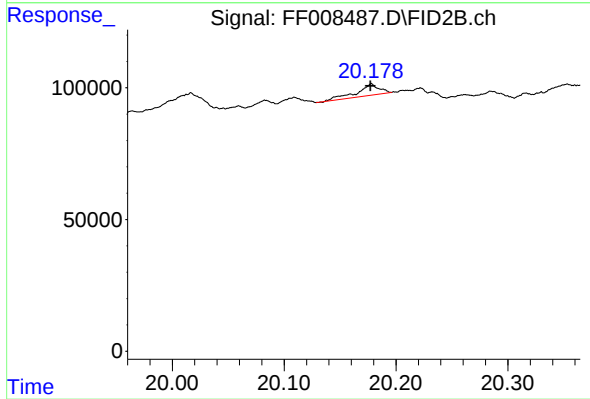

#16 N-HEXATRIACONTANE

R.T.: 20.178 min
Delta R.T.: 0.001 min
Response: 59284
Conc: 0.50 ug/ml