

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008489.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 11:58
 Operator : DD\AJ
 Sample : M2589-15 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:21:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.973	259957	1.823 ug/ml
13)	N-TRIACONTANE	17.835	169396	1.223 ug/ml
16)	N-HEXATRIACONTANE	20.214	736542	6.170 ug/ml
18)	N-TETRACONTANE	21.898	555602	4.887 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008489.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 11:58
Operator : DD\AJ
Sample : M2589-15 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:21:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

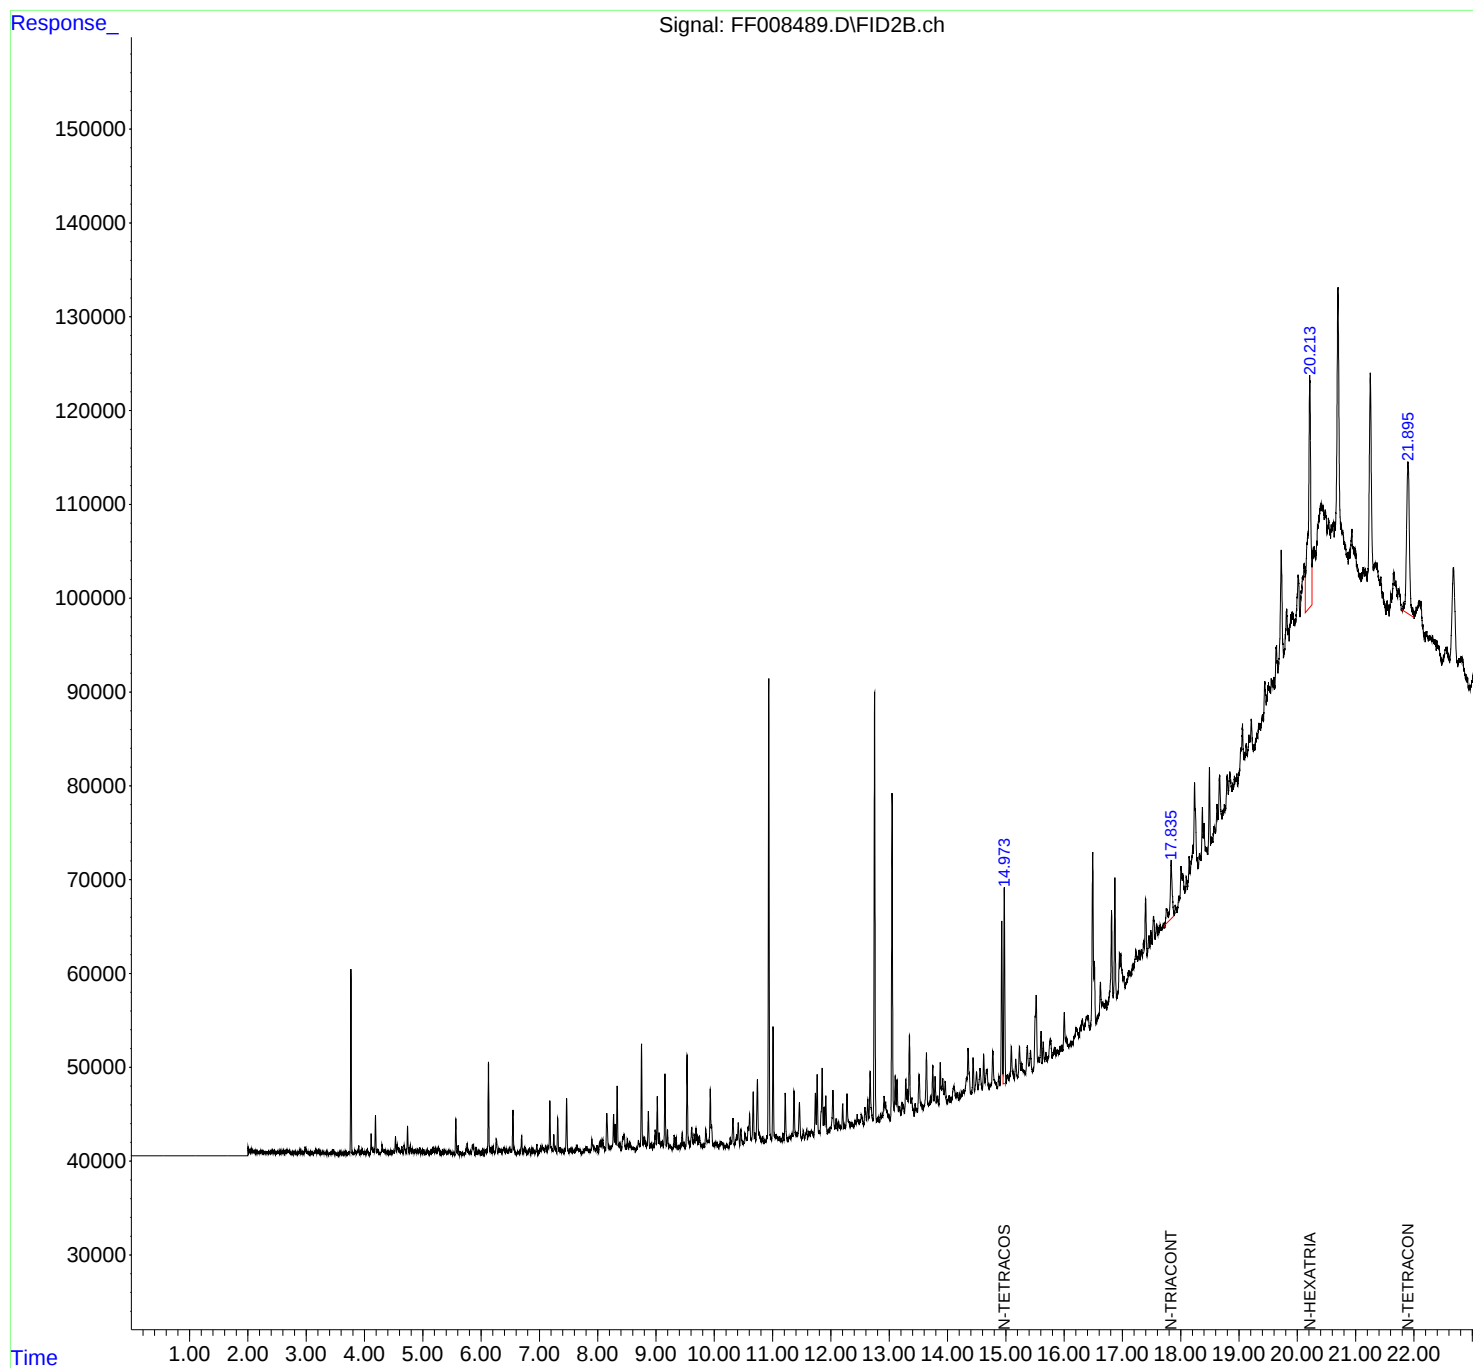


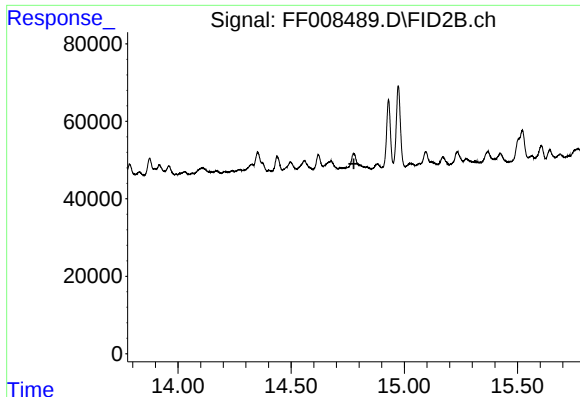

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

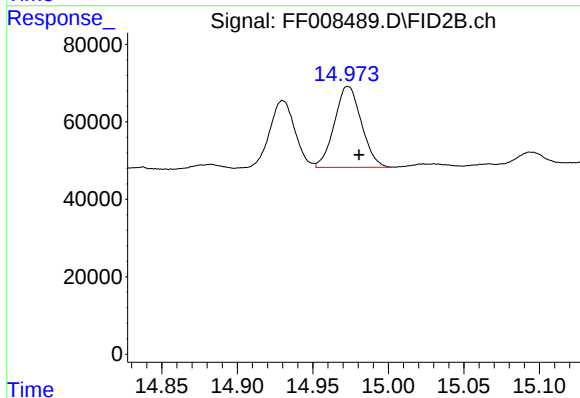


#10 N-TETRACOSANE

R.T.: 14.973 min
Delta R.T.: -0.007 min
Response: 259957
Conc: 1.82 ug/ml

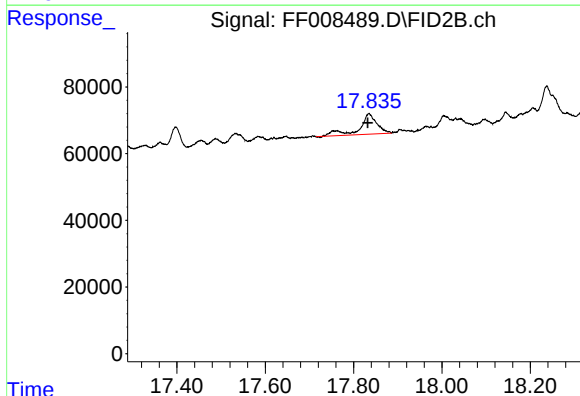


#13 N-TRIACONTANE

R.T.: 17.835 min
Delta R.T.: 0.002 min
Response: 169396
Conc: 1.22 ug/ml

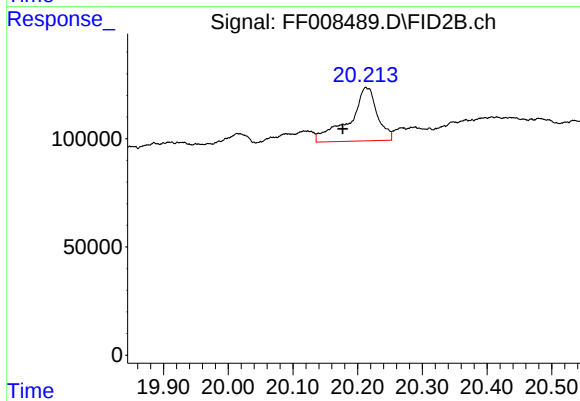

#16 N-HEXATRIACONTANE

R.T.: 20.214 min
Delta R.T.: 0.037 min
Response: 736542
Conc: 6.17 ug/ml

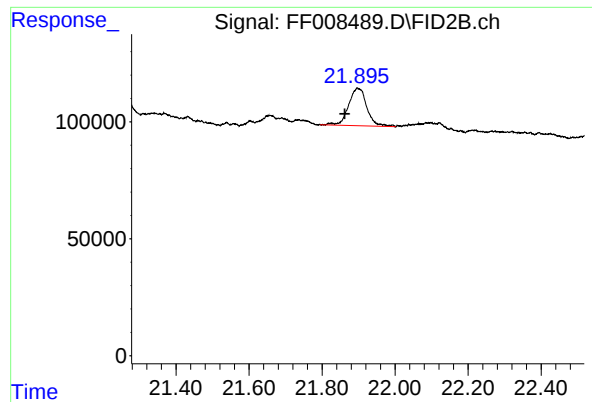

#18 N-TETRACONTANE

R.T.: 21.898 min
Delta R.T.: 0.035 min
Response: 555602
Conc: 4.89 ug/ml

Instrument :
FID_F
ClientSampleId :