

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008490.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 12:29
 Operator : DD\AJ
 Sample : M2589-16 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:21:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.546	66903	0.489 ug/ml
4) N-TETRADECANE	8.334	111624	0.799 ug/ml
7) N-EICOSANE	12.631	109480	0.771 ug/ml
8) N-DOCOSANE	13.878	120731	0.848 ug/ml
10) N-TETRACOSANE	14.978	1015525	7.121 ug/ml
11) N-HEXACOSANE	16.003	96906	0.687 ug/ml
12) N-OCTACOSANE	16.949	109510	0.780 ug/ml
13) N-TRIACONTANE	17.836	318523	2.299 ug/ml
14) N-DOTRIACONTANE	18.626	155623	1.149 ug/ml
16) N-HEXATRIACONTANE	20.166	92283	0.773 ug/ml
18) N-TETRACONTANE	21.897	445184	3.916 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008490.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 12:29
Operator : DD\AJ
Sample : M2589-16 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:21:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

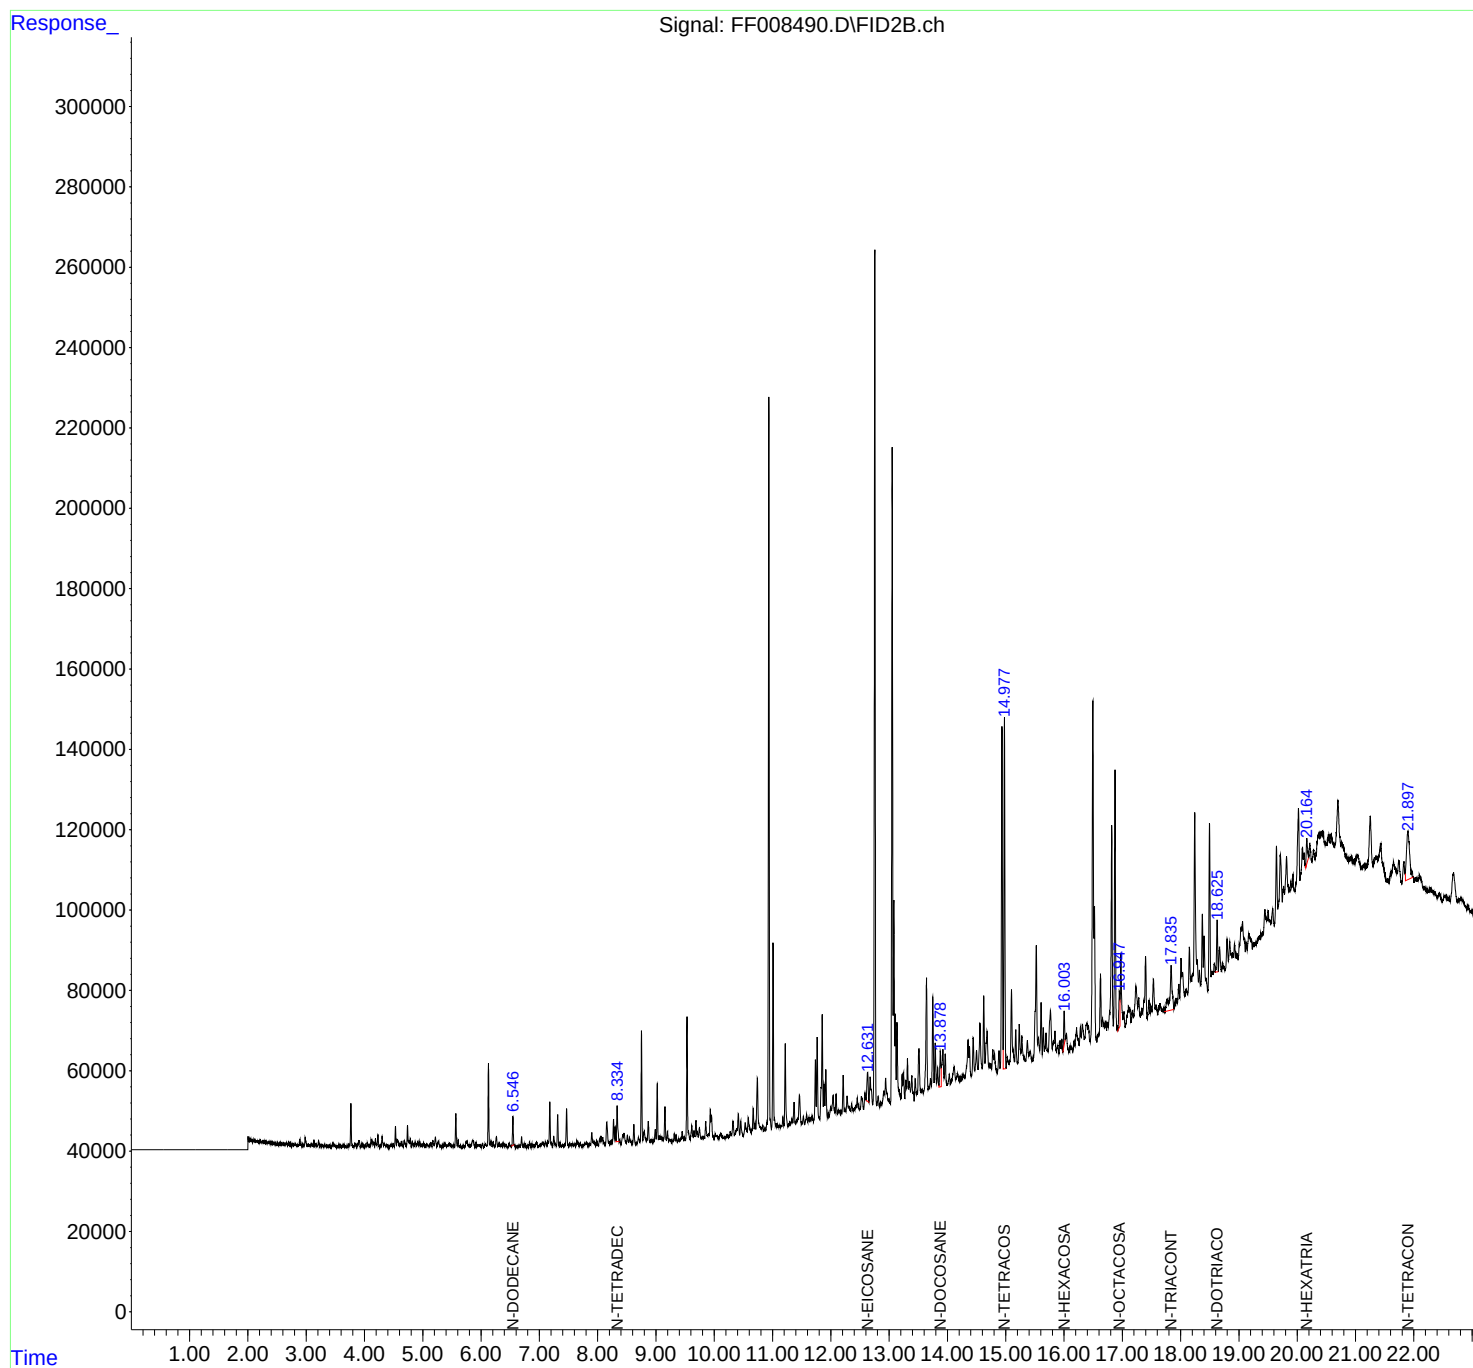


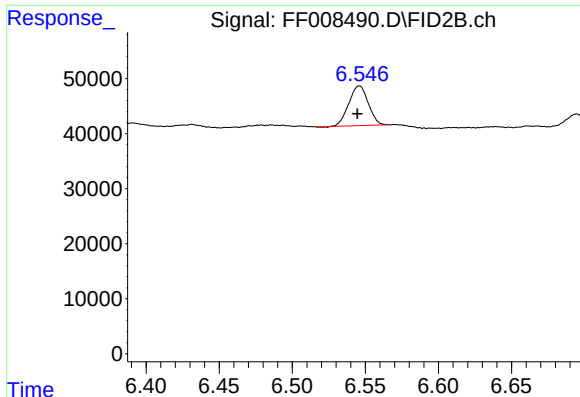

#3 N-DODECANE


R.T.: 6.546 min
Delta R.T.: 0.002 min
Response: 66903
Conc: 0.49 ug/ml

Instrument :
FID_F
ClientSampleId :

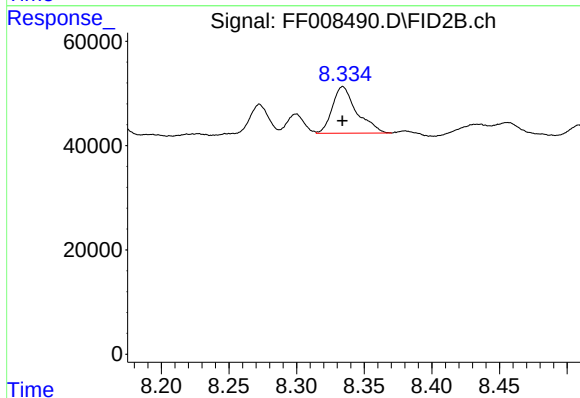


#4 N-TETRADECANE

R.T.: 8.334 min
Delta R.T.: 0.000 min
Response: 111624
Conc: 0.80 ug/ml

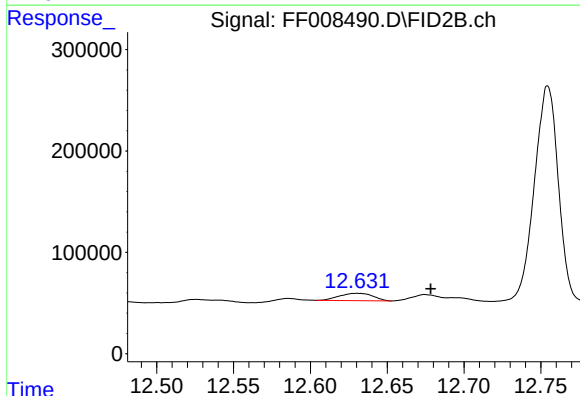


#7 N-EICOSANE

R.T.: 12.631 min
Delta R.T.: -0.047 min
Response: 109480
Conc: 0.77 ug/ml

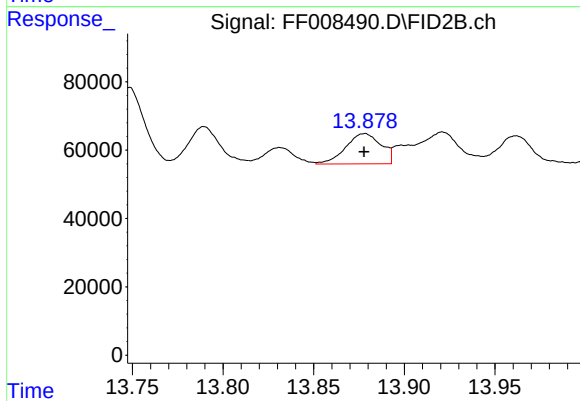

#8 N-DOCOSANE


R.T.: 13.878 min
Delta R.T.: 0.000 min
Response: 120731
Conc: 0.85 ug/ml

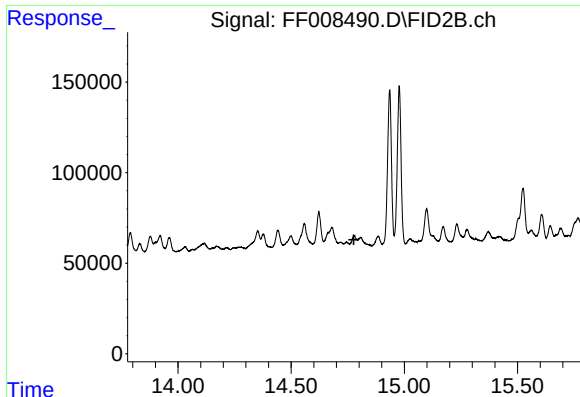

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

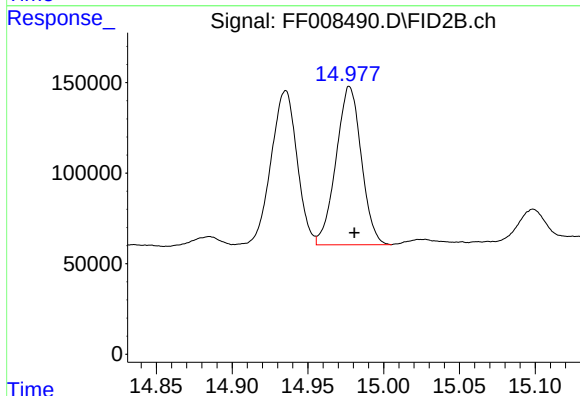


#10 N-TETRACOSANE

R.T.: 14.978 min
Delta R.T.: -0.003 min
Response: 1015525
Conc: 7.12 ug/ml

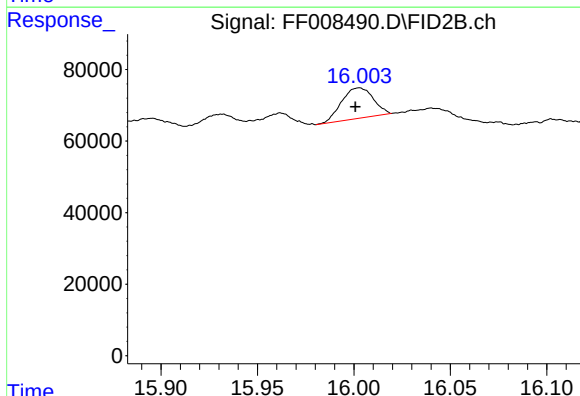


#11 N-HEXACOSANE

R.T.: 16.003 min
Delta R.T.: 0.002 min
Response: 96906
Conc: 0.69 ug/ml

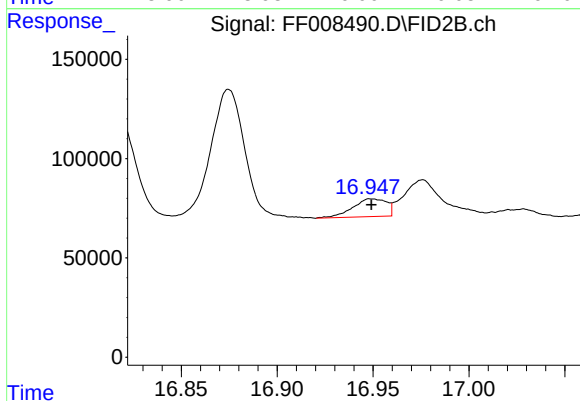

#12 N-OCTACOSANE


R.T.: 16.949 min
Delta R.T.: 0.000 min
Response: 109510
Conc: 0.78 ug/ml

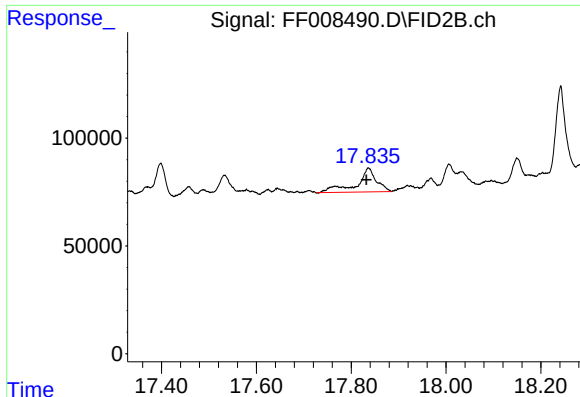

#13 N-TRIACONTANE


R.T.: 17.836 min
Delta R.T.: 0.004 min
Response: 318523
Conc: 2.30 ug/ml

Instrument :
FID_F
ClientSampleId :

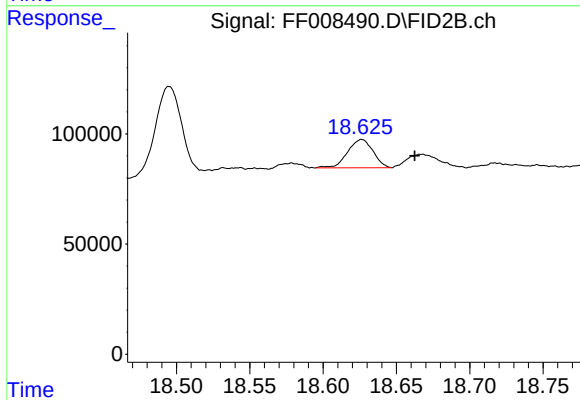


#14 N-DOTRIACONTANE

R.T.: 18.626 min
Delta R.T.: -0.036 min
Response: 155623
Conc: 1.15 ug/ml

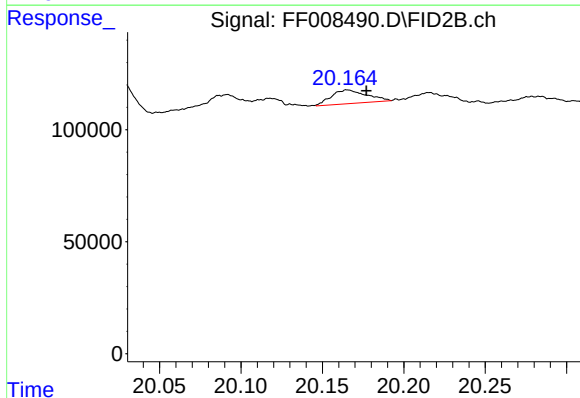

#16 N-HEXATRIACONTANE

R.T.: 20.166 min
Delta R.T.: -0.011 min
Response: 92283
Conc: 0.77 ug/ml

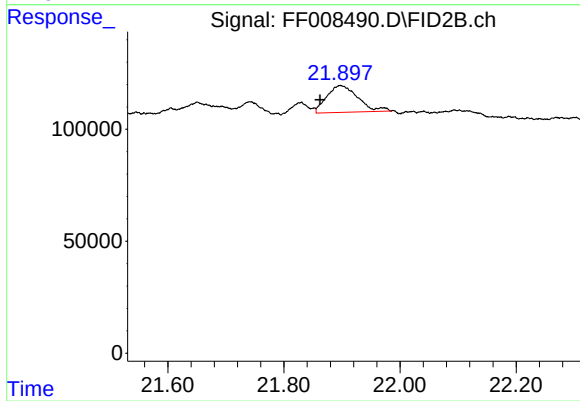

#18 N-TETRACONTANE

R.T.: 21.897 min
Delta R.T.: 0.035 min
Response: 445184
Conc: 3.92 ug/ml