

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008491.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 13:00
 Operator : DD\AJ
 Sample : M2589-17 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:21:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.635	71402	0.503 ug/ml
10)	N-TETRACOSANE	14.974	612896	4.297 ug/ml
12)	N-OCTACOSANE	16.976	143159	1.020 ug/ml
13)	N-TRIACONTANE	17.837	269739	1.947 ug/ml
14)	N-DOTRIACONTANE	18.628	87438	0.645 ug/ml
15)	N-TETRATRIACONTANE	19.446	121630	0.954 ug/ml
16)	N-HEXATRIACONTANE	20.171	82855	0.694 ug/ml
18)	N-TETRACONTANE	21.891	227043	1.997 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008491.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 13:00
Operator : DD\AJ
Sample : M2589-17 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:21:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

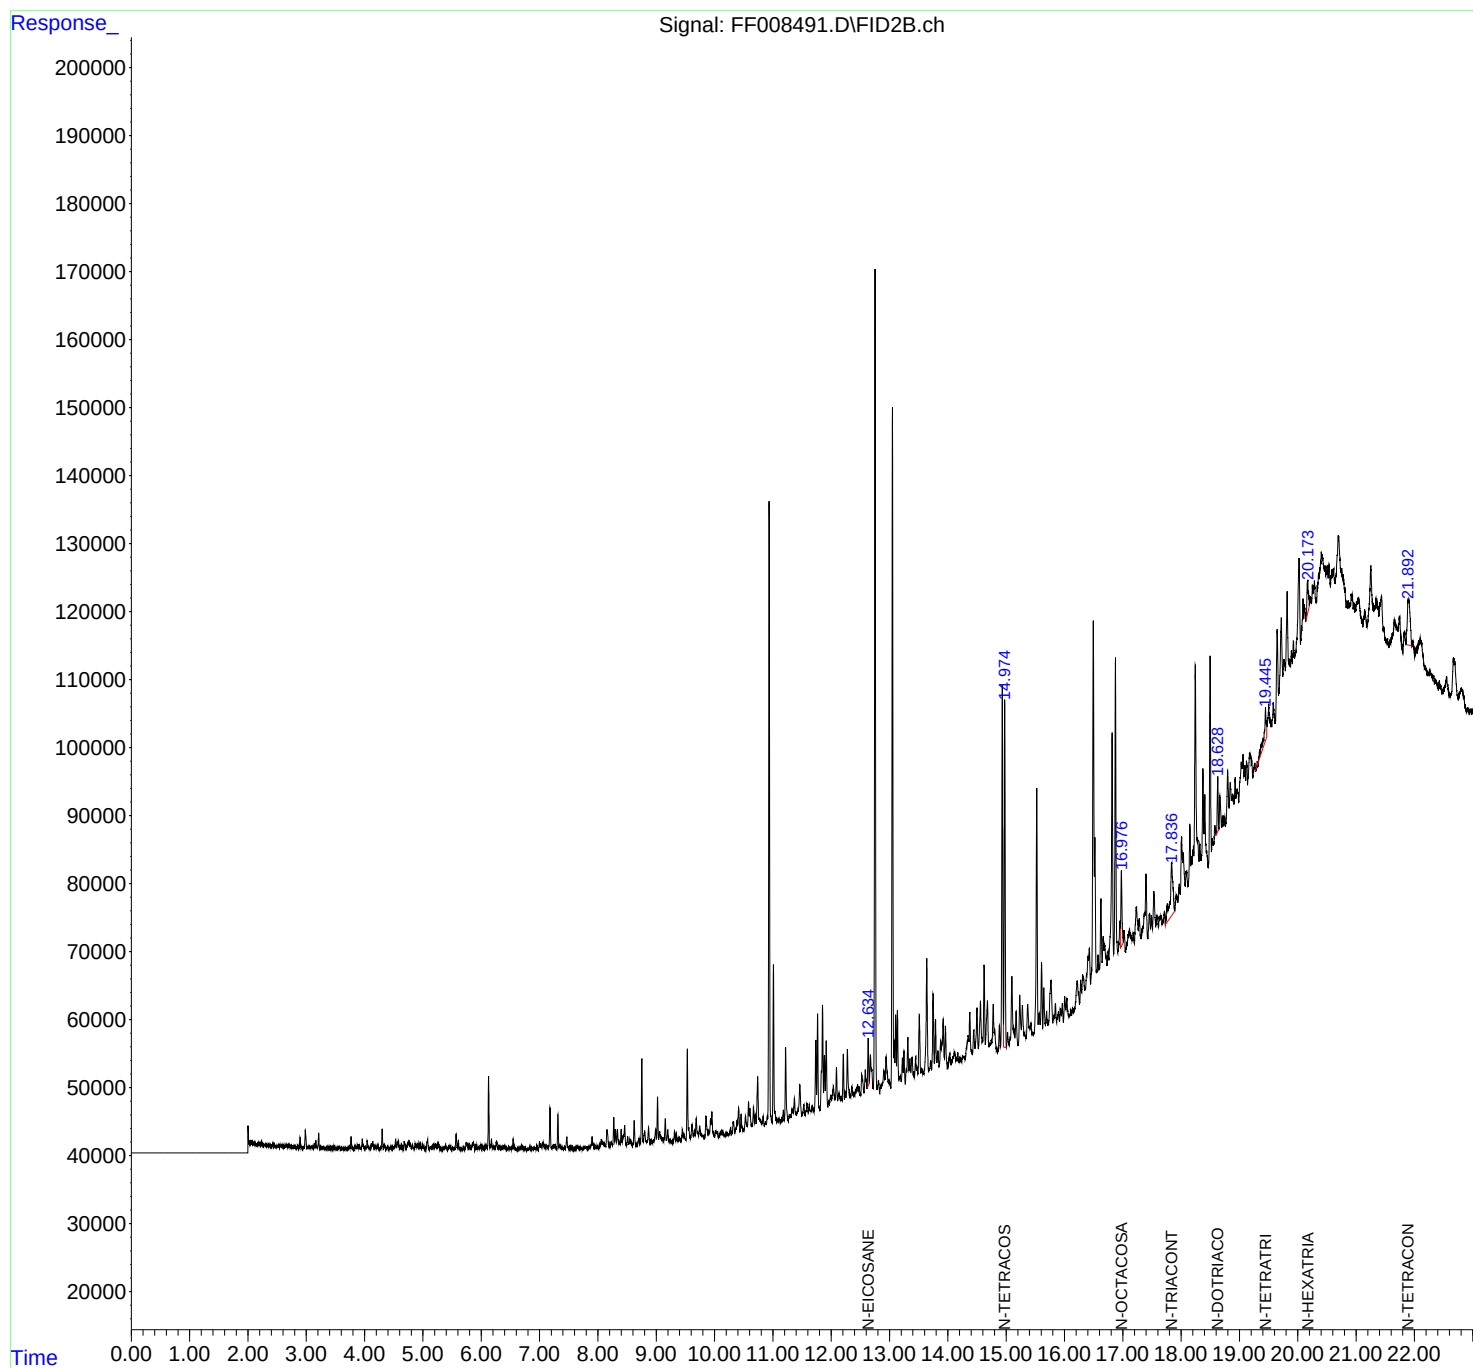


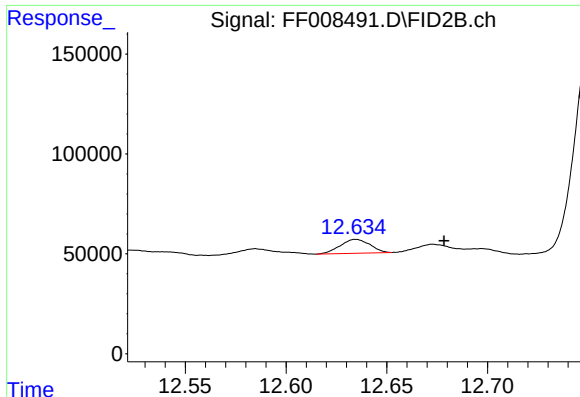

#7 N-EICOSANE


R.T.: 12.635 min
Delta R.T.: -0.044 min
Response: 71402
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

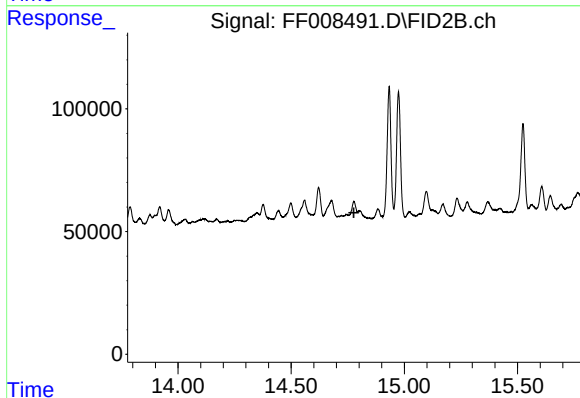


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

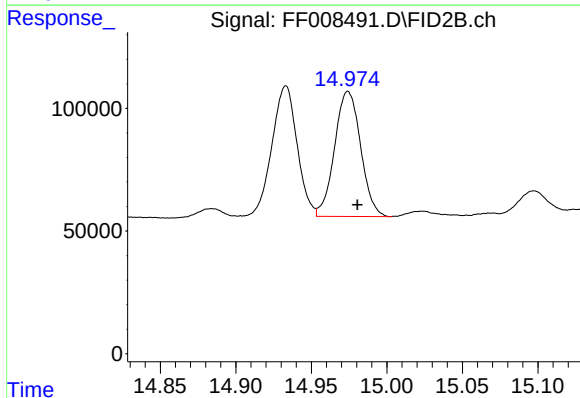


#10 N-TETRACOSANE

R.T.: 14.974 min
Delta R.T.: -0.006 min
Response: 612896
Conc: 4.30 ug/ml

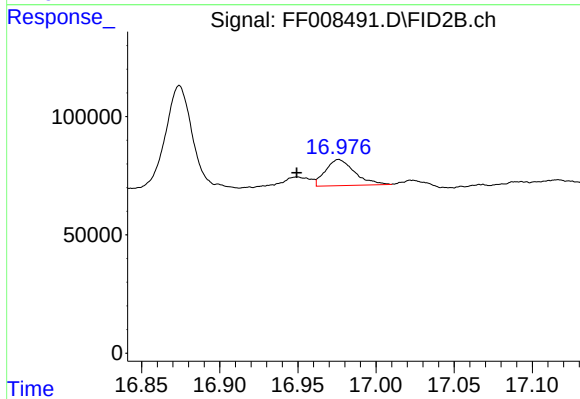

#12 N-OCTACOSANE


R.T.: 16.976 min
Delta R.T.: 0.027 min
Response: 143159
Conc: 1.02 ug/ml

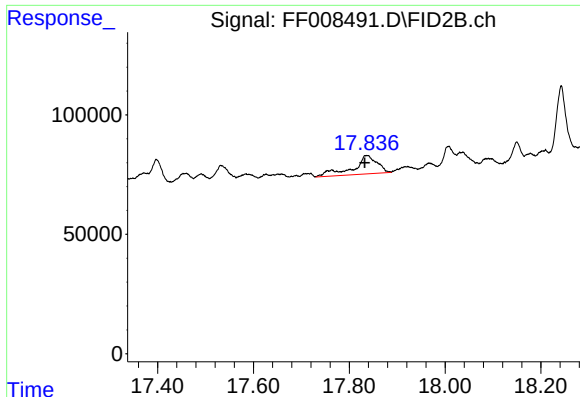

#13 N-TRIACONTANE


R.T.: 17.837 min
Delta R.T.: 0.005 min
Response: 269739
Conc: 1.95 ug/ml

Instrument :
FID_F
ClientSampleId :

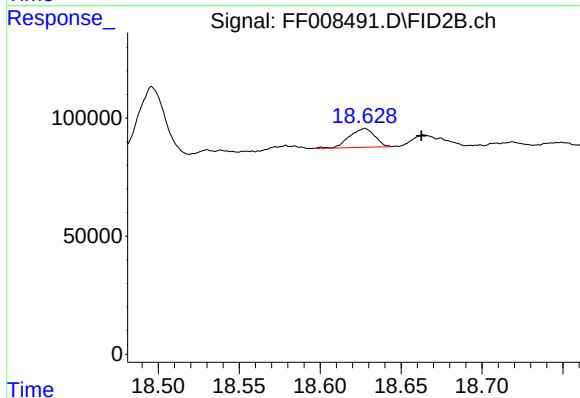


#14 N-DOTRIACONTANE

R.T.: 18.628 min
Delta R.T.: -0.035 min
Response: 87438
Conc: 0.65 ug/ml

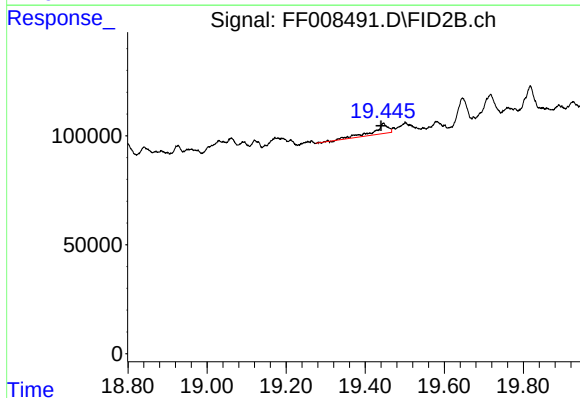


#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: 0.006 min
Response: 121630
Conc: 0.95 ug/ml

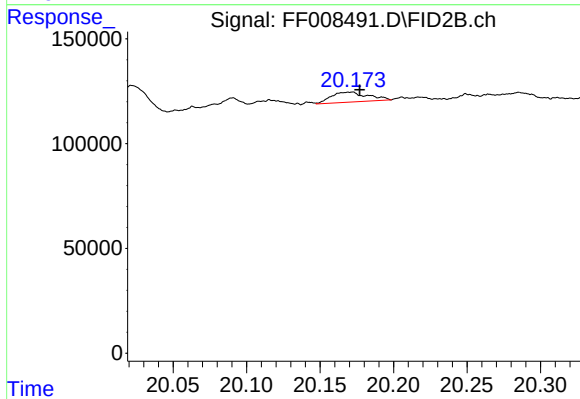

#16 N-HEXATRIACONTANE

R.T.: 20.171 min
Delta R.T.: -0.006 min
Response: 82855
Conc: 0.69 ug/ml

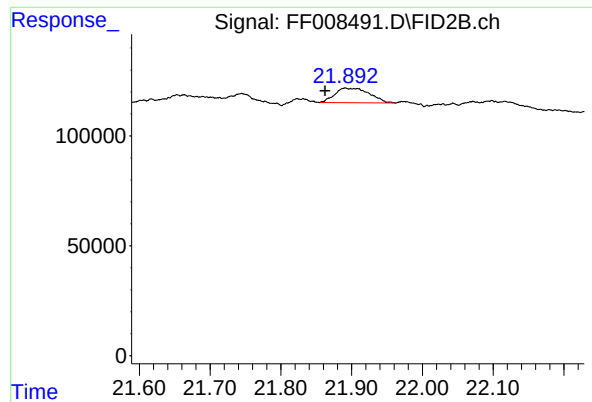

#18 N-TETRACONTANE

R.T.: 21.891 min
Delta R.T.: 0.029 min
Response: 227043
Conc: 2.00 ug/ml

Instrument :
FID_F
ClientSampleId :