

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008492.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 13:32
Operator : DD\AJ
Sample : M2589-18 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:21:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10)	N-TETRACOSANE	14.976	92996	0.652 ug/ml
13)	N-TRIACONTANE	17.836	33314	0.240 ug/ml
14)	N-DOTRIACONTANE	18.671	141547	1.045 ug/ml
15)	N-TETRATRIACONTANE	19.450	24297	0.191 ug/ml
18)	N-TETRACONTANE	21.896	48433	0.426 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008492.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 13:32
Operator : DD\AJ
Sample : M2589-18 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:21:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

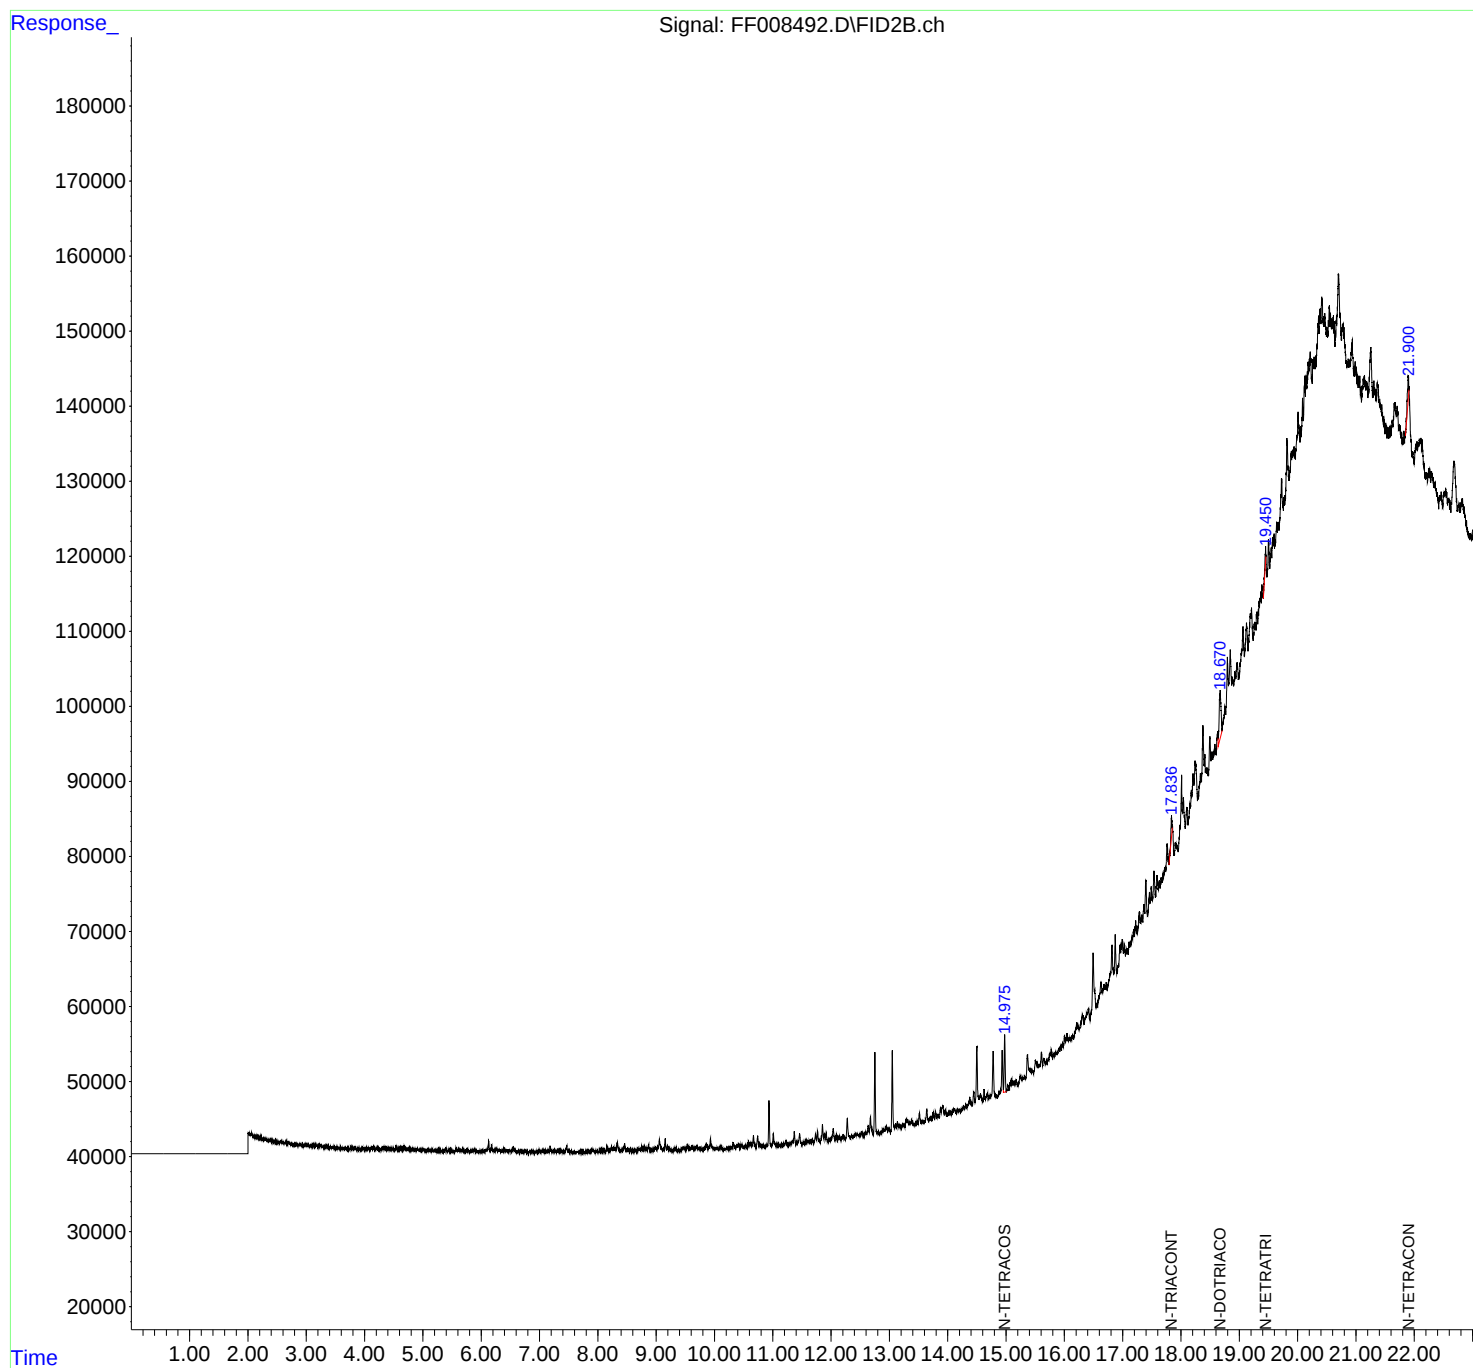


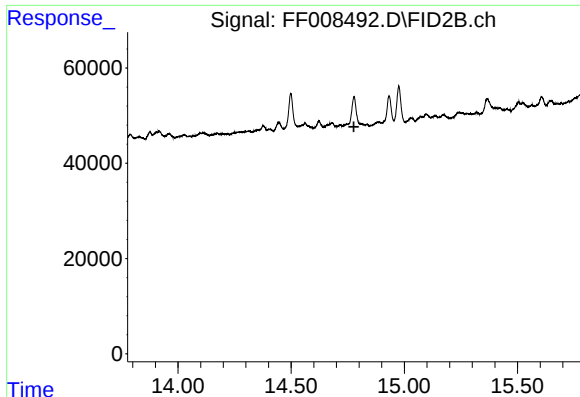

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

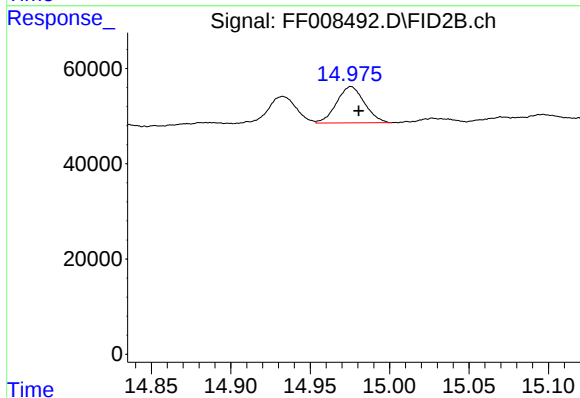


#10 N-TETRACOSANE

R.T.: 14.976 min
Delta R.T.: -0.005 min
Response: 92996
Conc: 0.65 ug/ml

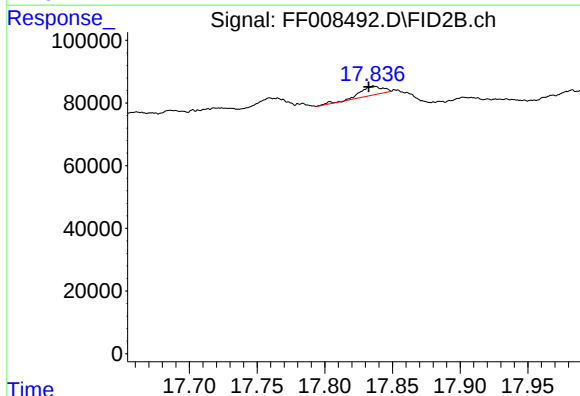


#13 N-TRIACONTANE

R.T.: 17.836 min
Delta R.T.: 0.004 min
Response: 33314
Conc: 0.24 ug/ml

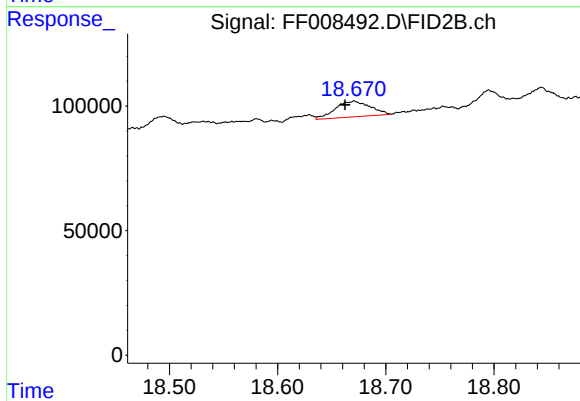

#14 N-DOTRIACONTANE


R.T.: 18.671 min
Delta R.T.: 0.008 min
Response: 141547
Conc: 1.04 ug/ml

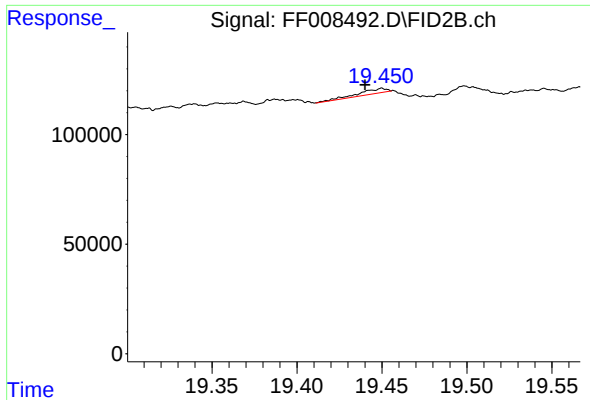

#15 N-TETRATRIACONTANE

R.T.: 19.450 min
Delta R.T.: 0.010 min
Response: 24297
Conc: 0.19 ug/ml

Instrument :
FID_F
ClientSampleId :

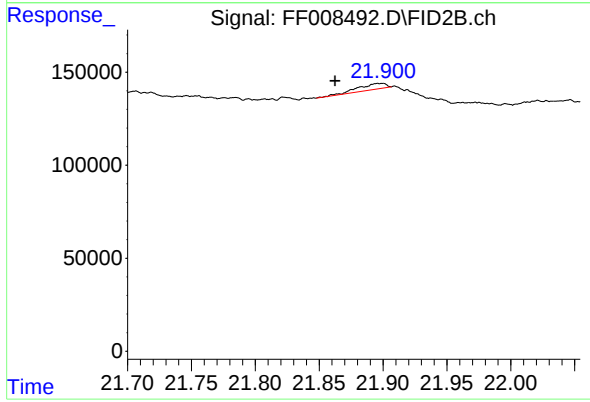

#18 N-TETRACONTANE

R.T.: 21.896 min
Delta R.T.: 0.034 min
Response: 48433
Conc: 0.43 ug/ml