

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008496.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 16:09
 Operator : DD\AJ
 Sample : M2589-12 30X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:22:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	69770	0.559 ug/ml
Target Compounds			
4) N-TETRADECANE	8.335	94298	0.675 ug/ml
5) N-HEXADECANE	9.931	55276	0.396 ug/ml
6) N-OCTADECANE	11.370	102230	0.717 ug/ml
7) N-EICOSANE	12.675	193828	1.364 ug/ml
8) N-DOCOSANE	13.877	130727	0.918 ug/ml
10) N-TETRACOSANE	14.978	1007983	7.068 ug/ml
11) N-HEXACOSANE	16.007	63986	0.454 ug/ml
12) N-OCTACOSANE	16.952	122088	0.870 ug/ml
13) N-TRIACONTANE	17.838	288258	2.080 ug/ml
14) N-DOTRIACONTANE	18.668	152407	1.125 ug/ml
15) N-TETRATRIACONTANE	19.449	201515	1.580 ug/ml
16) N-HEXATRIACONTANE	20.180	168361	1.410 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008496.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 16:09
Operator : DD\AJ
Sample : M2589-12 30X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:22:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

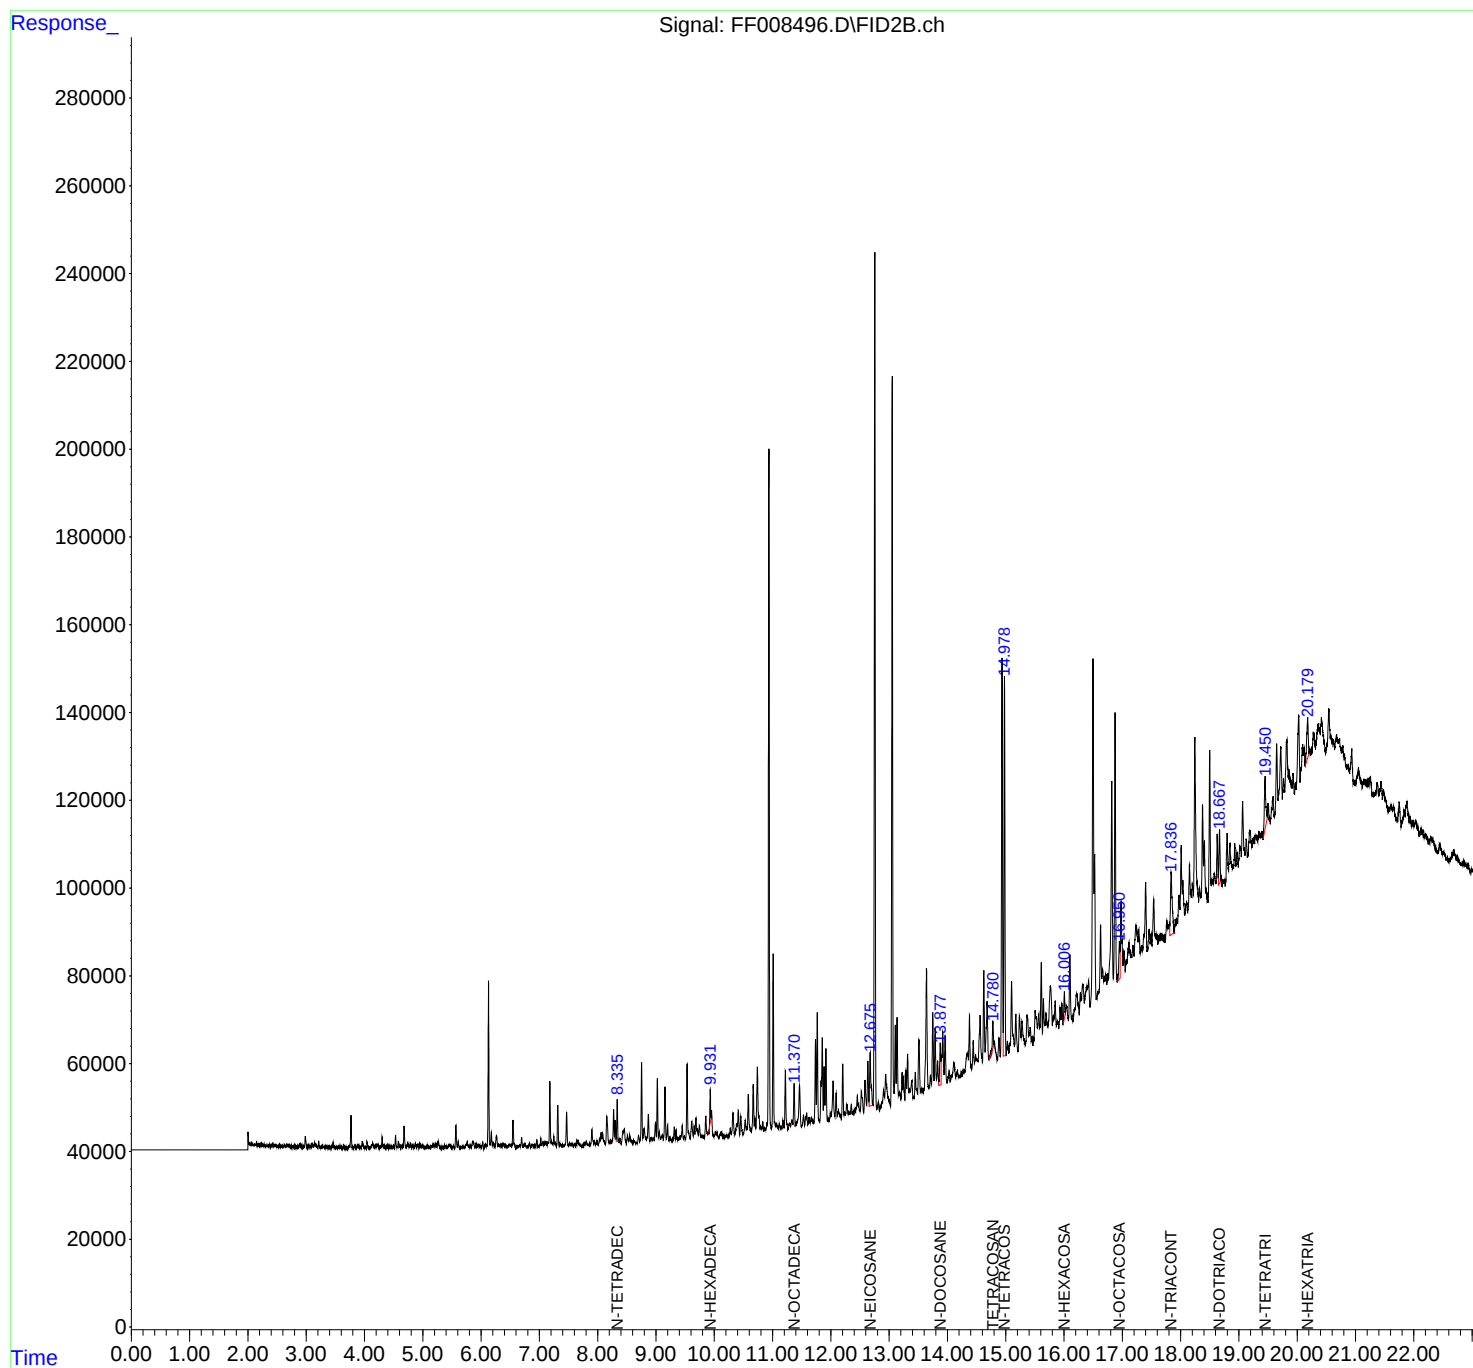


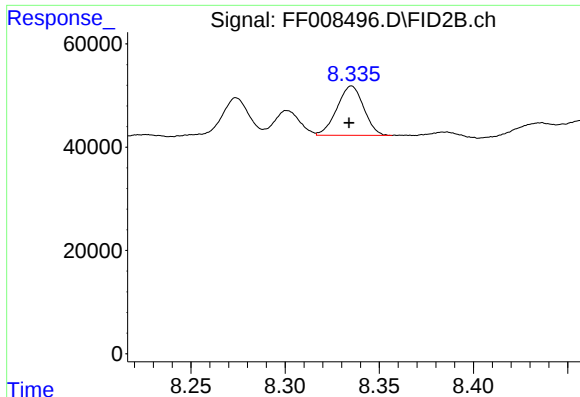

#4 N-TETRADECANE


R.T.: 8.335 min
Delta R.T.: 0.002 min
Response: 94298
Conc: 0.67 ug/ml

Instrument :
FID_F
ClientSampleId :

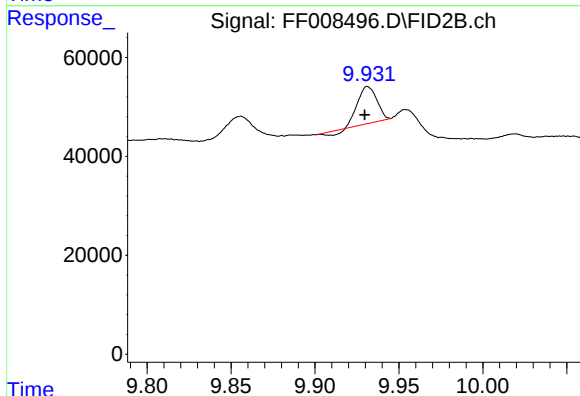


#5 N-HEXADECANE

R.T.: 9.931 min
Delta R.T.: 0.002 min
Response: 55276
Conc: 0.40 ug/ml

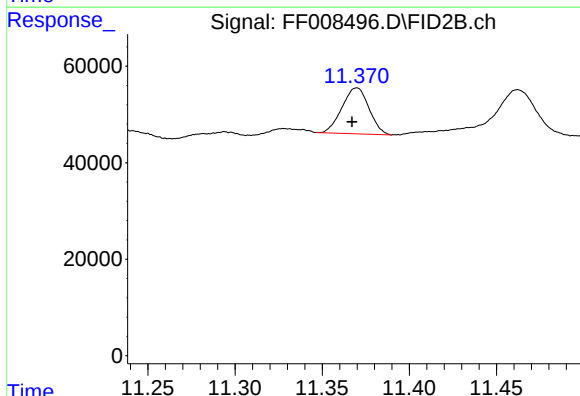


#6 N-OCTADECANE

R.T.: 11.370 min
Delta R.T.: 0.003 min
Response: 102230
Conc: 0.72 ug/ml

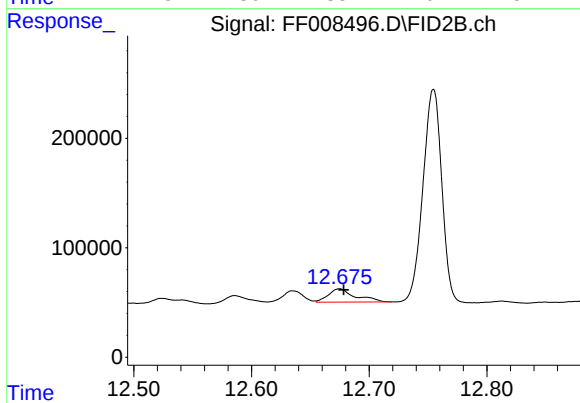

#7 N-EICOSANE


R.T.: 12.675 min
Delta R.T.: -0.004 min
Response: 193828
Conc: 1.36 ug/ml

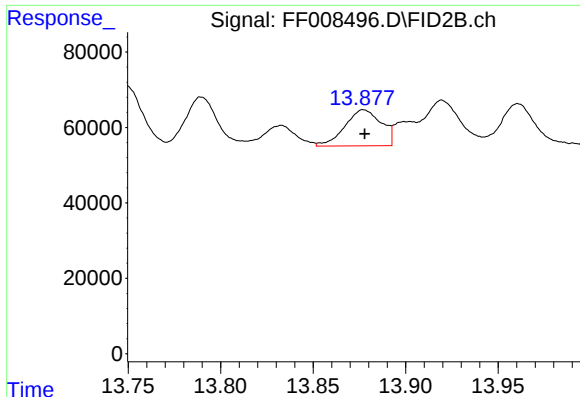

#8 N-DOCOSANE


R.T.: 13.877 min
Delta R.T.: 0.000 min
Response: 130727
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

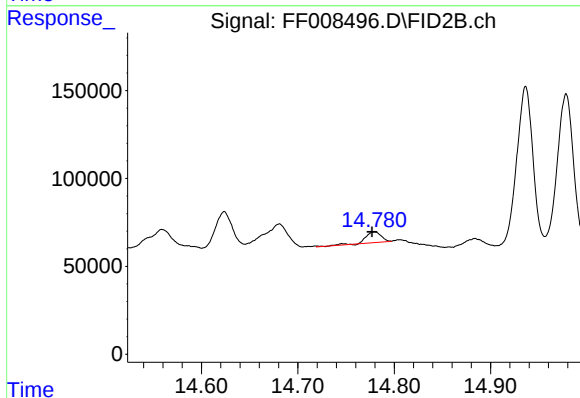


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.780 min
Delta R.T.: 0.003 min
Response: 69770
Conc: 0.56 ug/ml

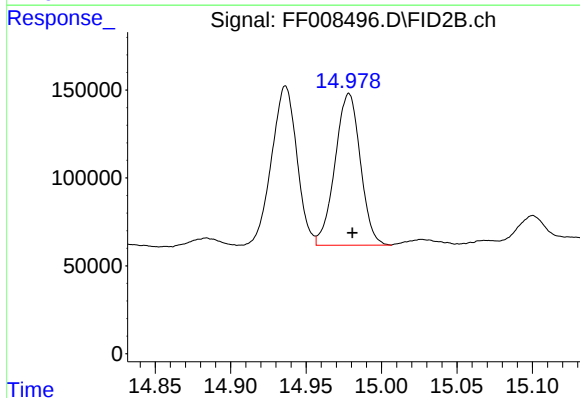


#10 N-TETRACOSANE

R.T.: 14.978 min
Delta R.T.: -0.002 min
Response: 1007983
Conc: 7.07 ug/ml

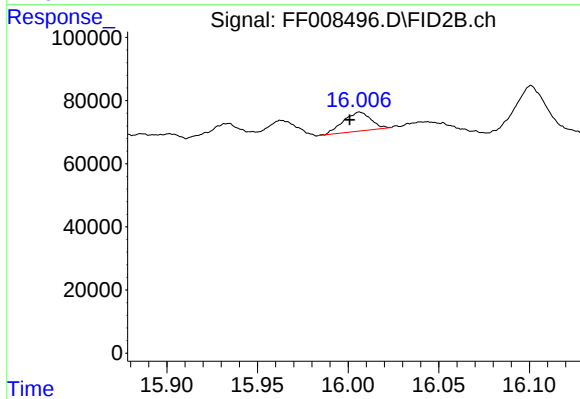

#11 N-HEXACOSANE


R.T.: 16.007 min
Delta R.T.: 0.006 min
Response: 63986
Conc: 0.45 ug/ml

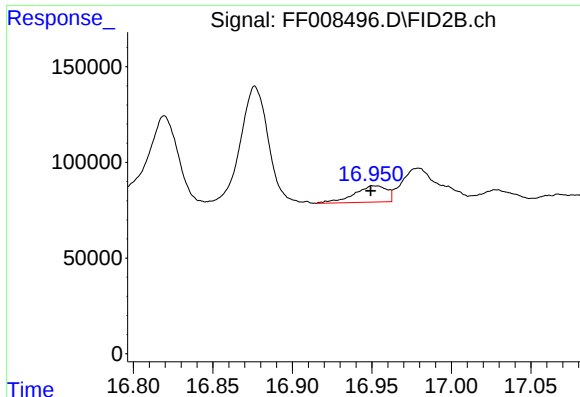

#12 N-OCTACOSANE


R.T.: 16.952 min
Delta R.T.: 0.002 min
Response: 122088
Conc: 0.87 ug/ml

Instrument :
FID_F
ClientSampleId :

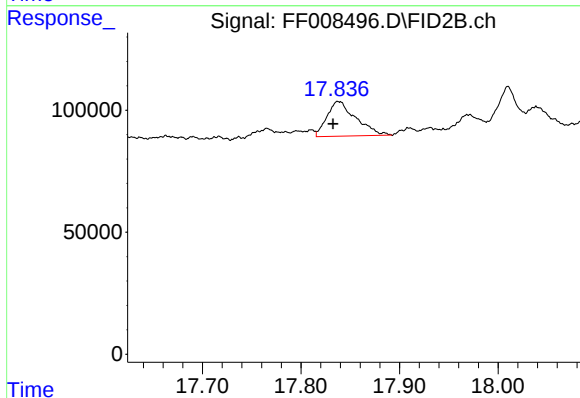


#13 N-TRIACONTANE

R.T.: 17.838 min
Delta R.T.: 0.005 min
Response: 288258
Conc: 2.08 ug/ml

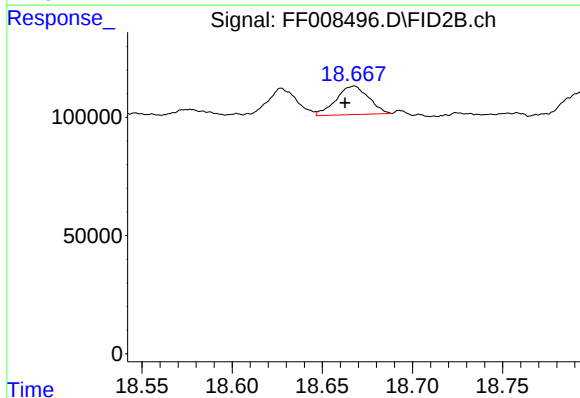


#14 N-DOTRIACONTANE

R.T.: 18.668 min
Delta R.T.: 0.005 min
Response: 152407
Conc: 1.12 ug/ml

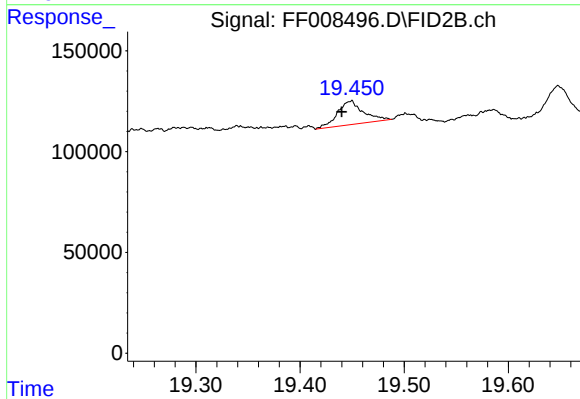

#15 N-TETRATRIACONTANE

R.T.: 19.449 min
Delta R.T.: 0.009 min
Response: 201515
Conc: 1.58 ug/ml

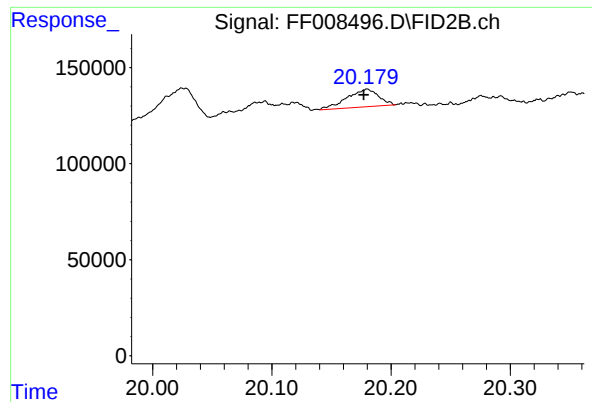

#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.003 min
Response: 168361
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :