

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008497.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 16:41
 Operator : DD\AJ
 Sample : M2589-16 20X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:22:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.547	72159	0.528 ug/ml
4)	N-TETRADECANE	8.336	115672	0.828 ug/ml
7)	N-EICOSANE	12.676	133545	0.940 ug/ml
8)	N-DOCOSANE	13.877	123824	0.870 ug/ml
10)	N-TETRACOSANE	14.978	1025086	7.188 ug/ml
11)	N-HEXACOSANE	16.004	102998	0.731 ug/ml
12)	N-OCTACOSANE	16.951	119983	0.855 ug/ml
13)	N-TRIACONTANE	17.837	292234	2.109 ug/ml
14)	N-DOTRIACONTANE	18.666	121114	0.894 ug/ml
16)	N-HEXATRIACONTANE	20.172	156089	1.308 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008497.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 16:41
Operator : DD\AJ
Sample : M2589-16 20X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:22:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

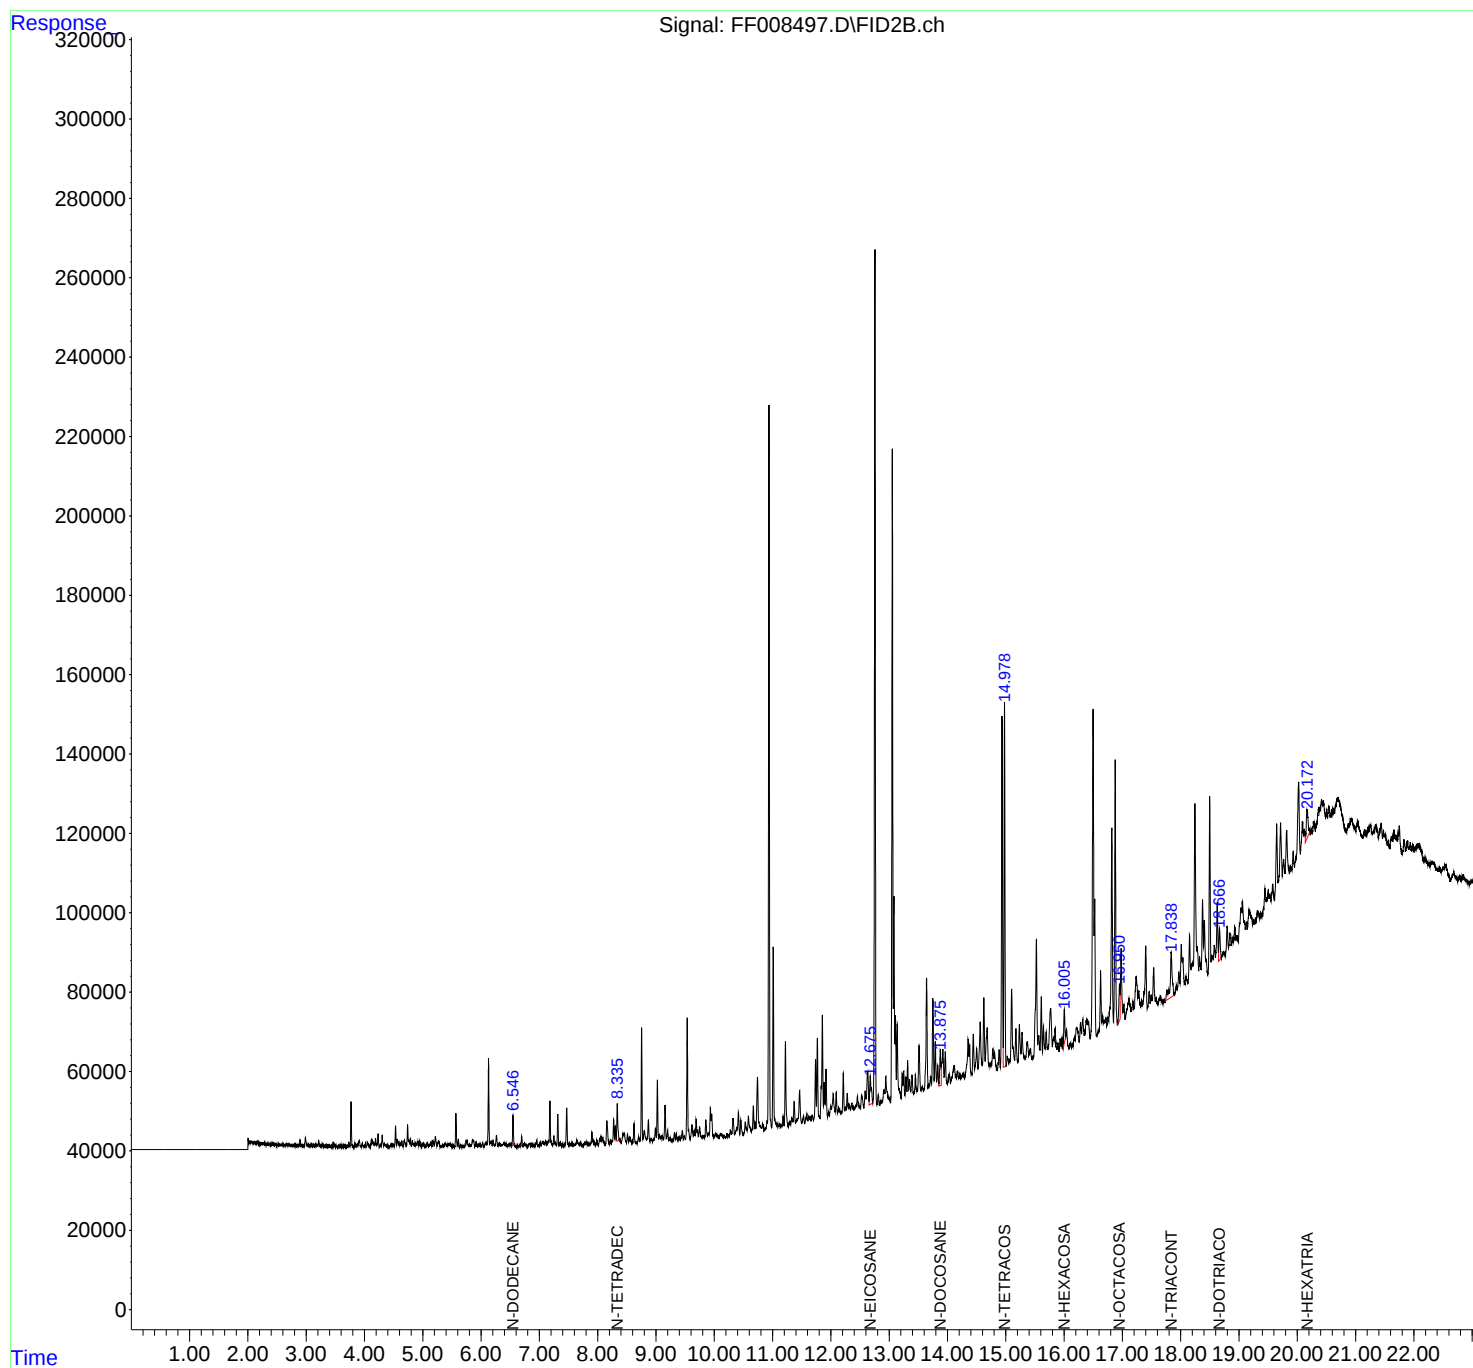


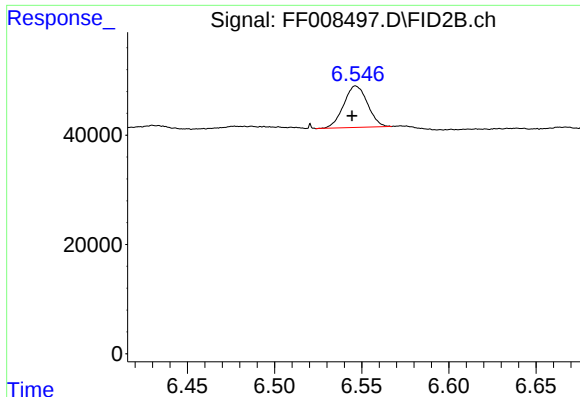

#3 N-DODECANE


R.T.: 6.547 min
Delta R.T.: 0.002 min
Response: 72159
Conc: 0.53 ug/ml

Instrument :
FID_F
ClientSampleId :

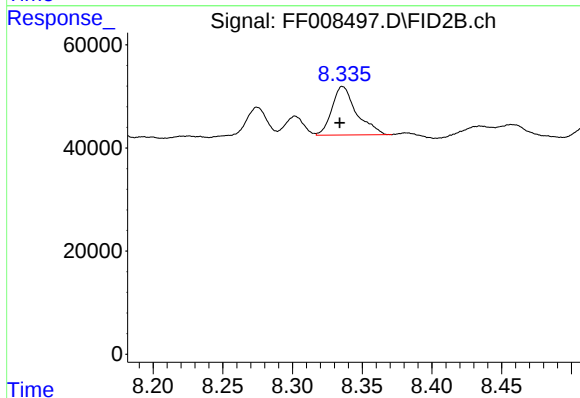


#4 N-TETRADECANE

R.T.: 8.336 min
Delta R.T.: 0.002 min
Response: 115672
Conc: 0.83 ug/ml

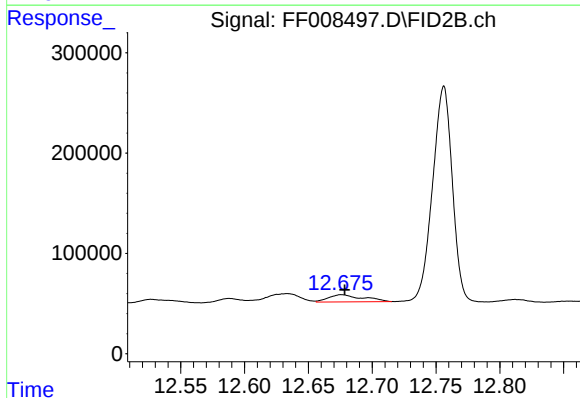


#7 N-EICOSANE

R.T.: 12.676 min
Delta R.T.: -0.002 min
Response: 133545
Conc: 0.94 ug/ml

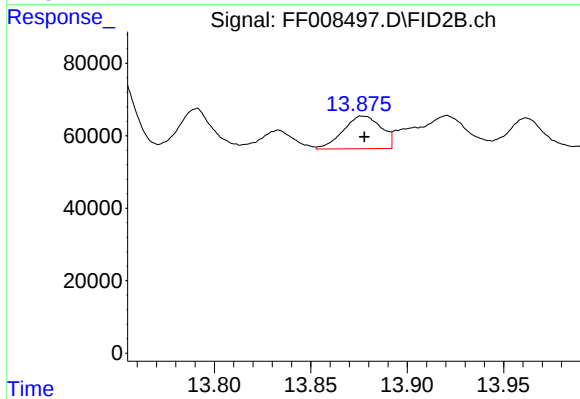

#8 N-DOCOSANE


R.T.: 13.877 min
Delta R.T.: 0.000 min
Response: 123824
Conc: 0.87 ug/ml

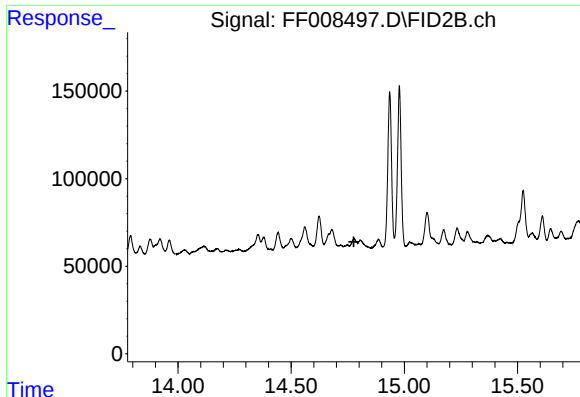

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

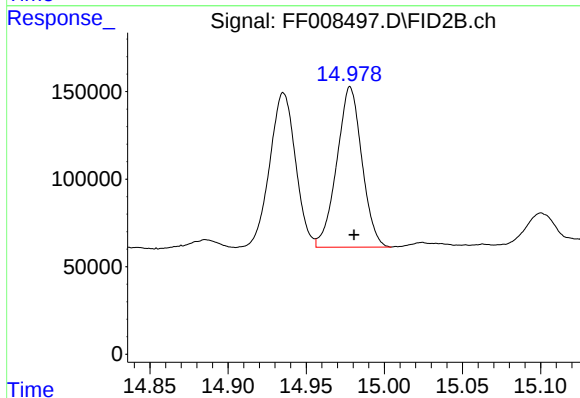


#10 N-TETRACOSANE

R.T.: 14.978 min
Delta R.T.: -0.002 min
Response: 1025086
Conc: 7.19 ug/ml

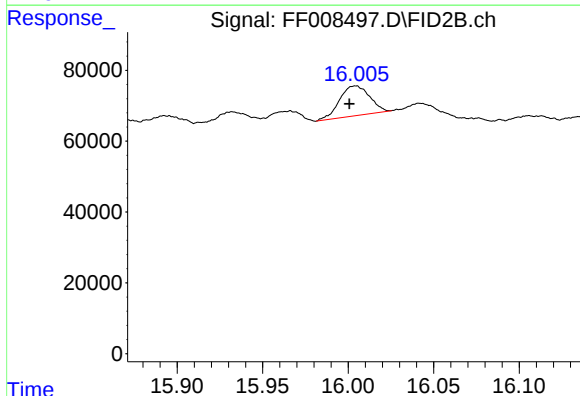


#11 N-HEXACOSANE

R.T.: 16.004 min
Delta R.T.: 0.003 min
Response: 102998
Conc: 0.73 ug/ml

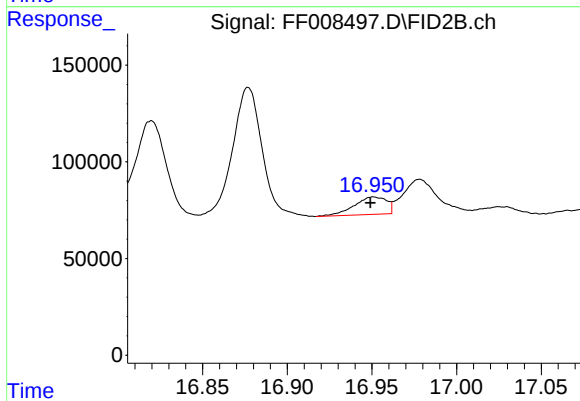

#12 N-OCTACOSANE


R.T.: 16.951 min
Delta R.T.: 0.002 min
Response: 119983
Conc: 0.86 ug/ml

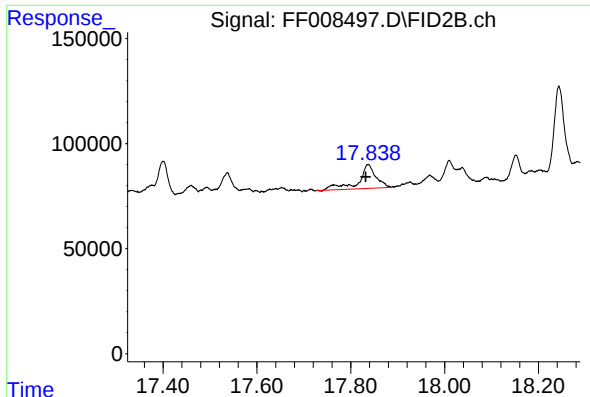

#13 N-TRIACONTANE


R.T.: 17.837 min
Delta R.T.: 0.005 min
Response: 292234
Conc: 2.11 ug/ml

Instrument :
FID_F
ClientSampleId :

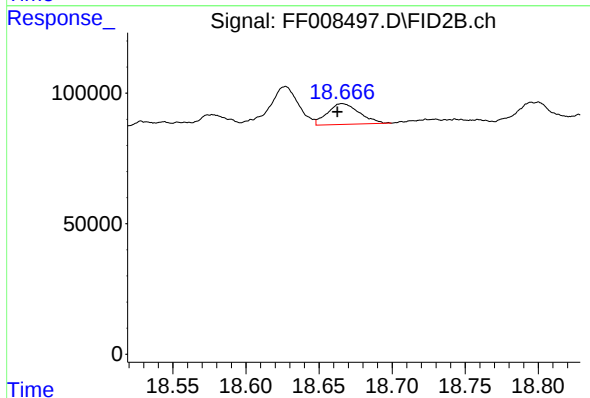

#14 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.003 min
Response: 121114
Conc: 0.89 ug/ml

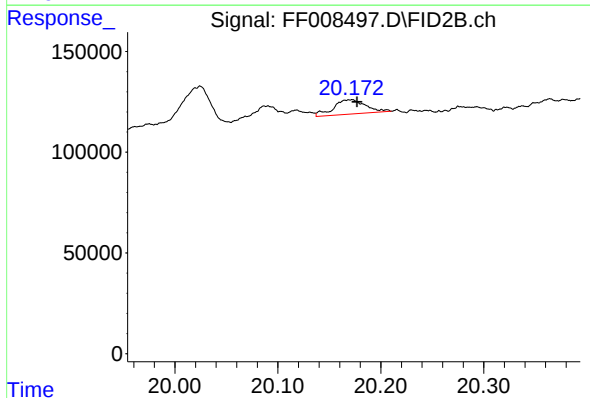

#16 N-HEXATRIACONTANE

R.T.: 20.172 min
Delta R.T.: -0.005 min
Response: 156089
Conc: 1.31 ug/ml