

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
 Data File : FF008498.D
 Signal(s) : FID2B.ch
 Acq On : 04 Jun 2021 17:12
 Operator : DD\AJ
 Sample : M2589-17 20X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 00:23:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
 Quant Title :
 QLast Update : Thu May 06 08:43:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

7)	N-EICOSANE	12.636	72851	0.513 ug/ml
10)	N-TETRACOSANE	14.977	629328	4.413 ug/ml
12)	N-OCTACOSANE	16.978	149870	1.068 ug/ml
13)	N-TRIACONTANE	17.836	268560	1.938 ug/ml
14)	N-DOTRIACONTANE	18.670	89842	0.663 ug/ml
15)	N-TETRATRIACONTANE	19.448	83790	0.657 ug/ml
16)	N-HEXATRIACONTANE	20.173	80940	0.678 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008498.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 17:12
Operator : DD\AJ
Sample : M2589-17 20X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:23:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

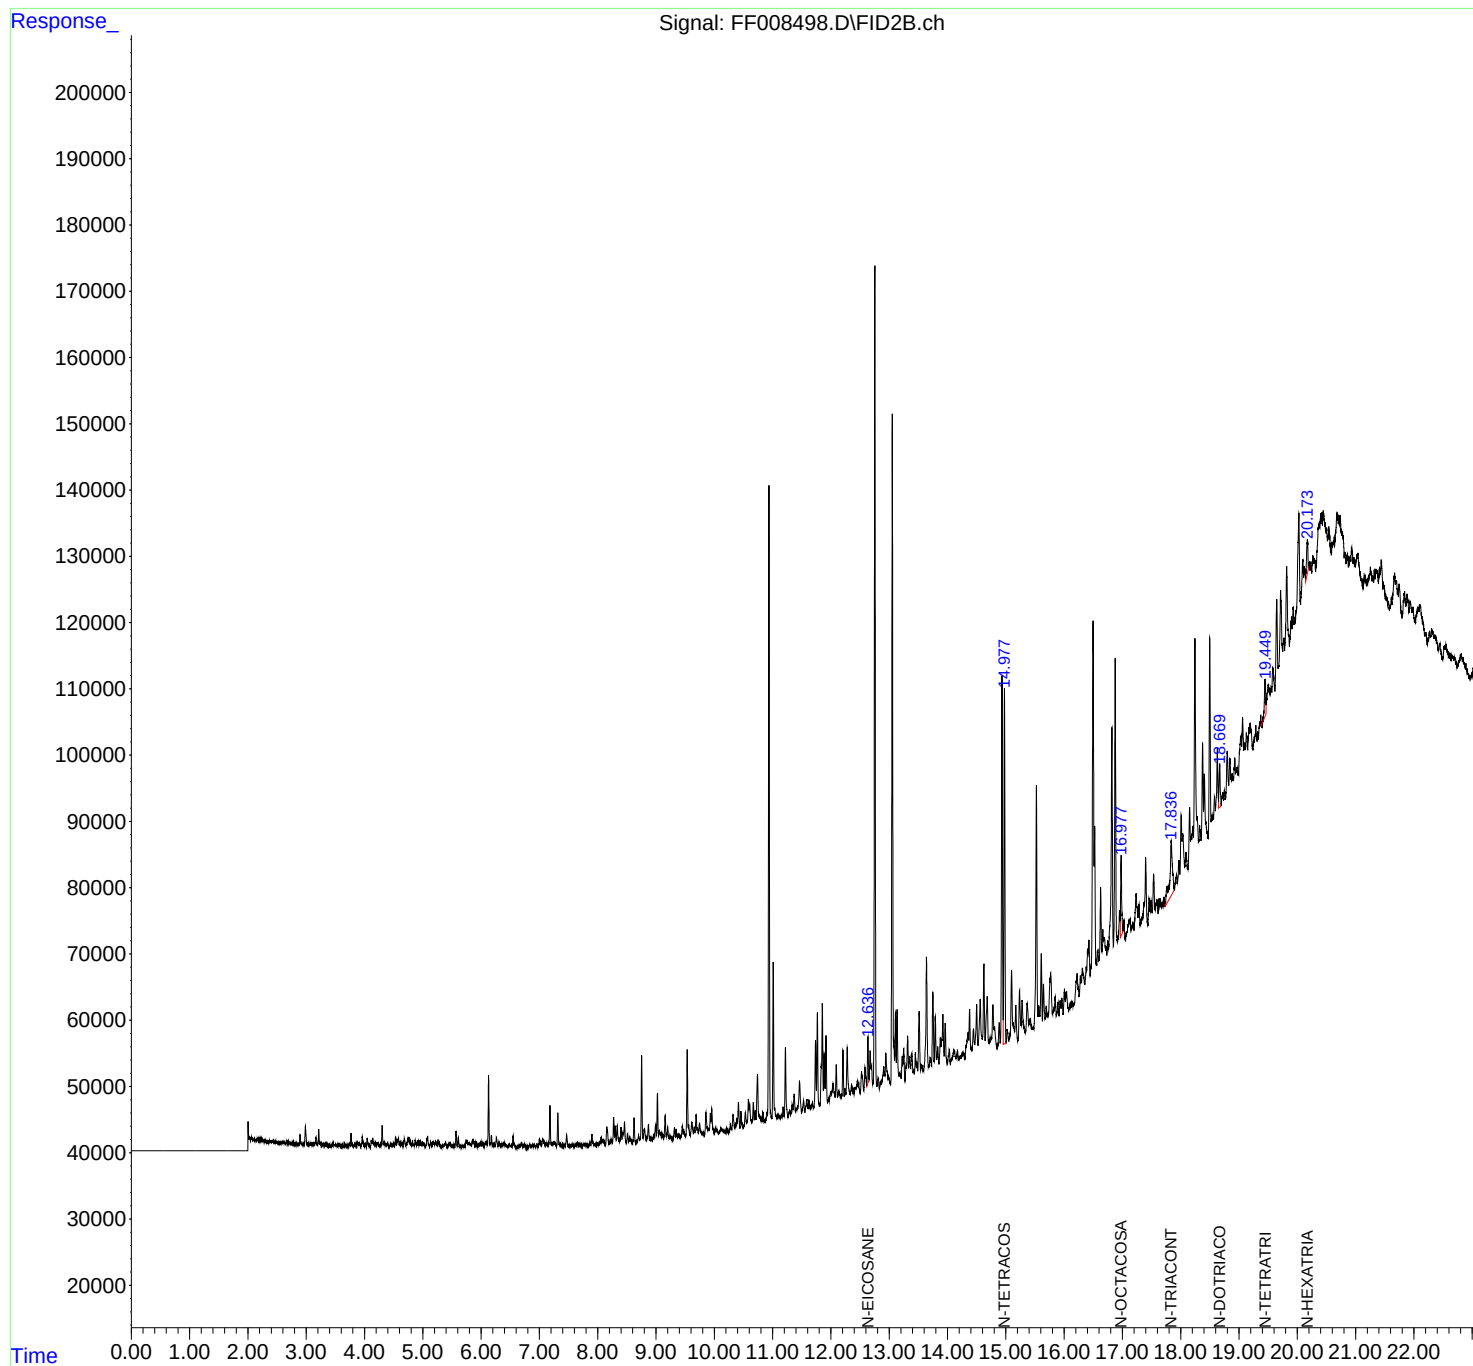


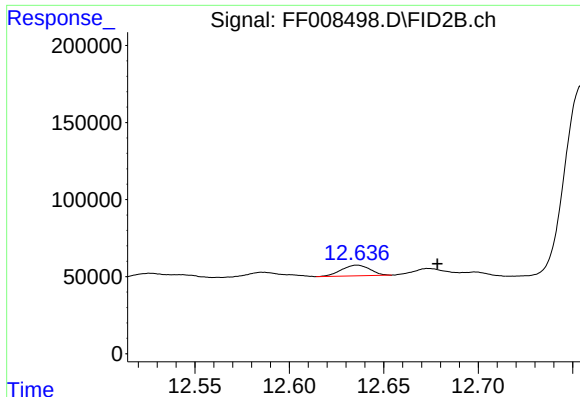

#7 N-EICOSANE


R.T.: 12.636 min
Delta R.T.: -0.042 min
Response: 72851
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

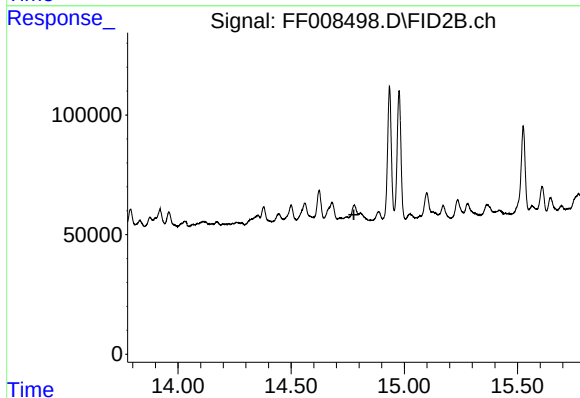


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

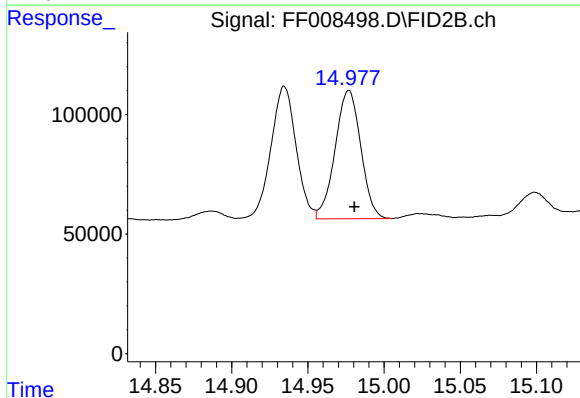


#10 N-TETRACOSANE

R.T.: 14.977 min
Delta R.T.: -0.004 min
Response: 629328
Conc: 4.41 ug/ml

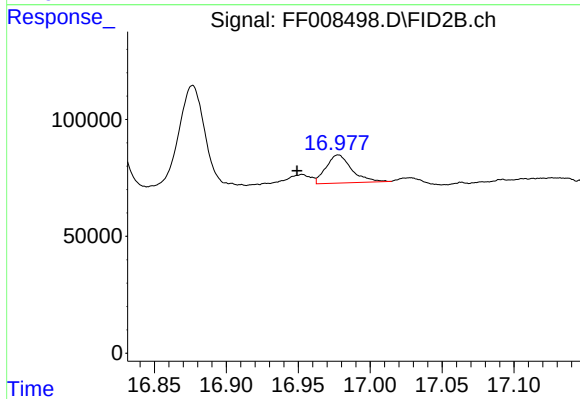

#12 N-OCTACOSANE


R.T.: 16.978 min
Delta R.T.: 0.029 min
Response: 149870
Conc: 1.07 ug/ml

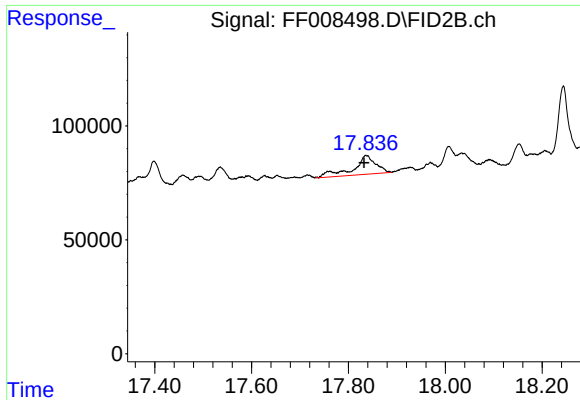

#13 N-TRIACONTANE


R.T.: 17.836 min
Delta R.T.: 0.004 min
Response: 268560
Conc: 1.94 ug/ml

Instrument :
FID_F
ClientSampleId :

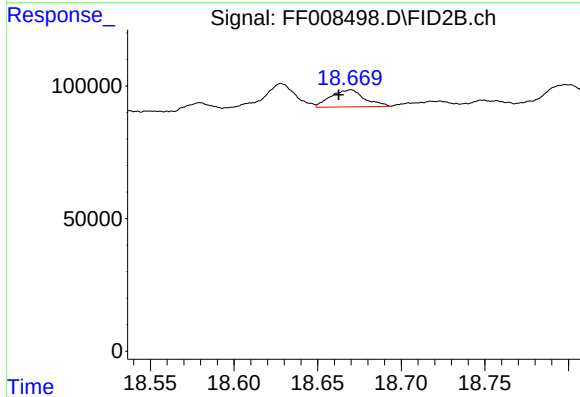


#14 N-DOTRIACONTANE

R.T.: 18.670 min
Delta R.T.: 0.007 min
Response: 89842
Conc: 0.66 ug/ml

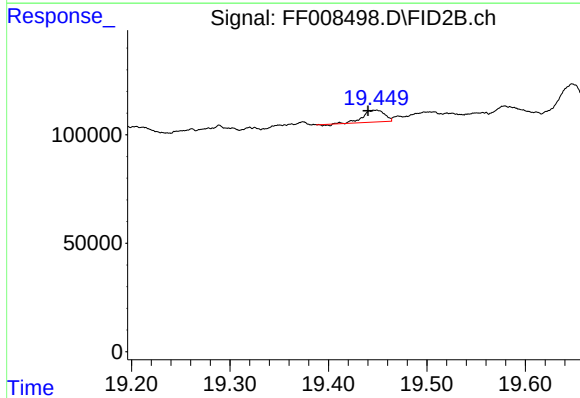

#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: 0.008 min
Response: 83790
Conc: 0.66 ug/ml

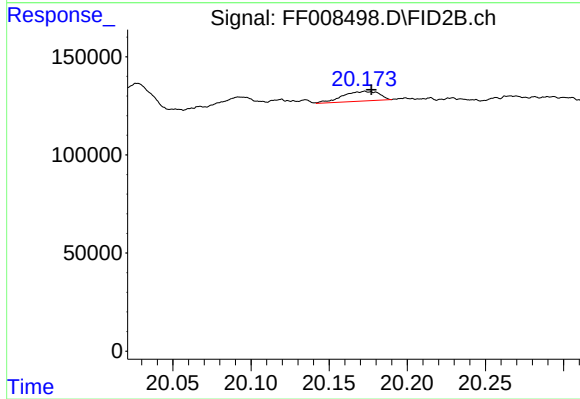

#16 N-HEXATRIACONTANE

R.T.: 20.173 min
Delta R.T.: -0.004 min
Response: 80940
Conc: 0.68 ug/ml