

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008499.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 17:44
Operator : DD\AJ
Sample : M2589-18 20X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:23:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.975	97484	0.684 ug/ml
13)	N-TRIACONTANE	17.835	22077	0.159 ug/ml
14)	N-DOTRIACONTANE	18.667	50228	0.371 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060421\
Data File : FF008499.D
Signal(s) : FID2B.ch
Acq On : 04 Jun 2021 17:44
Operator : DD\AJ
Sample : M2589-18 20X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 00:23:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF050521.M
Quant Title :
QLast Update : Thu May 06 08:43:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

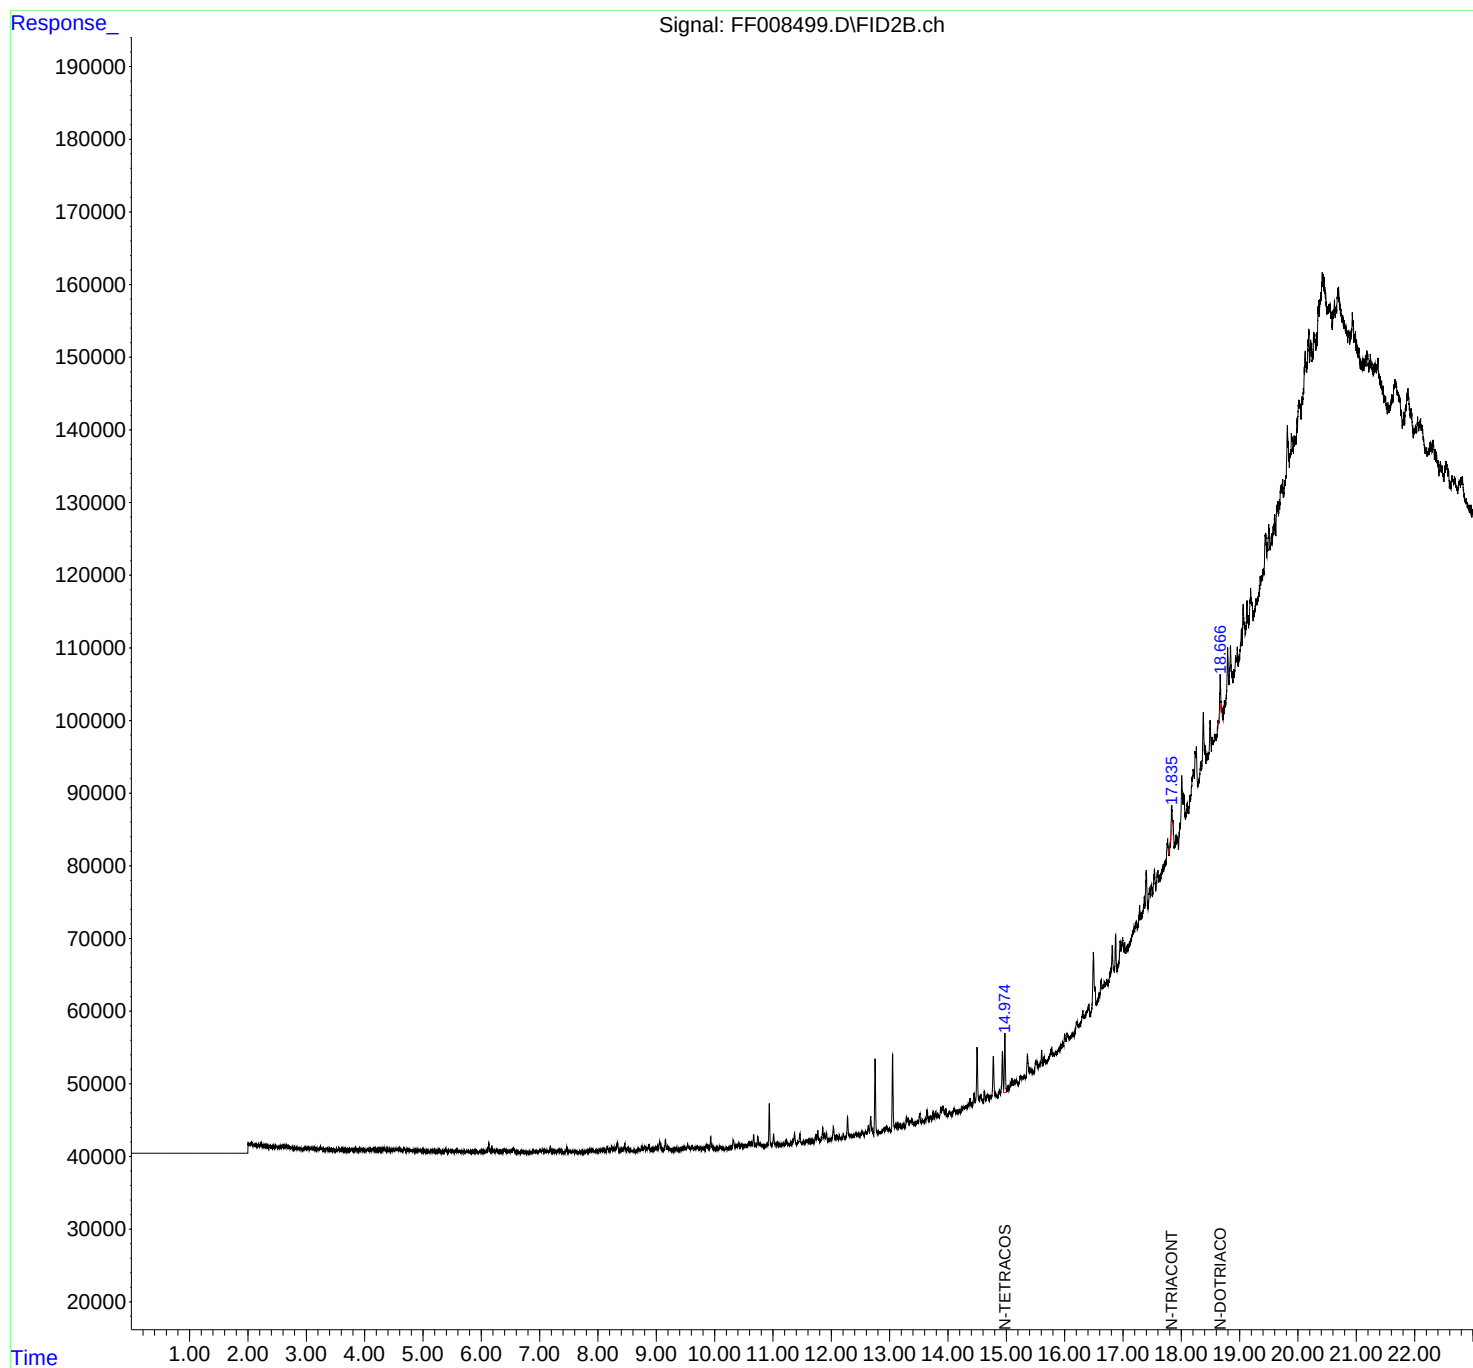


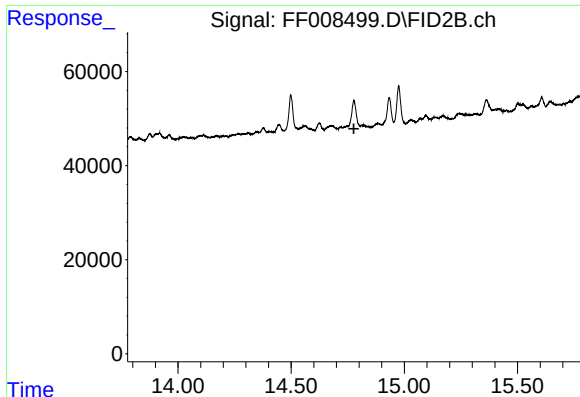

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

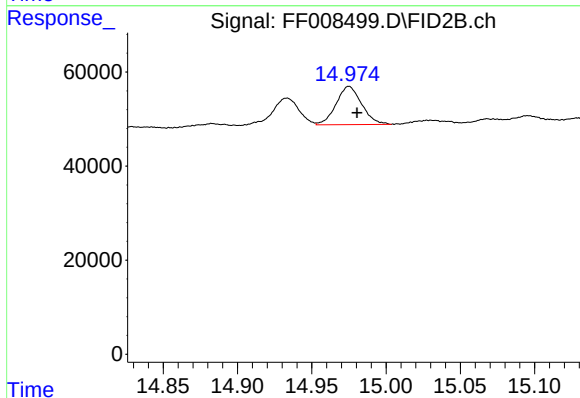


#10 N-TETRACOSANE

R.T.: 14.975 min
Delta R.T.: -0.006 min
Response: 97484
Conc: 0.68 ug/ml

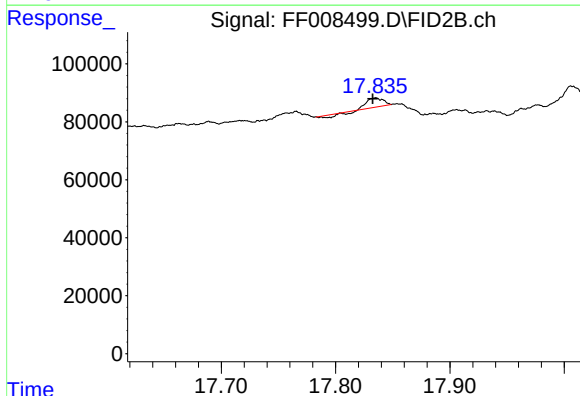

#13 N-TRIACONTANE

R.T.: 17.835 min
Delta R.T.: 0.003 min
Response: 22077
Conc: 0.16 ug/ml

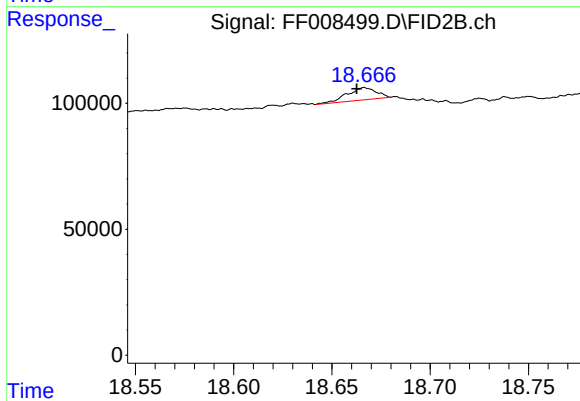

#14 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: 0.004 min
Response: 50228
Conc: 0.37 ug/ml