

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
 Data File : FF012813.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2023 09:32
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 07:04:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Fri Jun 02 06:12:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.979	1917023	16.416 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.037	55220	0.428 ug/ml
14) N-DOTRIACONTANE	18.868	70595	0.559 ug/ml
15) N-TETRATRIACONTANE	19.649	64181	0.540 ug/ml
16) N-HEXATRIACONTANE	20.389	43617	0.363 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
Data File : FF012813.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2023 09:32
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 07:04:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

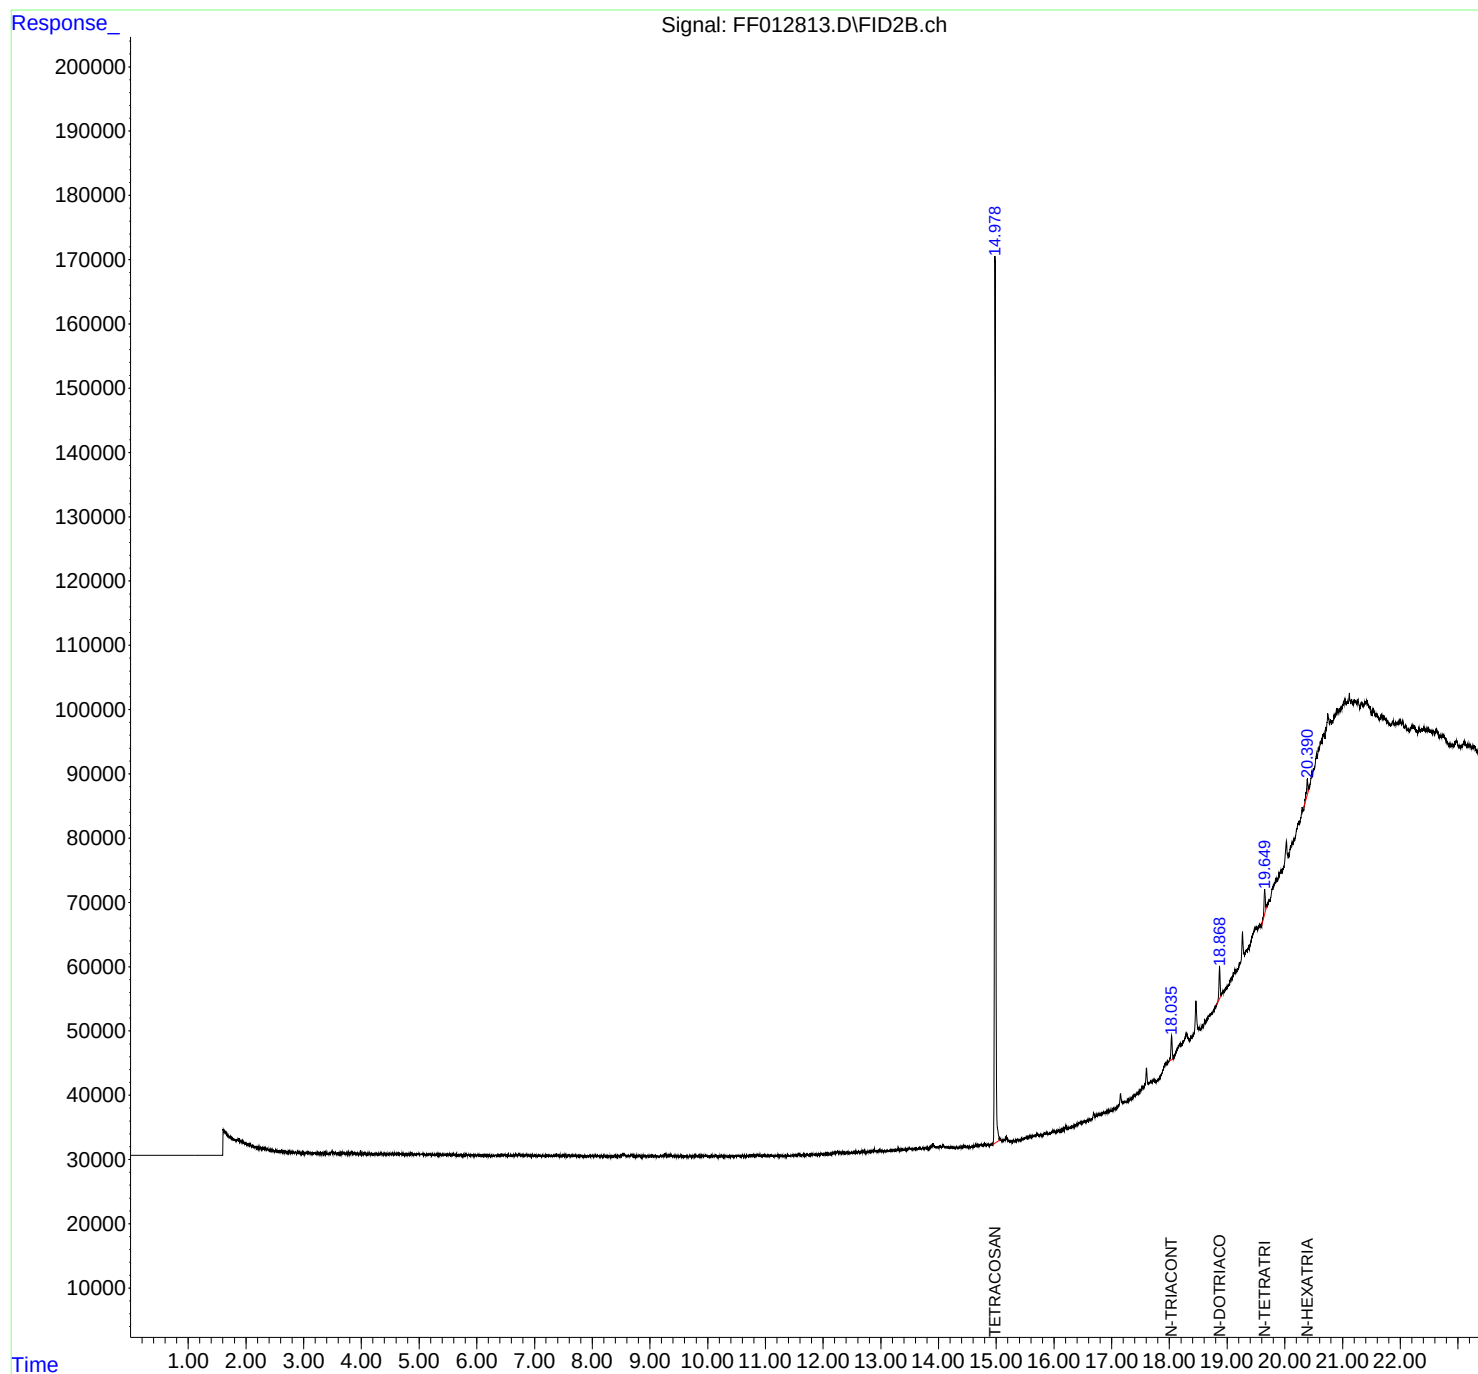


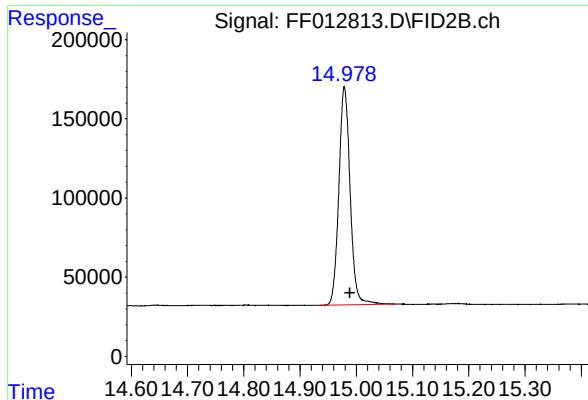

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.979 min
Delta R.T.: -0.010 min
Response: 1917023
Conc: 16.42 ug/ml

Instrument :
FID_F
ClientSampleId :

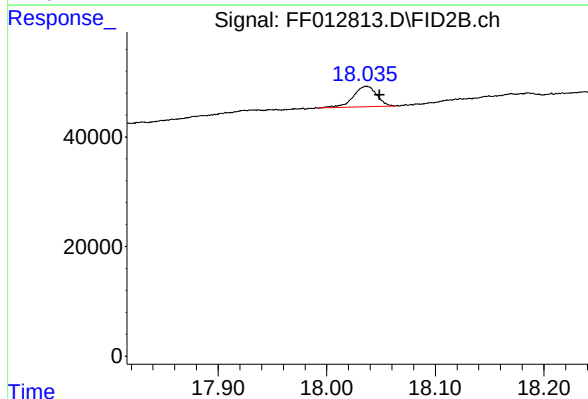


#13 N-TRIACONTANE

R.T.: 18.037 min
Delta R.T.: -0.012 min
Response: 55220
Conc: 0.43 ug/ml

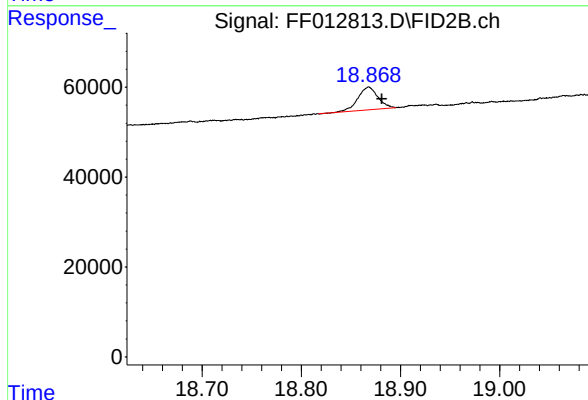


#14 N-DOTRIACONTANE

R.T.: 18.868 min
Delta R.T.: -0.013 min
Response: 70595
Conc: 0.56 ug/ml

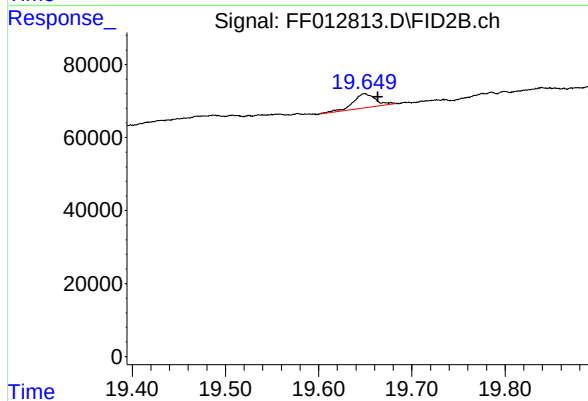

#15 N-TETRATRIACONTANE

R.T.: 19.649 min
Delta R.T.: -0.014 min
Response: 64181
Conc: 0.54 ug/ml

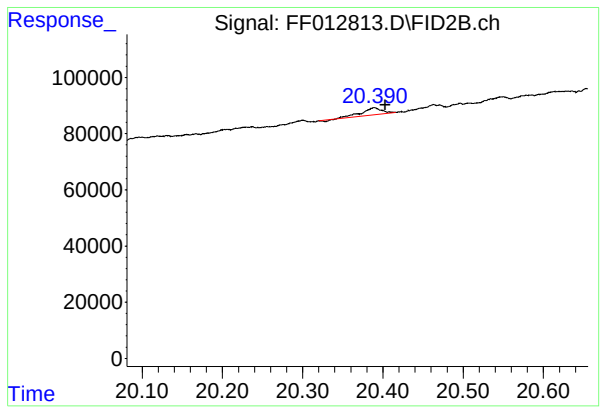

#16 N-HEXATRIACONTANE

R.T.: 20.389 min
Delta R.T.: -0.014 min
Response: 43617
Conc: 0.36 ug/ml

Instrument :
FID_F
ClientSampleId :