

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
 Data File : FF012816.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2023 12:27
 Operator : YP\AJ
 Sample : 03002-03
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 06:57:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Fri Jun 02 06:12:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.978	1482179	12.692 ug/ml
Target Compounds			
7) N-EICOSANE	12.904	76823	0.561 ug/ml
8) N-DOCOSANE	14.082	181289	1.371 ug/ml
10) N-TETRACOSANE	15.180	2181383	16.505 ug/ml
11) N-HEXACOSANE	16.203	228558	1.768 ug/ml
12) N-OCTACOSANE	17.149	337465	2.633 ug/ml
13) N-TRIACONTANE	18.036	388957	3.016 ug/ml
14) N-DOTRIACONTANE	18.856	1092004	8.639 ug/ml
15) N-TETRATRIACONTANE	19.647	85661	0.721 ug/ml
16) N-HEXATRIACONTANE	20.387	209611	1.745 ug/ml
17) N-OCTATRIACONTANE	21.115	79775	0.686 ug/ml
18) N-TETRACONTANE	22.003	102217	0.822 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
Data File : FF012816.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2023 12:27
Operator : YP\AJ
Sample : 03002-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 06:57:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

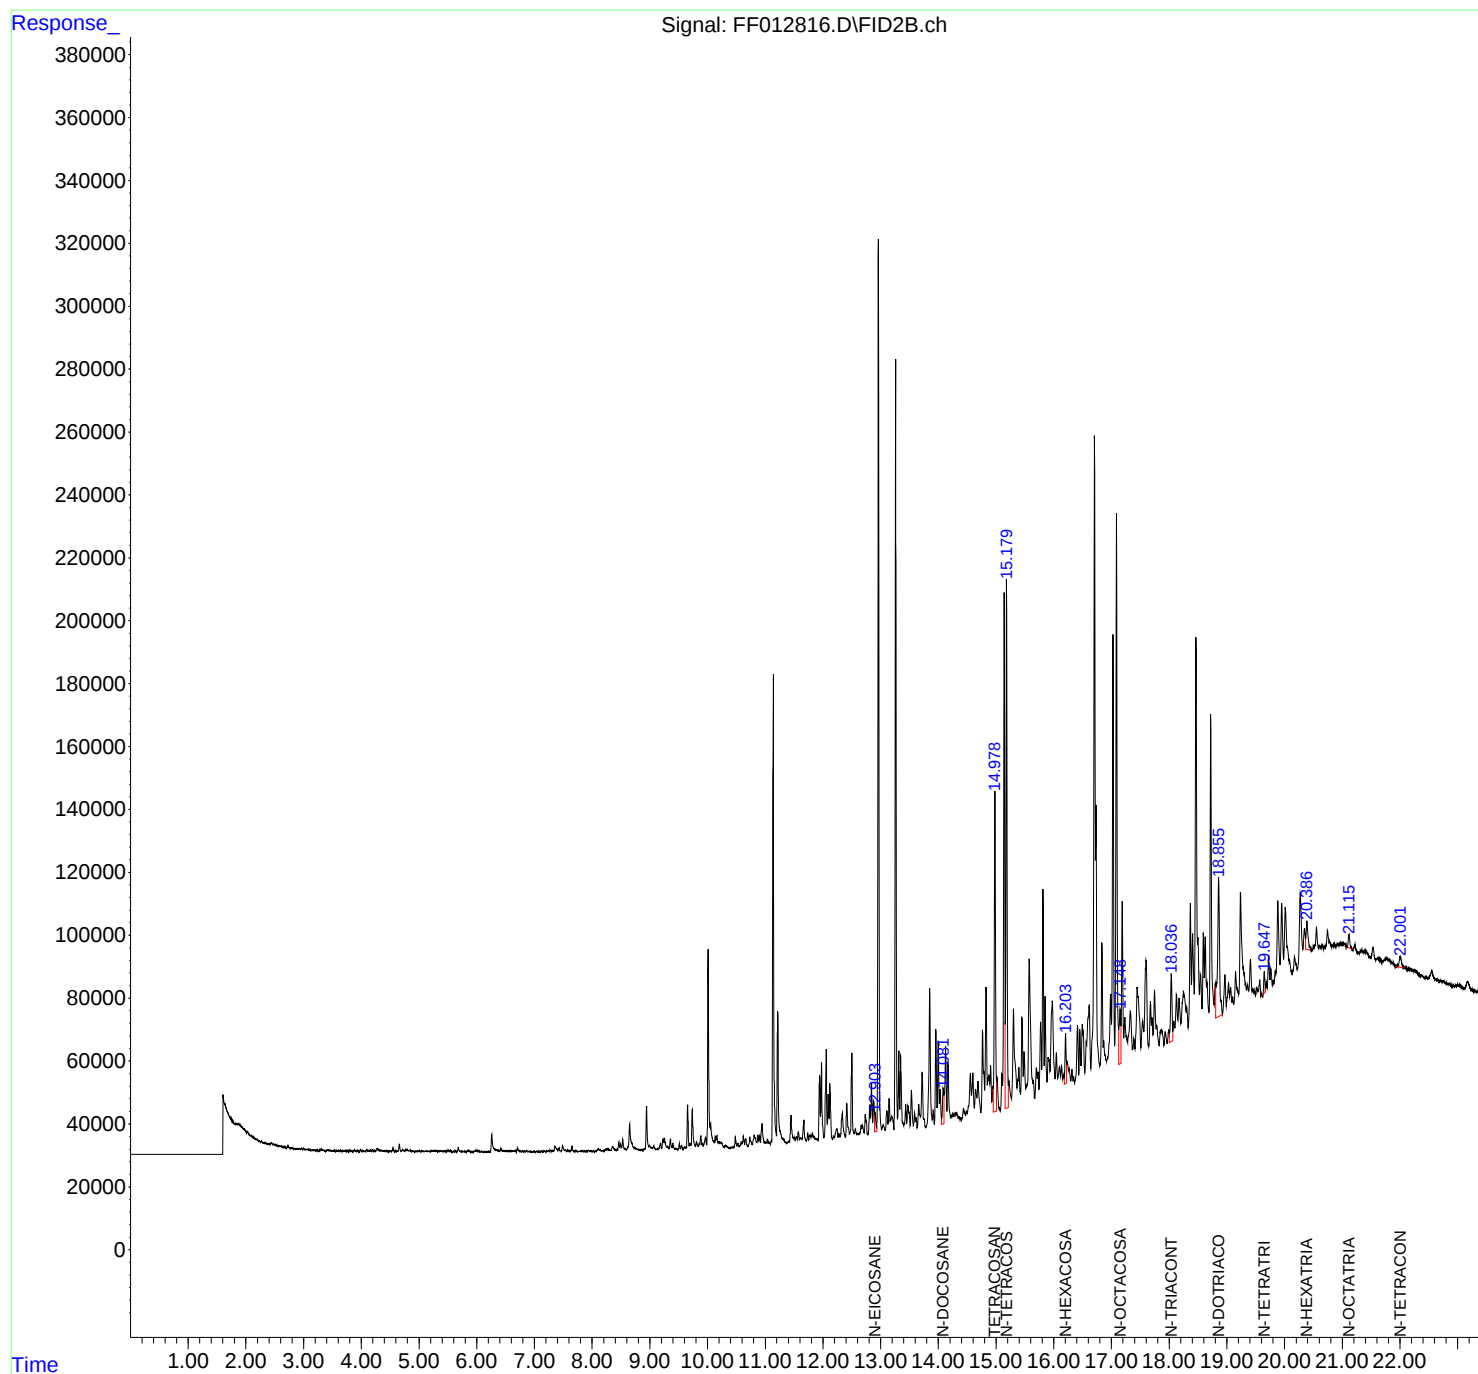


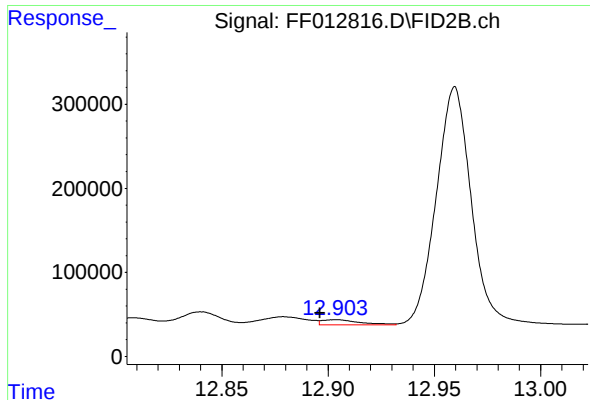

#7 N-EICOSANE


R.T.: 12.904 min
Delta R.T.: 0.008 min
Response: 76823
Conc: 0.56 ug/ml

Instrument :
FID_F
ClientSampleId :

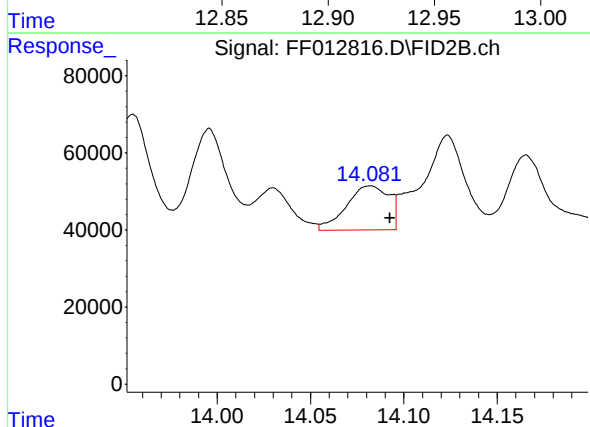


#8 N-DOCOSANE

R.T.: 14.082 min
Delta R.T.: -0.011 min
Response: 181289
Conc: 1.37 ug/ml

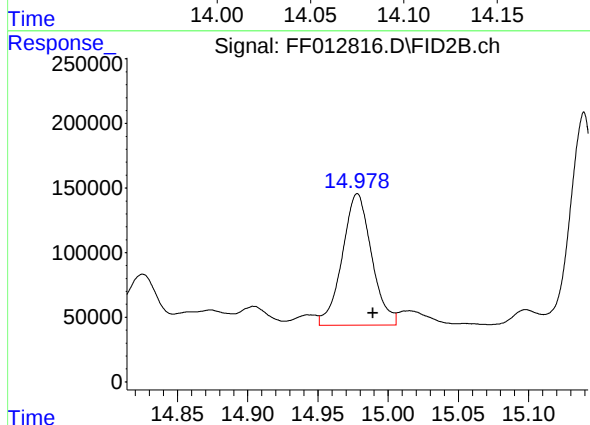


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.978 min
Delta R.T.: -0.011 min
Response: 1482179
Conc: 12.69 ug/ml

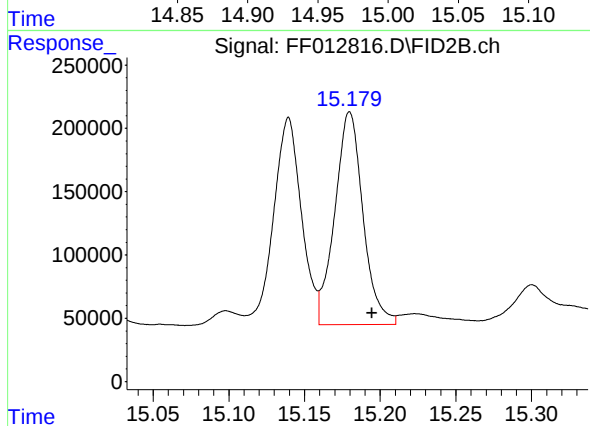

#10 N-TETRACOSANE


R.T.: 15.180 min
Delta R.T.: -0.015 min
Response: 2181383
Conc: 16.51 ug/ml

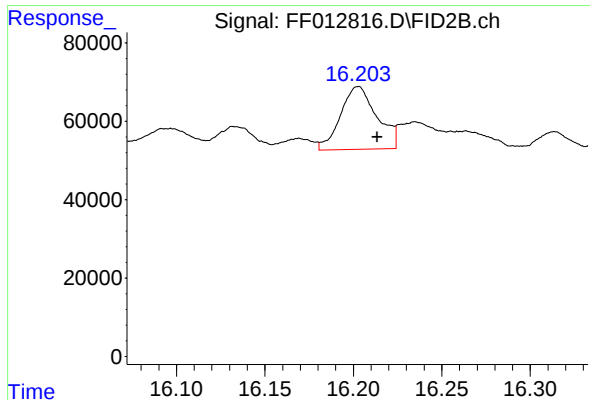

#11 N-HEXACOSANE


R.T.: 16.203 min
Delta R.T.: -0.011 min
Response: 228558
Conc: 1.77 ug/ml

Instrument :
FID_F
ClientSampleId :

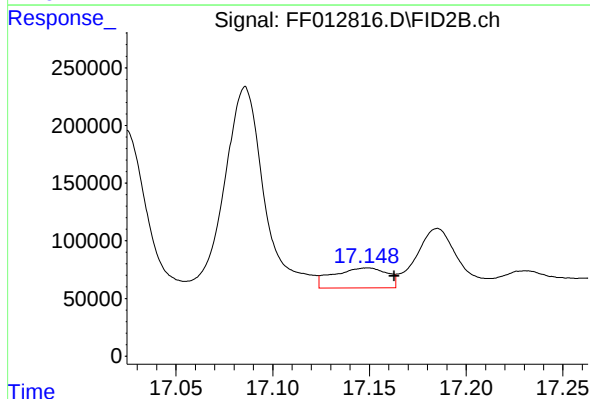


#12 N-OCTACOSANE

R.T.: 17.149 min
Delta R.T.: -0.014 min
Response: 337465
Conc: 2.63 ug/ml

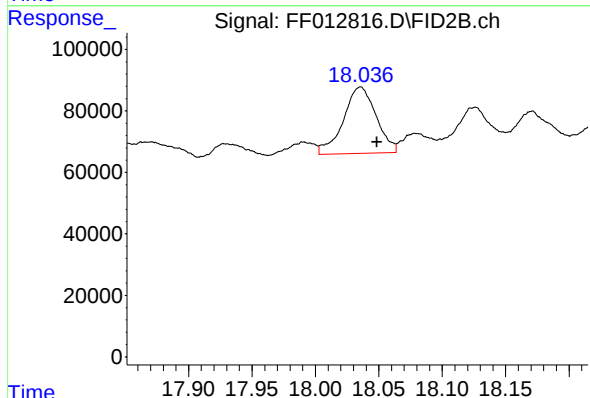


#13 N-TRIACONTANE

R.T.: 18.036 min
Delta R.T.: -0.013 min
Response: 388957
Conc: 3.02 ug/ml

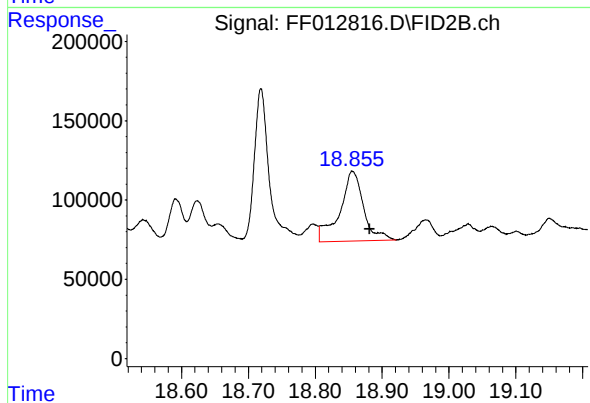

#14 N-DOTRIACONTANE


R.T.: 18.856 min
Delta R.T.: -0.026 min
Response: 1092004
Conc: 8.64 ug/ml

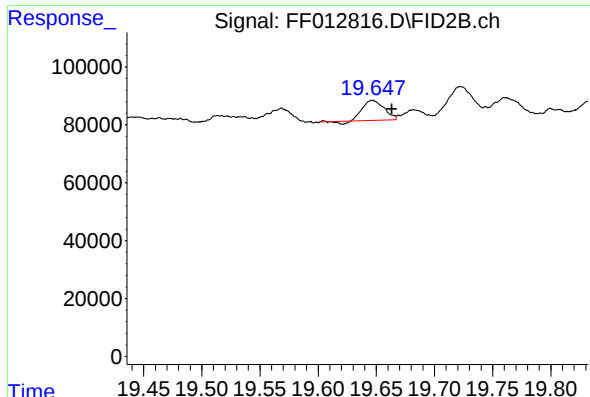

#15 N-TETRATRIACONTANE


R.T.: 19.647 min
Delta R.T.: -0.017 min
Response: 85661
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

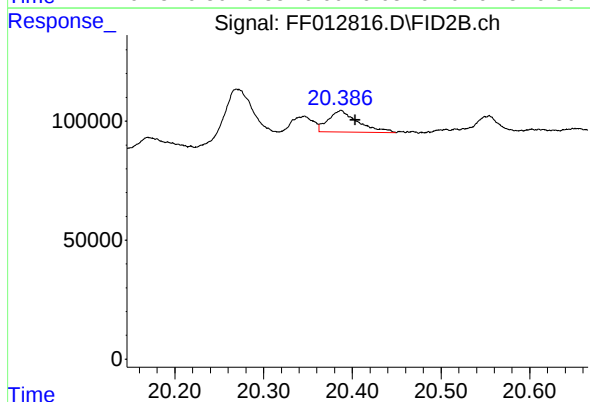


#16 N-HEXATRIACONTANE

R.T.: 20.387 min
Delta R.T.: -0.016 min
Response: 209611
Conc: 1.75 ug/ml

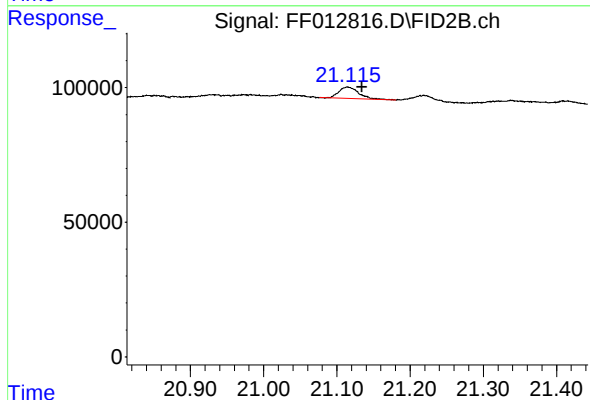

#17 N-OCTATRIACONTANE

R.T.: 21.115 min
Delta R.T.: -0.020 min
Response: 79775
Conc: 0.69 ug/ml

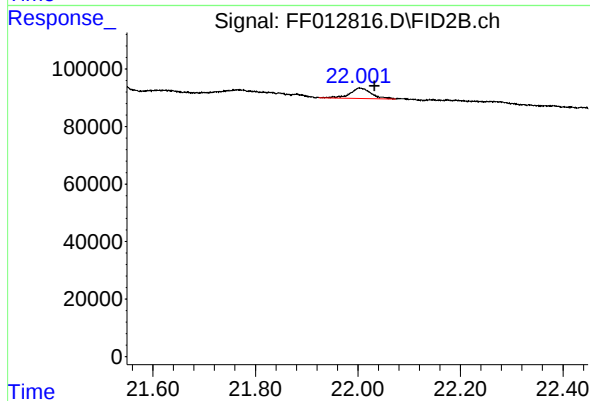

#18 N-TETRACONTANE

R.T.: 22.003 min
Delta R.T.: -0.030 min
Response: 102217
Conc: 0.82 ug/ml