

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
 Data File : FF012823.D
 Signal(s) : FID2B.ch
 Acq On : 03 Jun 2023 15:51
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 05 06:58:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
 Quant Title :
 QLast Update : Fri Jun 02 06:12:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.977	1945240	16.658 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.033	63211	0.490 ug/ml
14) N-DOTRIACONTANE	18.866	113520	0.898 ug/ml
15) N-TETRATRIACONTANE	19.650	60836	0.512 ug/ml
16) N-HEXATRIACONTANE	20.386	62297	0.519 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
Data File : FF012823.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2023 15:51
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 05 06:58:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

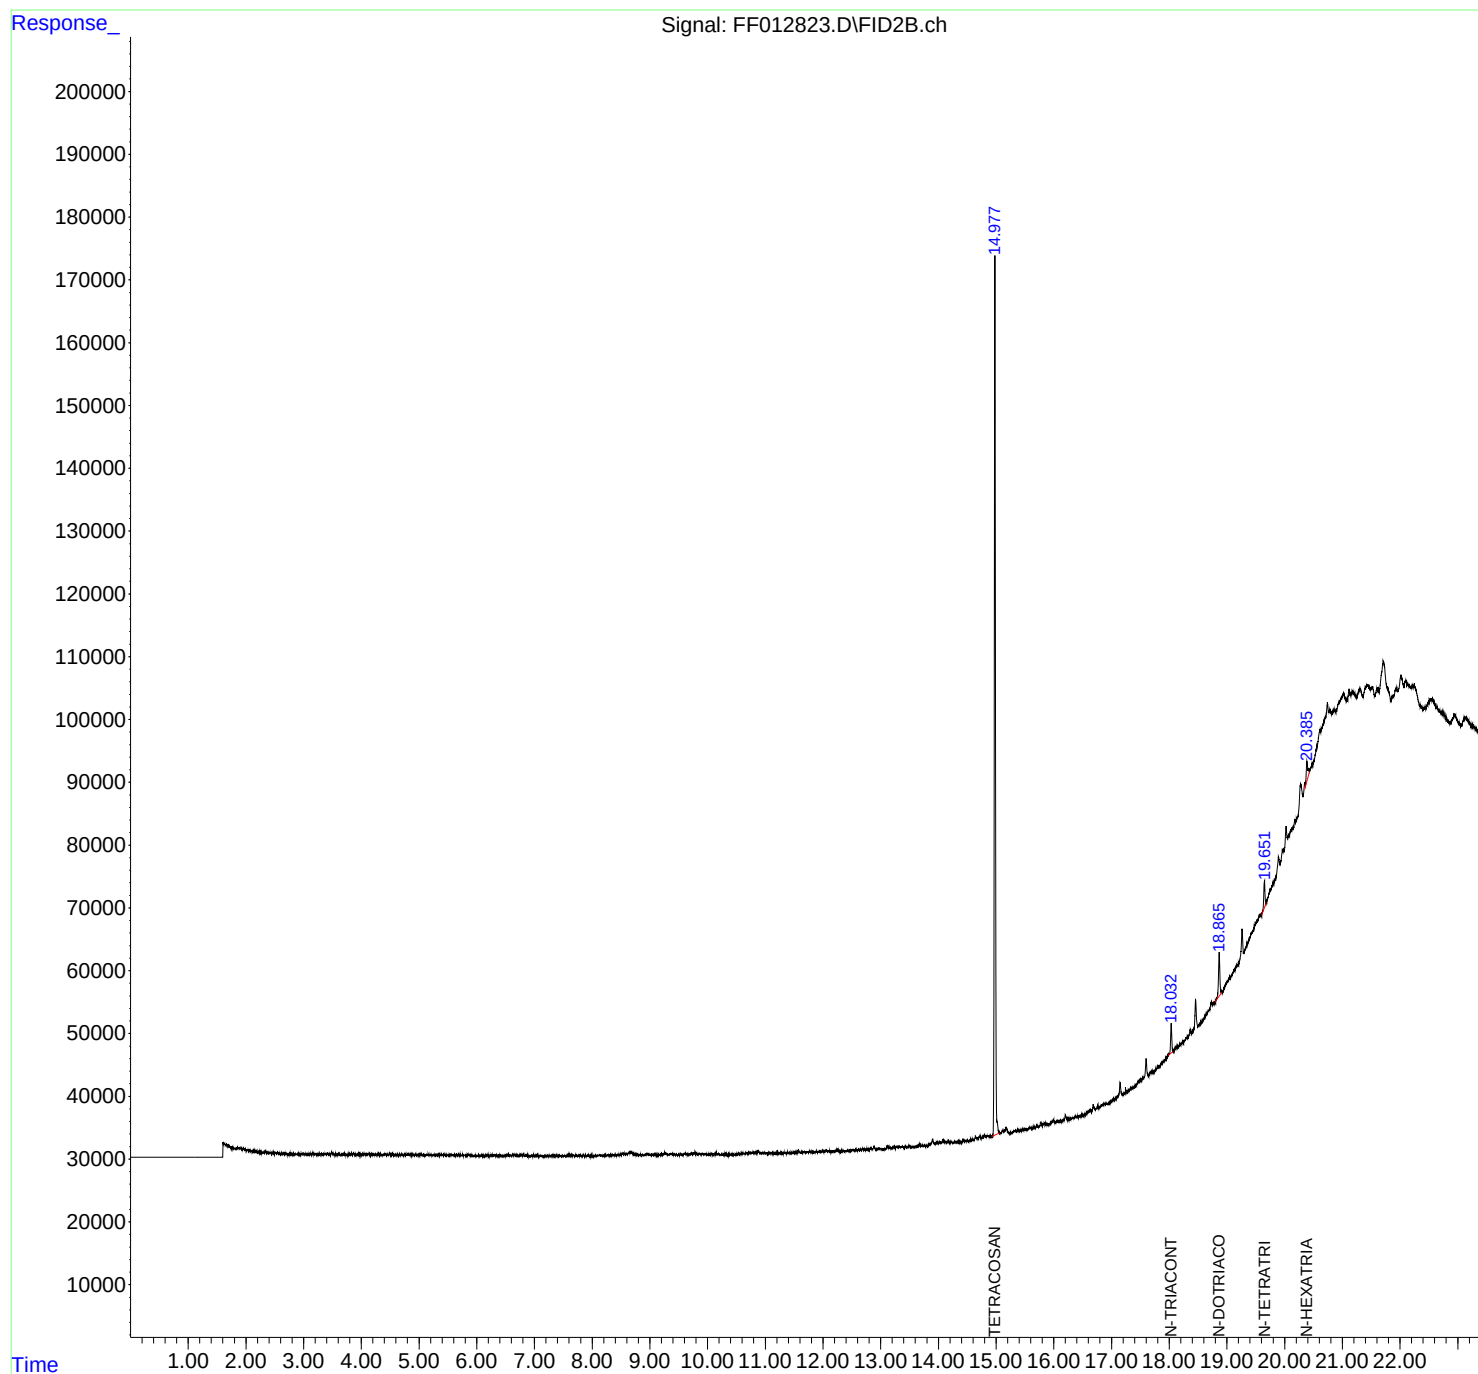


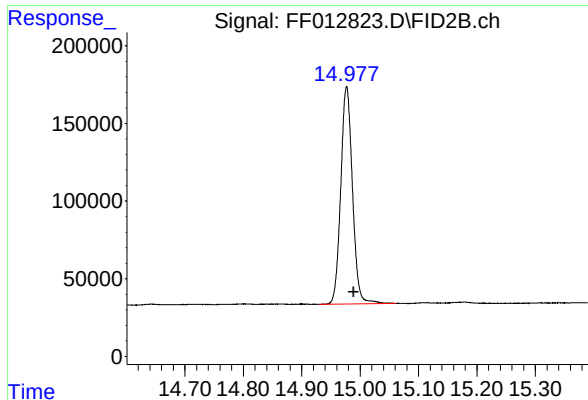

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.977 min
Delta R.T.: -0.012 min
Response: 1945240
Conc: 16.66 ug/ml

Instrument :
FID_F
ClientSampleId :

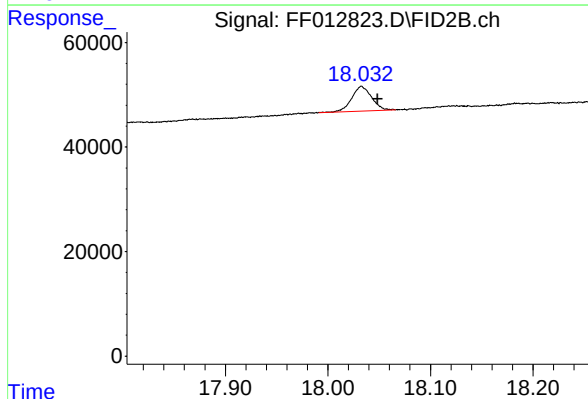


#13 N-TRIACONTANE

R.T.: 18.033 min
Delta R.T.: -0.016 min
Response: 63211
Conc: 0.49 ug/ml

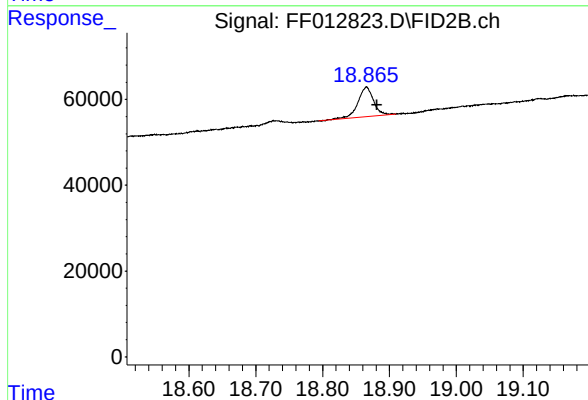


#14 N-DOTRIACONTANE

R.T.: 18.866 min
Delta R.T.: -0.016 min
Response: 113520
Conc: 0.90 ug/ml

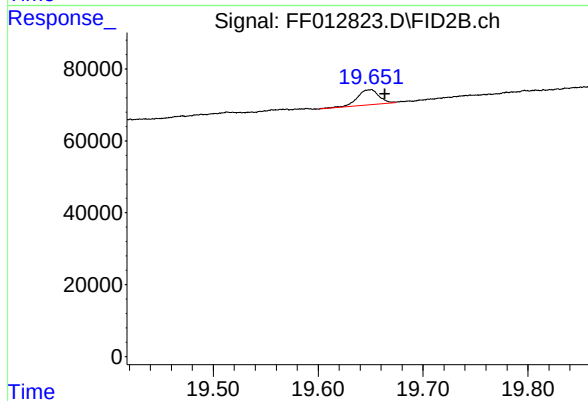

#15 N-TETRATRIACONTANE

R.T.: 19.650 min
Delta R.T.: -0.014 min
Response: 60836
Conc: 0.51 ug/ml

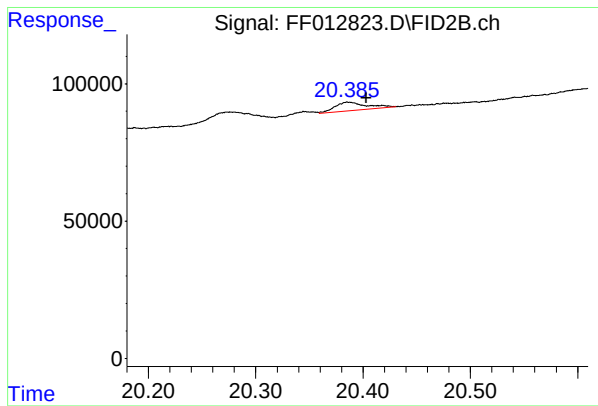

#16 N-HEXATRIACONTANE

R.T.: 20.386 min
Delta R.T.: -0.017 min
Response: 62297
Conc: 0.52 ug/ml

Instrument :

FID_F

ClientSampleId :