

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
Data File : FF012815.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2023 11:29
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 05 06:57:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.709	4292900	32.940 ug/ml
12) N-OCTACOSANE	17.151	4393578	34.282 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060423\
Data File : FF012815.D
Signal(s) : FID2B.ch
Acq On : 03 Jun 2023 11:29
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 05 06:57:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060223.M
Quant Title :
QLast Update : Fri Jun 02 06:12:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

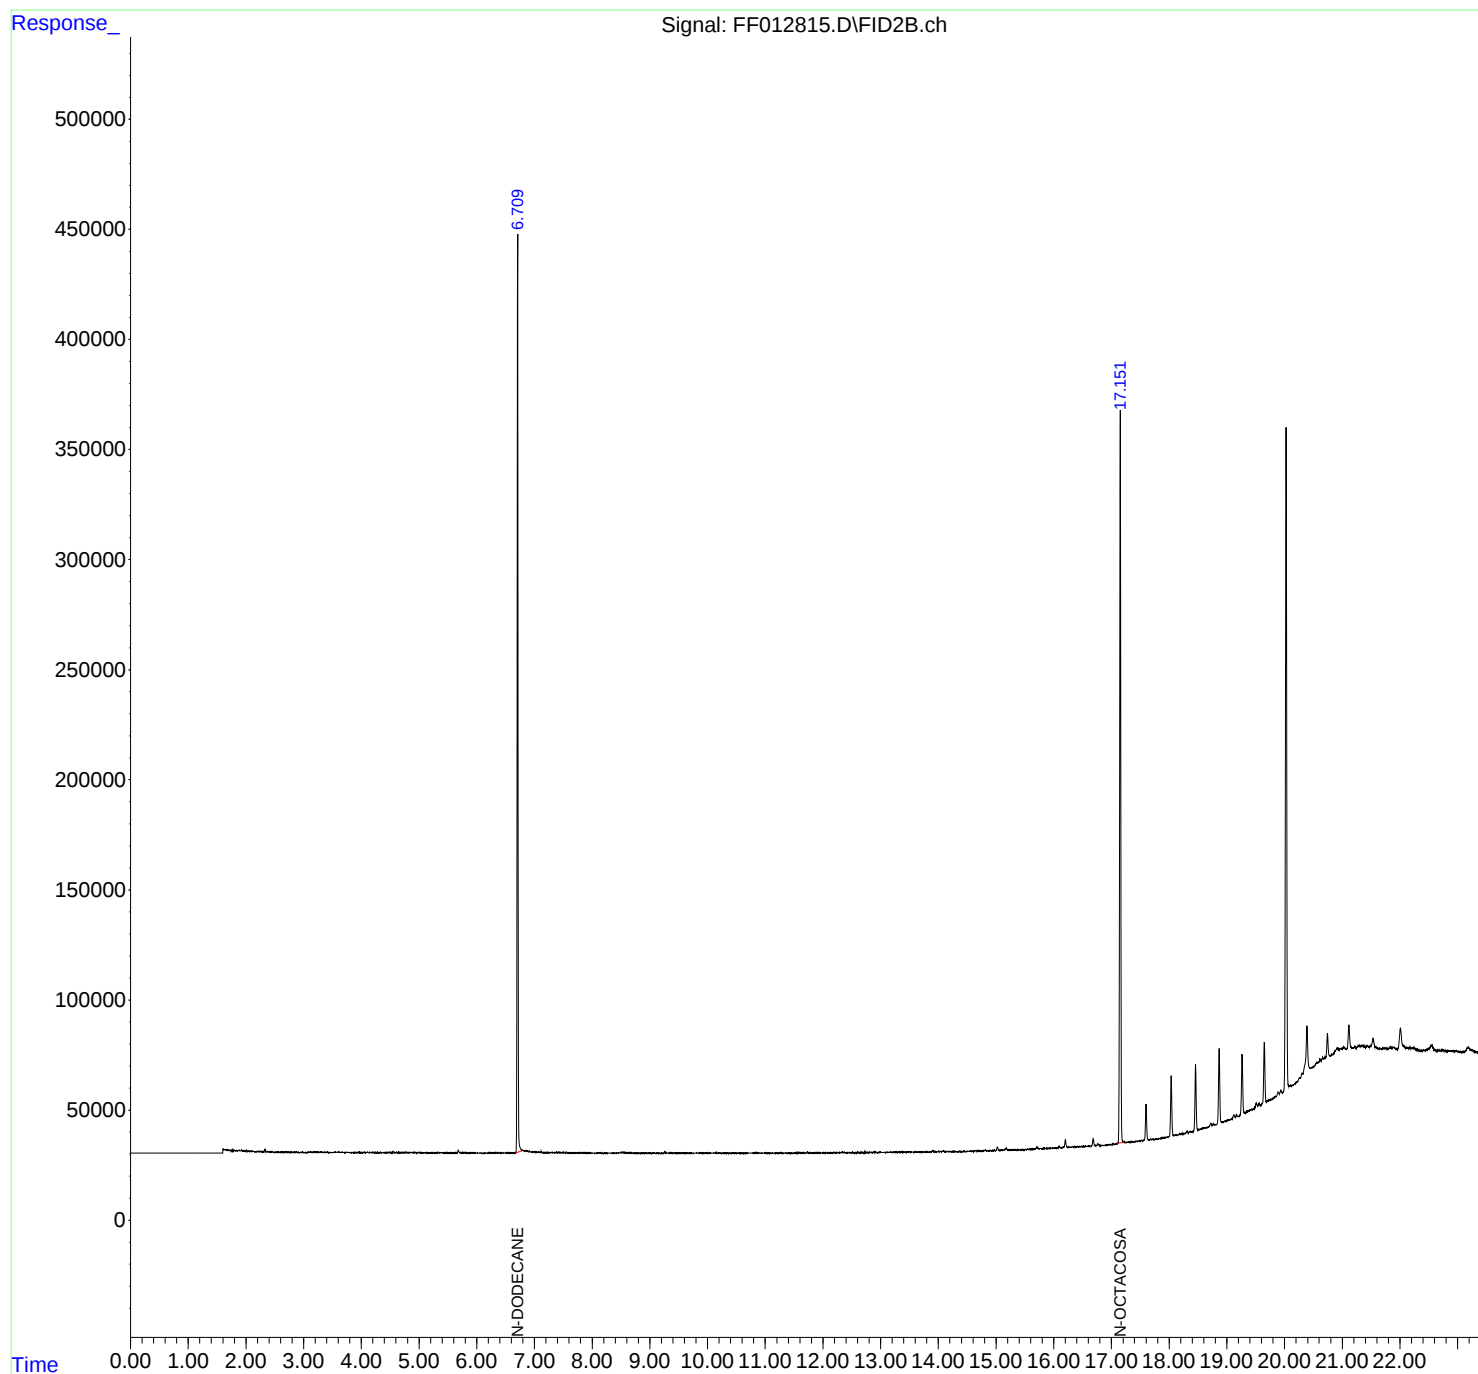


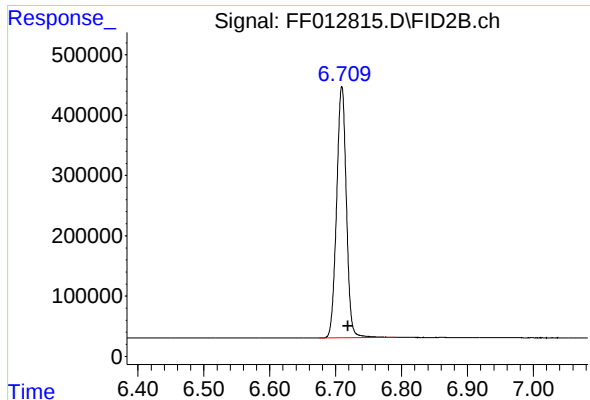

#3 N-DODECANE


R.T.: 6.709 min
Delta R.T.: -0.009 min
Response: 4292900
Conc: 32.94 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

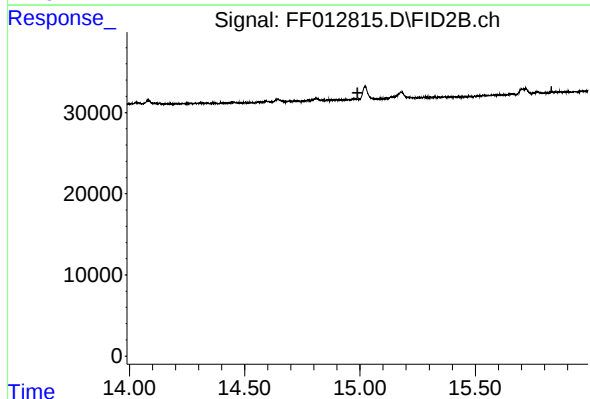

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.989 min
Response: 0
Conc: N.D.

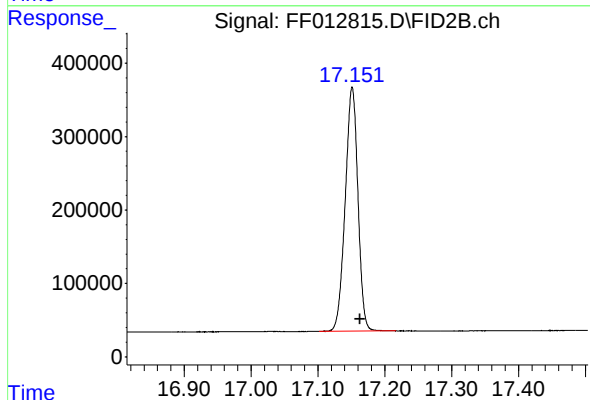

#12 N-OCTACOSANE

R.T.: 17.151 min
Delta R.T.: -0.012 min
Response: 4393578
Conc: 34.28 ug/ml