

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060619\
 Data File : FF004730.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2019 18:23
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 07 01:07:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
 Quant Title :
 QLast Update : Thu May 23 07:21:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	5624312	46.059 ug/ml
Target Compounds			
2) N-DECANE	4.419	7256170	49.553 ug/ml
3) N-DODECANE	6.444	7188270	48.575 ug/ml
4) N-TETRADECANE	8.241	7007693	47.707 ug/ml
5) N-HEXADECANE	9.845	6892465	46.683 ug/ml
6) N-OCTADECANE	11.292	6663992	45.901 ug/ml
7) N-EICOSANE	12.607	6580566	45.437 ug/ml
8) N-DOCOSANE	13.809	6441649	45.587 ug/ml
10) N-TETRACOSANE	14.918	6408520	46.242 ug/ml
11) N-HEXACOSANE	15.944	6408484	47.034 ug/ml
12) N-OCTACOSANE	16.899	6463611	47.540 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060619\
Data File : FF004730.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2019 18:23
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 07 01:07:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF052219.M
Quant Title :
QLast Update : Thu May 23 07:21:19 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

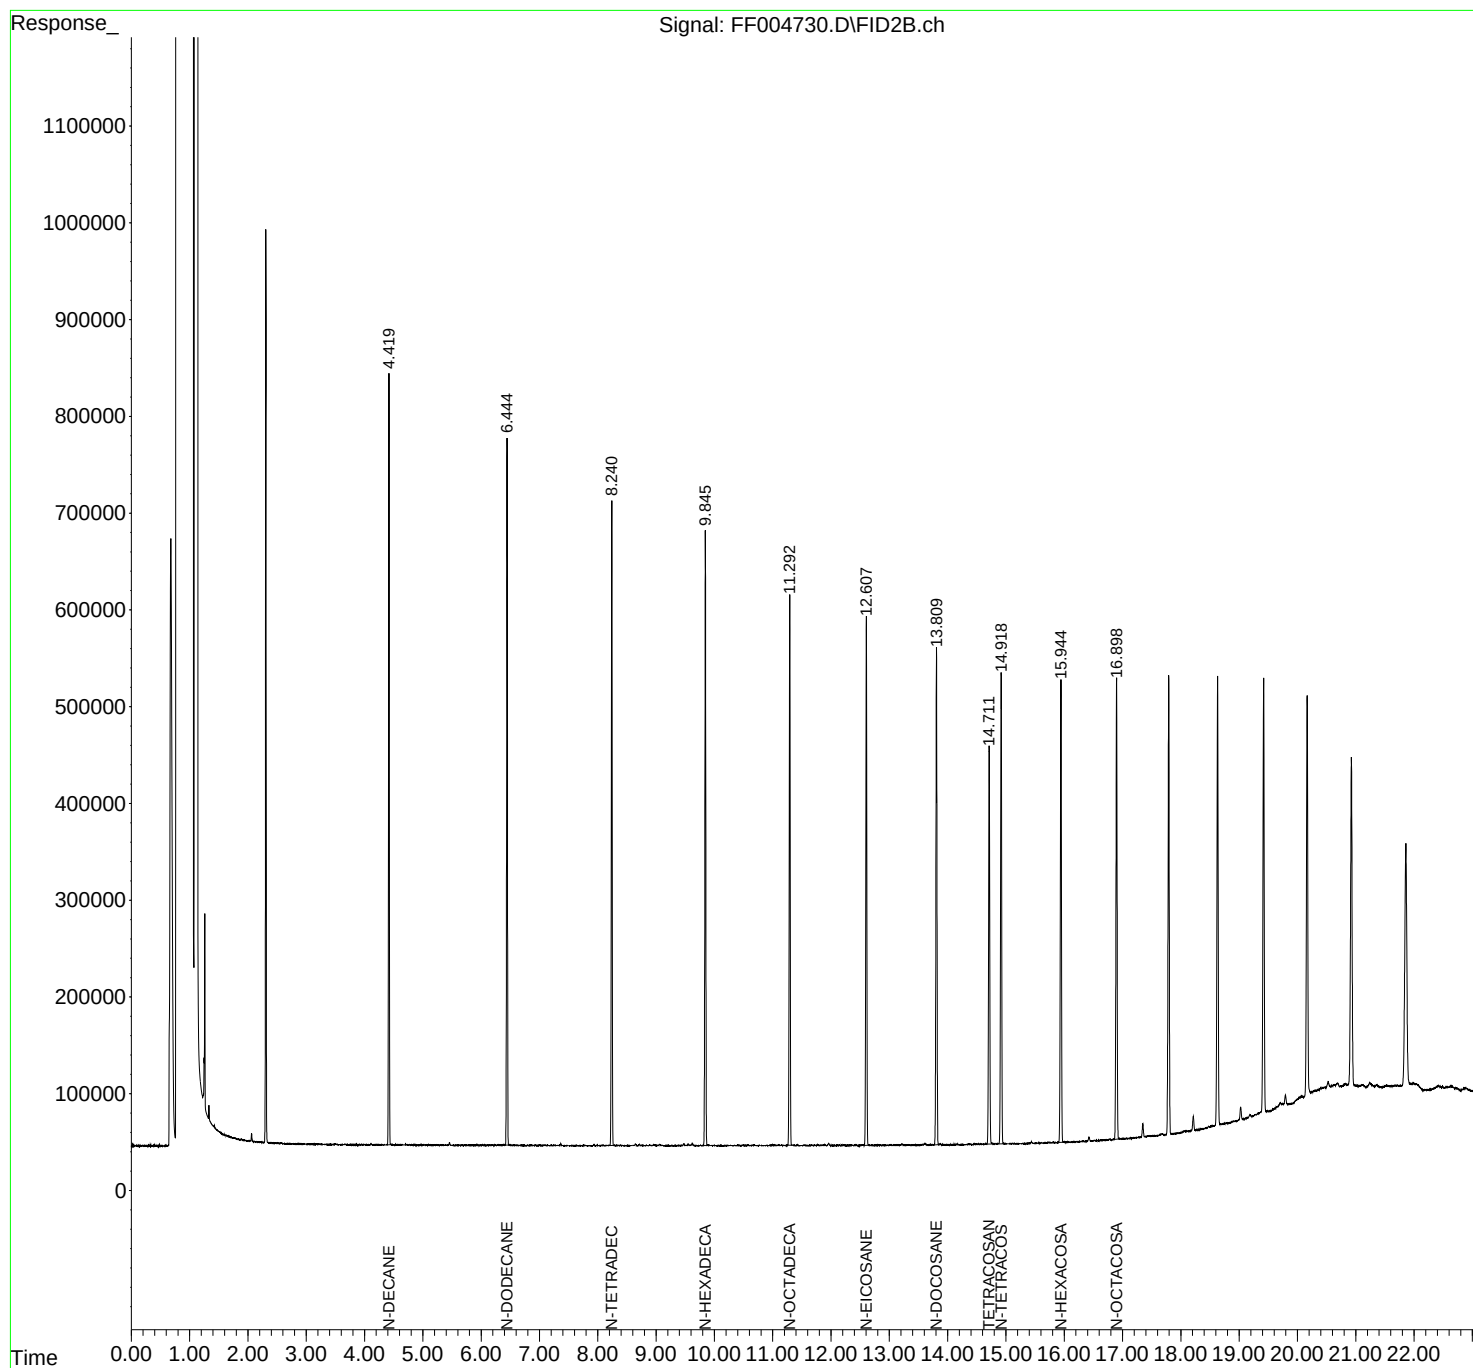

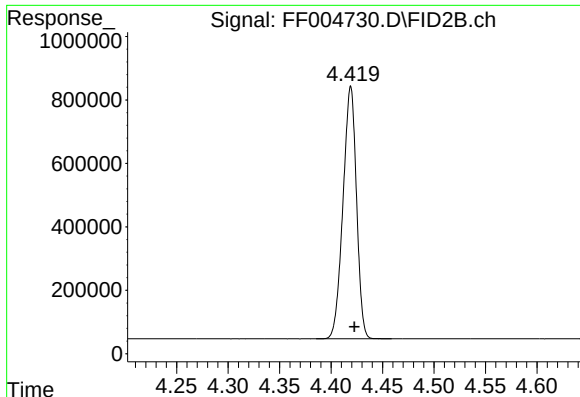


#2 N-DECANE

R.T.: 4.419 min
Delta R.T.: -0.004 min
Response: 7256170
Conc: 49.55 ug/ml

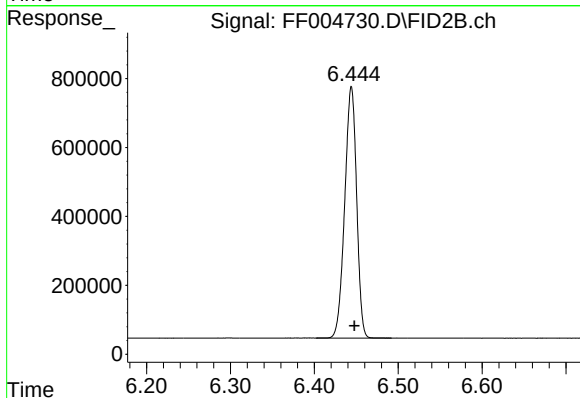


#3 N-DODECANE

R.T.: 6.444 min
Delta R.T.: -0.004 min
Response: 7188270
Conc: 48.58 ug/ml

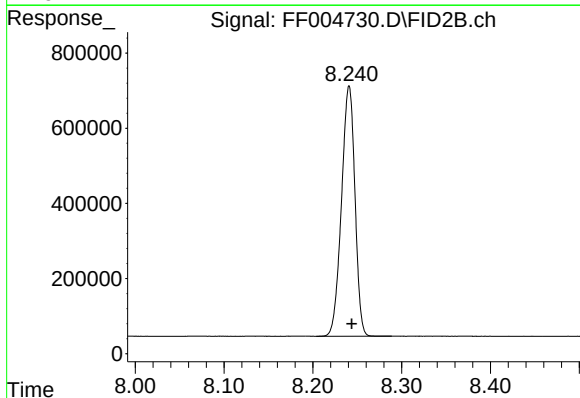


#4 N-TETRADECANE

R.T.: 8.241 min
Delta R.T.: -0.003 min
Response: 7007693
Conc: 47.71 ug/ml

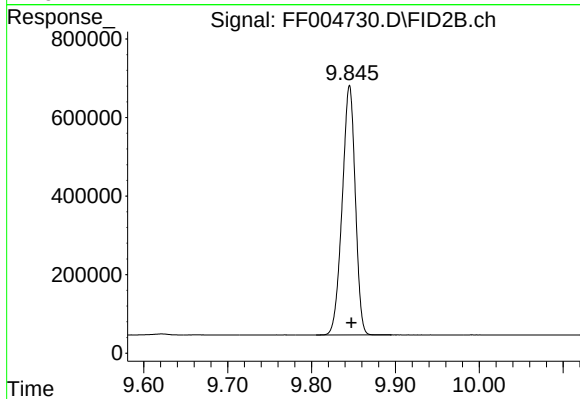


#5 N-HEXADECANE

R.T.: 9.845 min
Delta R.T.: -0.002 min
Response: 6892465
Conc: 46.68 ug/ml

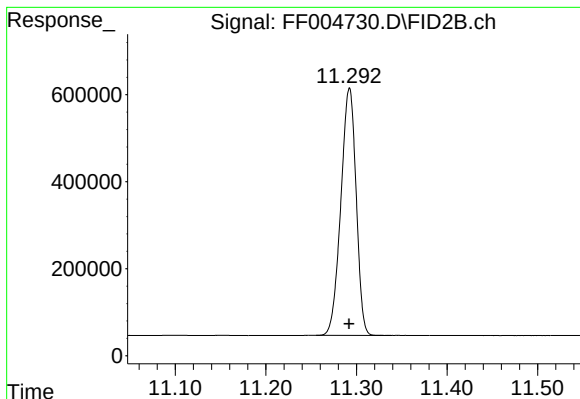


#6 N-OCTADECANE

R.T.: 11.292 min
Delta R.T.: 0.000 min
Response: 6663992
Conc: 45.90 ug/ml

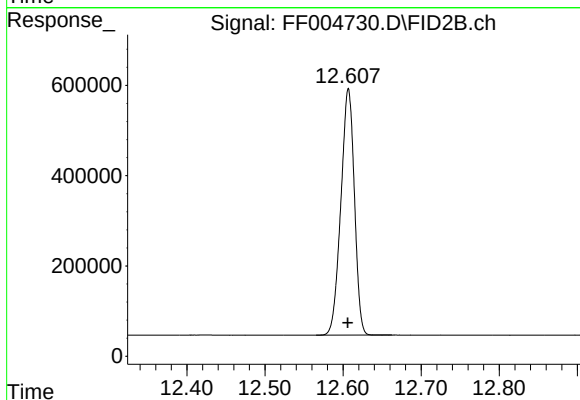


#7 N-EICOSANE

R.T.: 12.607 min
Delta R.T.: 0.000 min
Response: 6580566
Conc: 45.44 ug/ml

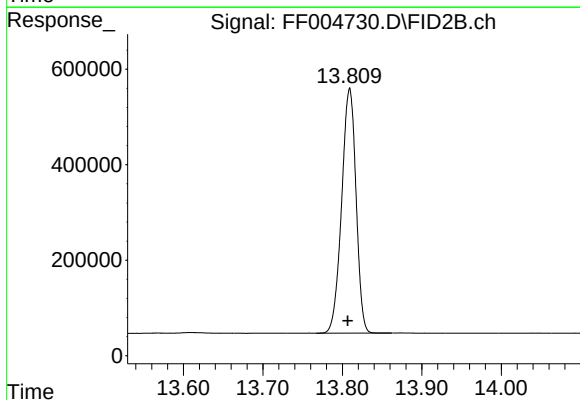


#8 N-DOCOSANE

R.T.: 13.809 min
Delta R.T.: 0.003 min
Response: 6441649
Conc: 45.59 ug/ml

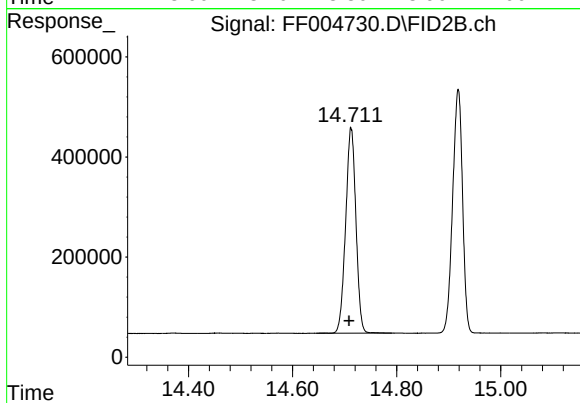


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.713 min
Delta R.T.: 0.004 min
Response: 5624312
Conc: 46.06 ug/ml

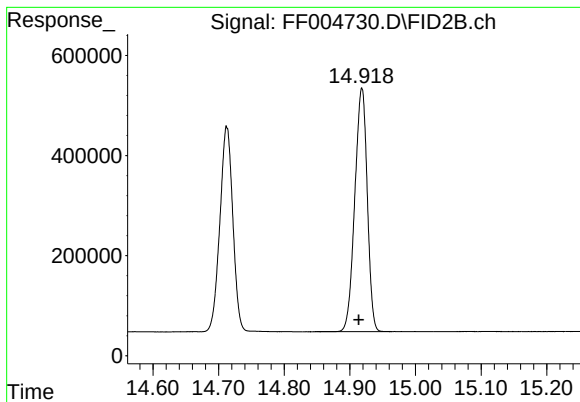


#10 N-TETRACOSANE

R.T.: 14.918 min
Delta R.T.: 0.005 min
Response: 6408520
Conc: 46.24 ug/ml

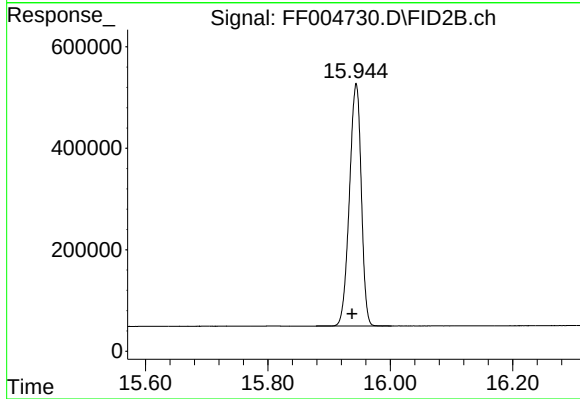

#11 N-HEXACOSANE

R.T.: 15.944 min
Delta R.T.: 0.007 min
Response: 6408484
Conc: 47.03 ug/ml

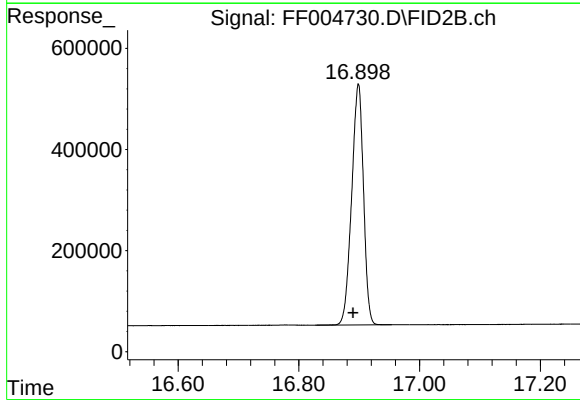

#12 N-OCTACOSANE

R.T.: 16.899 min
Delta R.T.: 0.009 min
Response: 6463611
Conc: 47.54 ug/ml