

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
 Data File : FF008531.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2021 20:46
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 05:22:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.544	5101567	40.890 ug/ml
11)	N-HEXACOSANE	15.993	92883	0.775 ug/ml
12)	N-OCTACOSANE	16.946	5270432	44.429 ug/ml
13)	N-TRIACONTANE	17.827	605433	5.112 ug/ml
14)	N-DOTRIACONTANE	18.657	835193	6.940 ug/ml
15)	N-TETRATRIACONTANE	19.434	564782	5.144 ug/ml
16)	N-HEXATRIACONTANE	20.171	306116	2.761 ug/ml
17)	N-OCTATRIACONTANE	20.919	257906	2.542 ug/ml
18)	N-TETRACONTANE	21.858	69665	0.659 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008531.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 20:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 05:22:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

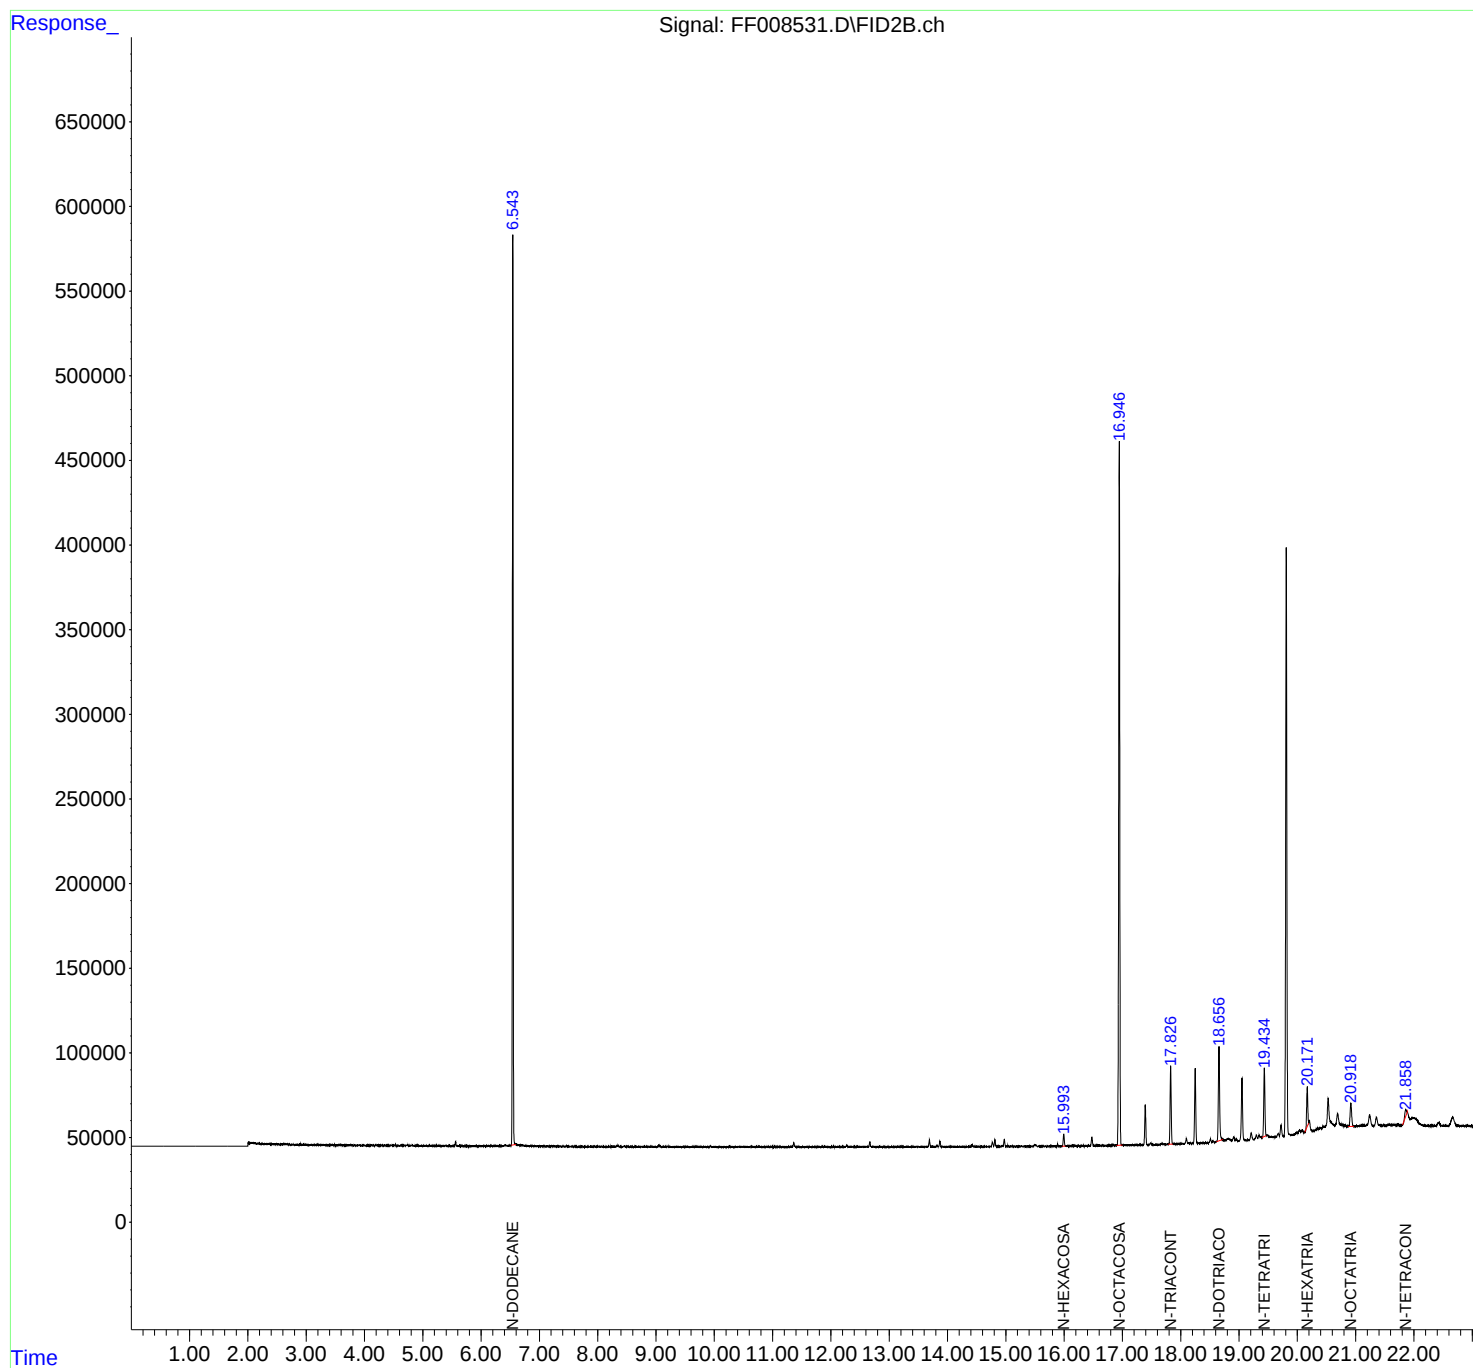


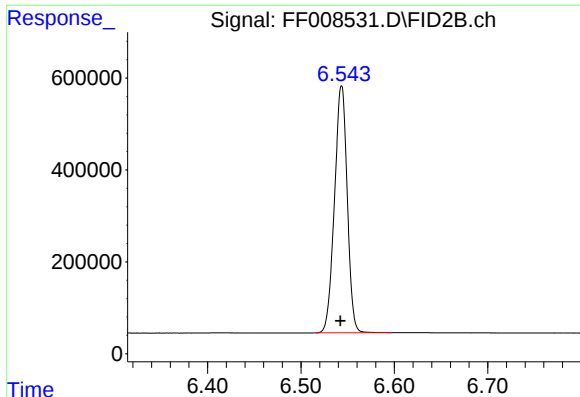

#3 N-DODECANE


R.T.: 6.544 min
Delta R.T.: 0.002 min
Response: 5101567
Conc: 40.89 ug/ml

Instrument :
FID_F
ClientSampleId :

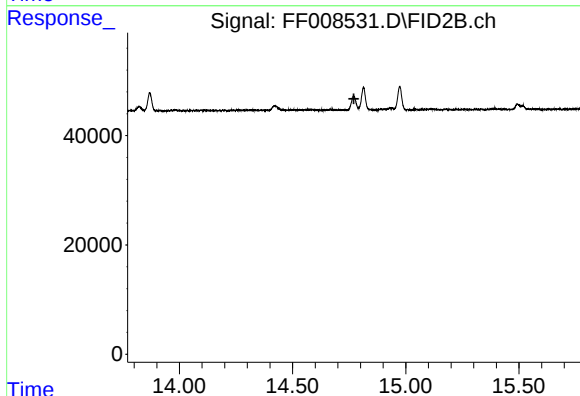


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.771 min
Response: 0
Conc: N.D.

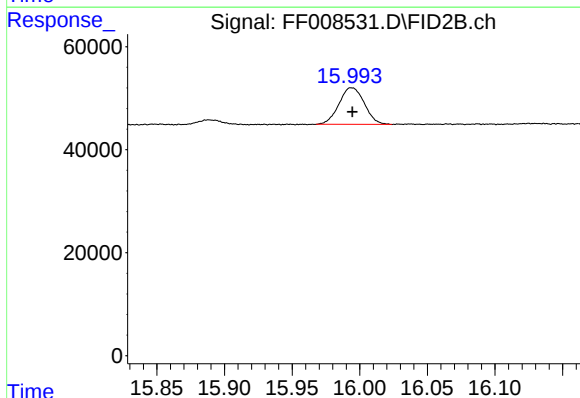


#11 N-HEXACOSANE

R.T.: 15.993 min
Delta R.T.: -0.001 min
Response: 92883
Conc: 0.77 ug/ml

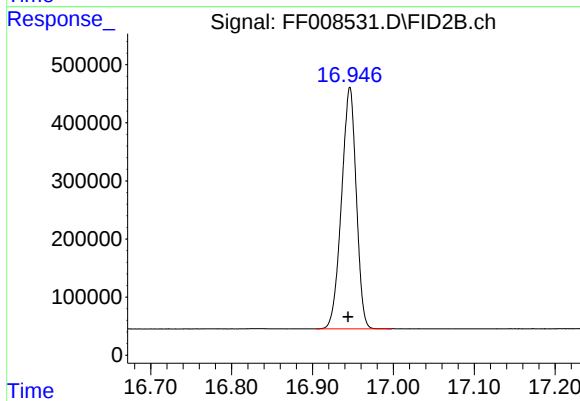

#12 N-OCTACOSANE


R.T.: 16.946 min
Delta R.T.: 0.003 min
Response: 5270432
Conc: 44.43 ug/ml

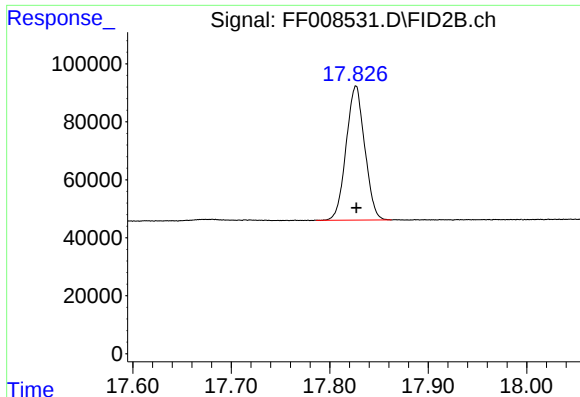

#13 N-TRIACONTANE


R.T.: 17.827 min
Delta R.T.: 0.000 min
Response: 605433
Conc: 5.11 ug/ml

Instrument :
FID_F
ClientSampleId :

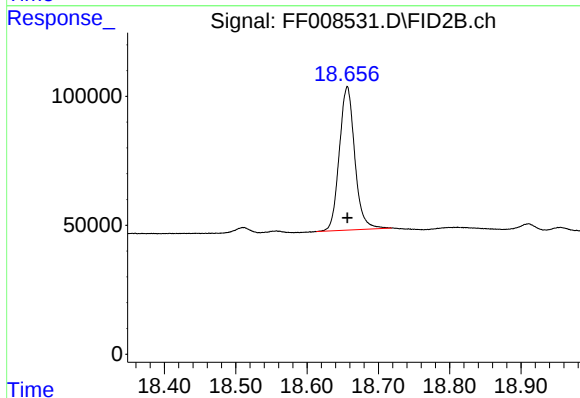


#14 N-DOTRIACONTANE

R.T.: 18.657 min
Delta R.T.: 0.000 min
Response: 835193
Conc: 6.94 ug/ml

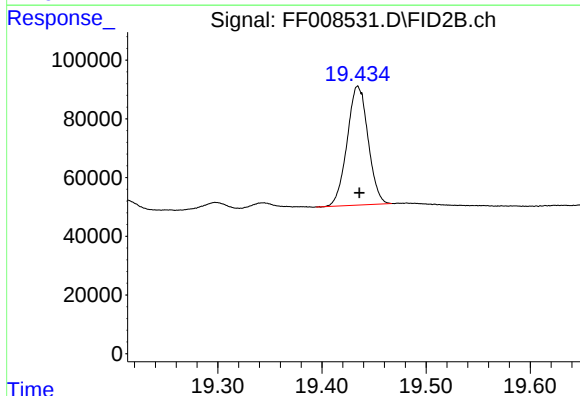


#15 N-TETRATRIACONTANE

R.T.: 19.434 min
Delta R.T.: -0.002 min
Response: 564782
Conc: 5.14 ug/ml

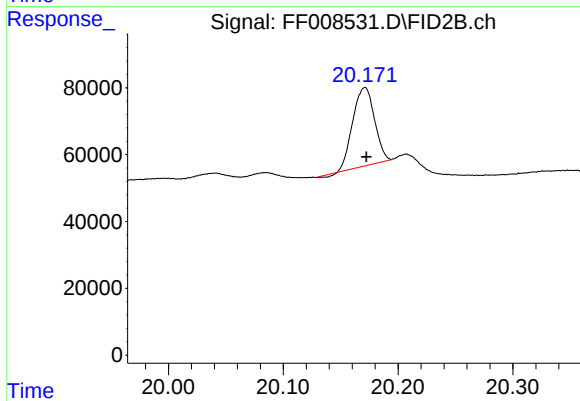

#16 N-HEXATRIACONTANE


R.T.: 20.171 min
Delta R.T.: -0.001 min
Response: 306116
Conc: 2.76 ug/ml

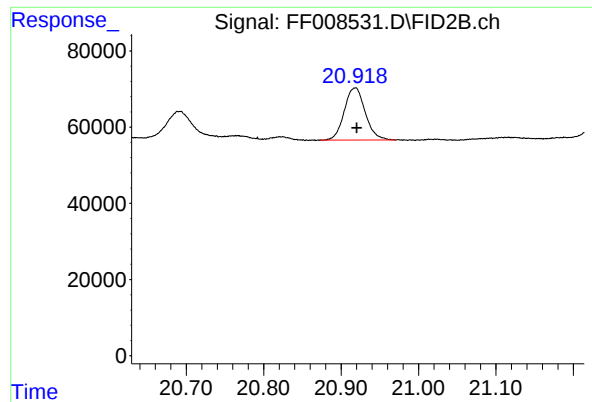

#17 N-OCTATRIACONTANE

R.T.: 20.919 min
Delta R.T.: 0.000 min
Response: 257906
Conc: 2.54 ug/ml

Instrument :
FID_F
ClientSampleId :

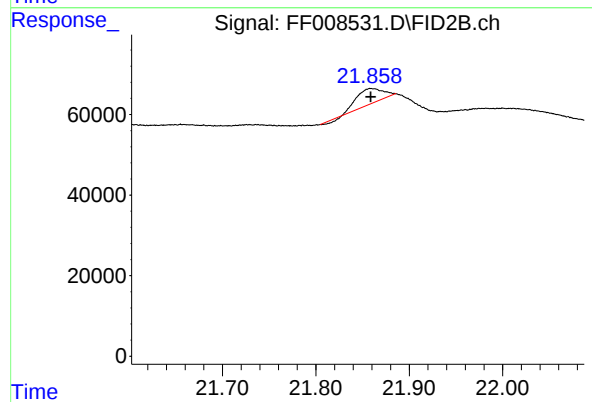

#18 N-TETRACONTANE

R.T.: 21.858 min
Delta R.T.: 0.000 min
Response: 69665
Conc: 0.66 ug/ml