

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008534.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 22:20
Operator : DD\AJ
Sample : M2589-17 20X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 05:23:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.966	336982	2.750 ug/ml
14)	N-DOTRIACONTANE	18.664	225690	1.875 ug/ml
16)	N-HEXATRIACONTANE	20.209	514343	4.639 ug/ml
18)	N-TETRACONTANE	21.891	657603	6.225 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008534.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 22:20
Operator : DD\AJ
Sample : M2589-17 20X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Jun 07 05:23:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

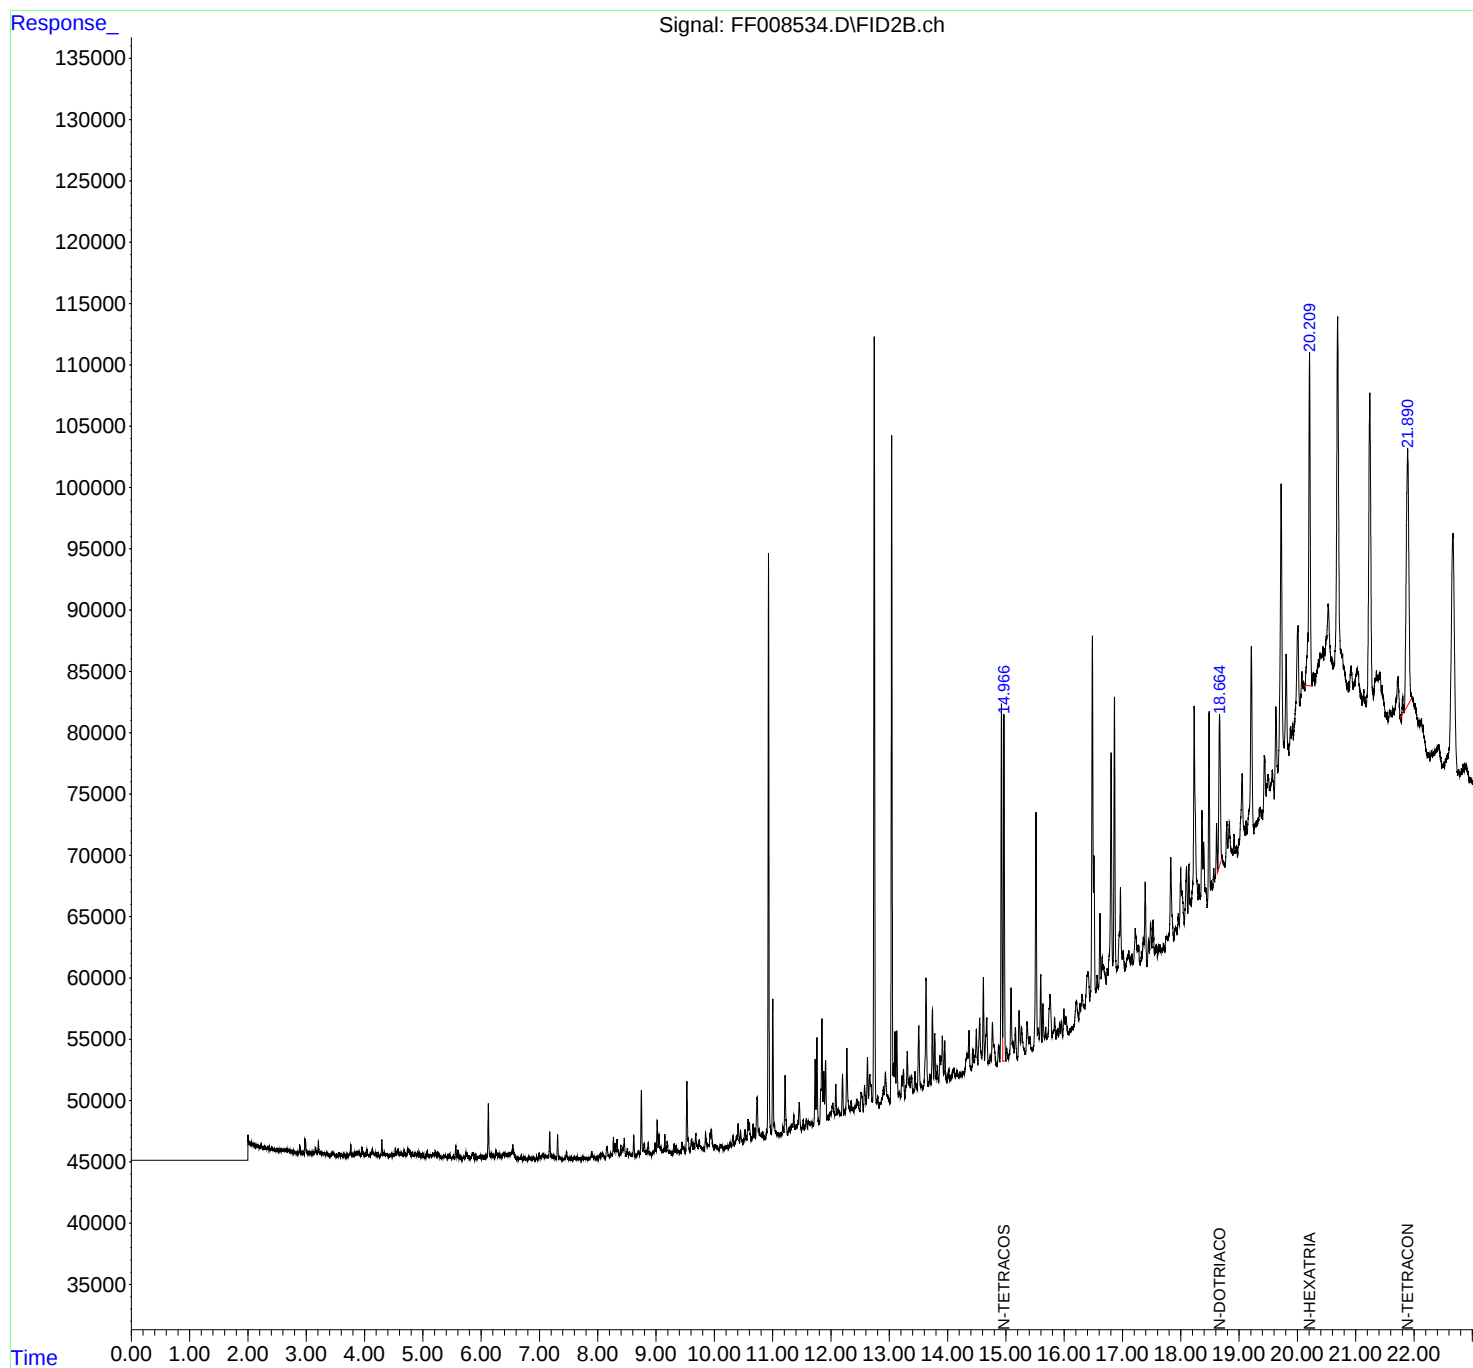


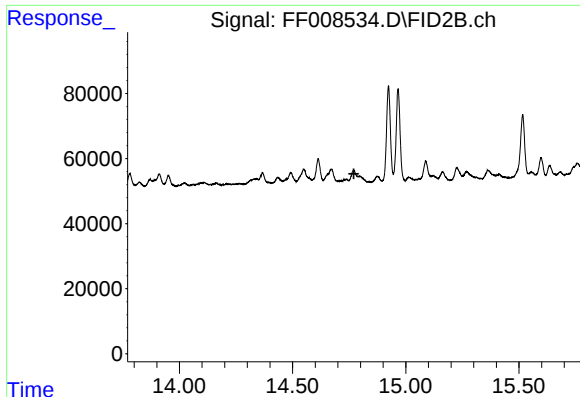

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.771 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

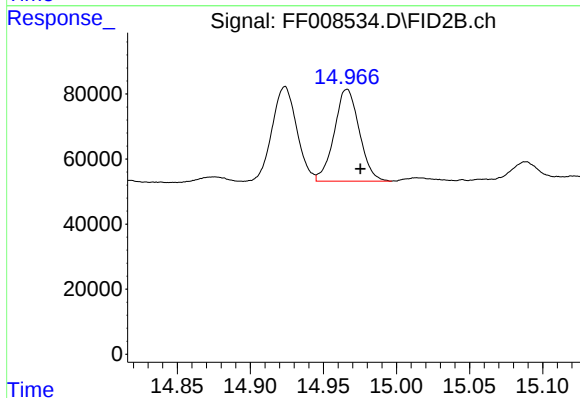


#10 N-TETRACOSANE

R.T.: 14.966 min
Delta R.T.: -0.009 min
Response: 336982
Conc: 2.75 ug/ml

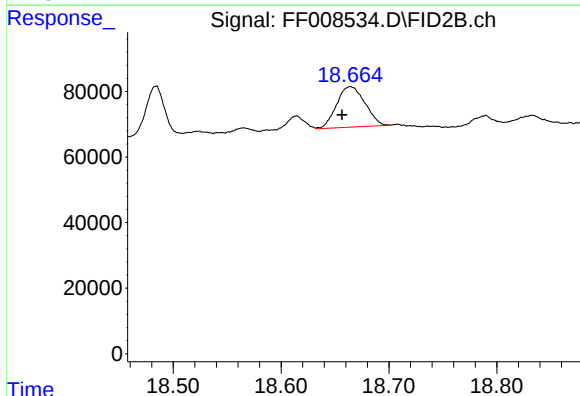


#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: 0.008 min
Response: 225690
Conc: 1.88 ug/ml

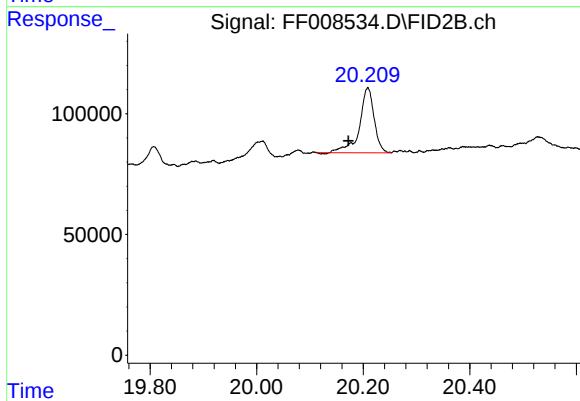

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.036 min
Response: 514343
Conc: 4.64 ug/ml

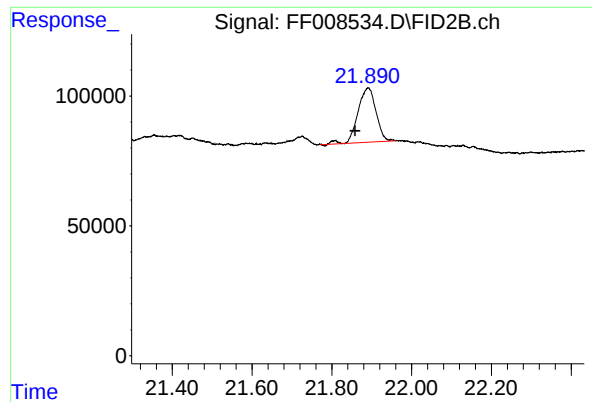

#18 N-TETRACONTANE

R.T.: 21.891 min
Delta R.T.: 0.033 min
Response: 657603
Conc: 6.22 ug/ml

Instrument :
FID_F
ClientSampleId :