

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008535.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 22:52
Operator : DD\AJ
Sample : M2589-18 20X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 05:23:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

13)	N-TRIACONTANE	17.828	140131	1.183 ug/ml
14)	N-DOTRIACONTANE	18.666	412161	3.425 ug/ml
15)	N-TETRATRIACONTANE	19.438	78168	0.712 ug/ml
16)	N-HEXATRIACONTANE	20.209	417752	3.768 ug/ml
18)	N-TETRACONTANE	21.893	420160	3.977 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008535.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 22:52
Operator : DD\AJ
Sample : M2589-18 20X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 05:23:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

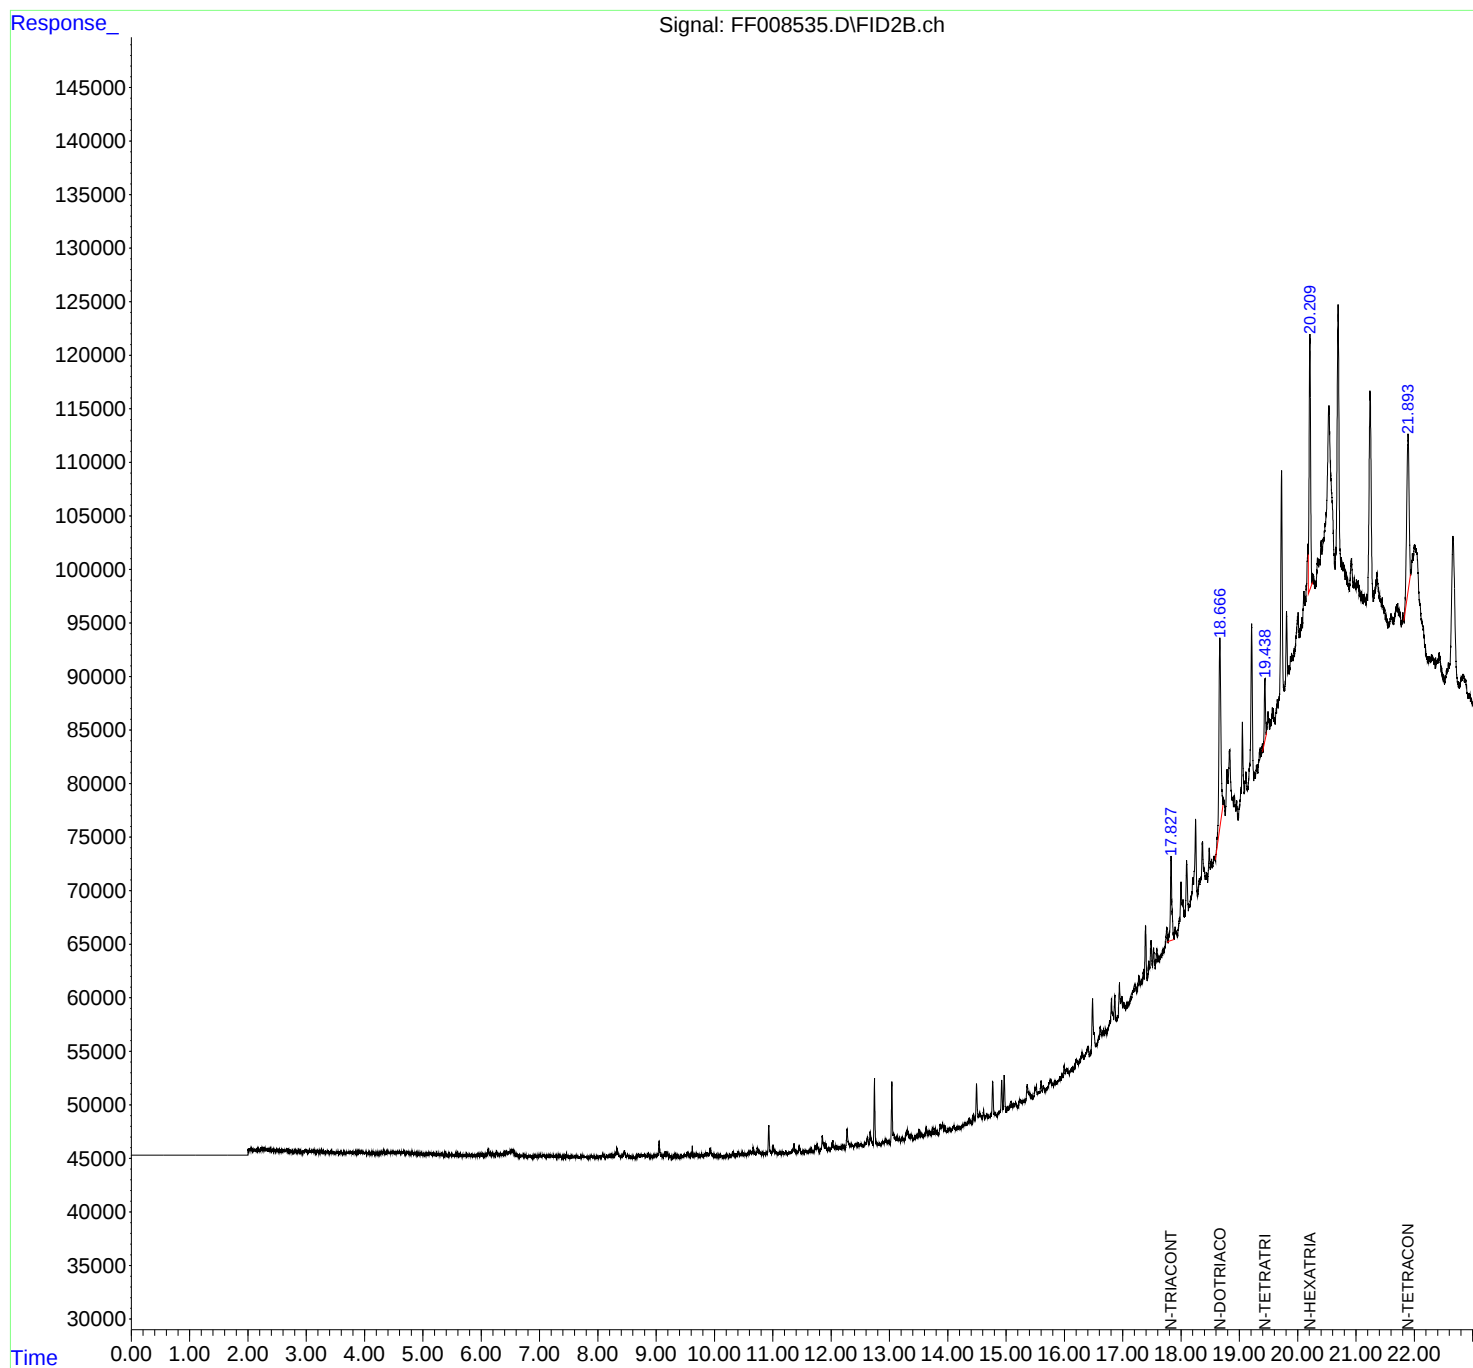


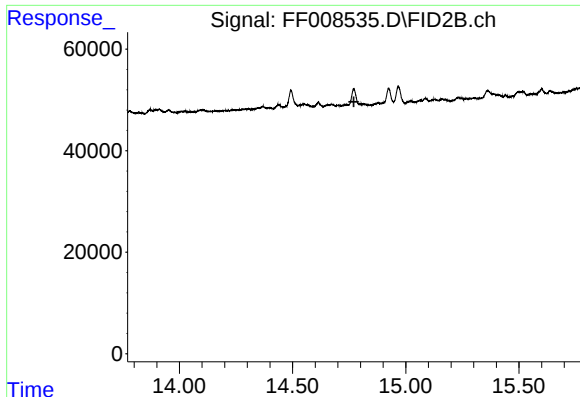

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.771 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

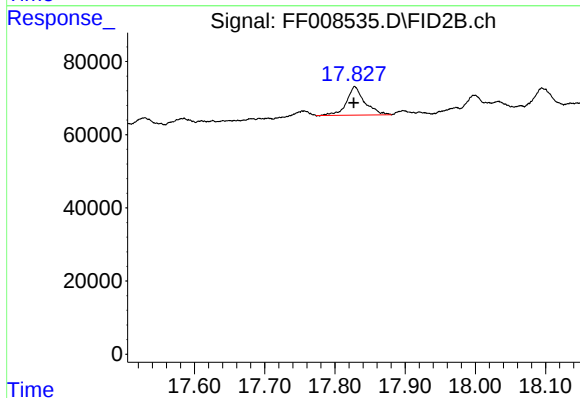


#13 N-TRIACONTANE

R.T.: 17.828 min
Delta R.T.: 0.000 min
Response: 140131
Conc: 1.18 ug/ml

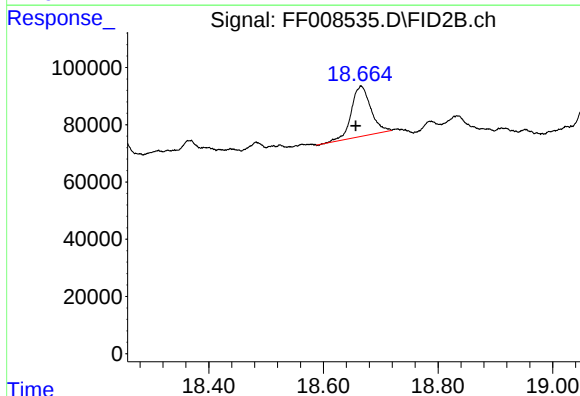


#14 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.009 min
Response: 412161
Conc: 3.42 ug/ml

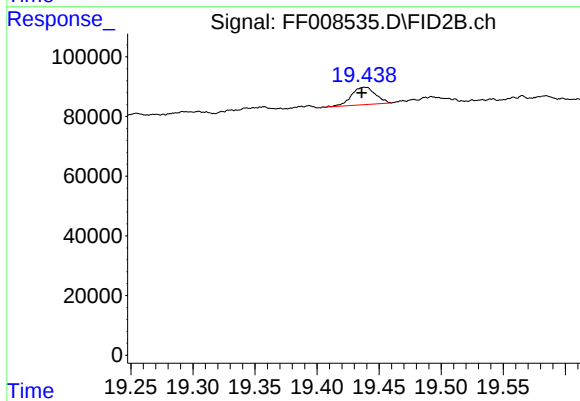

#15 N-TETRATRIACONTANE


R.T.: 19.438 min
Delta R.T.: 0.002 min
Response: 78168
Conc: 0.71 ug/ml

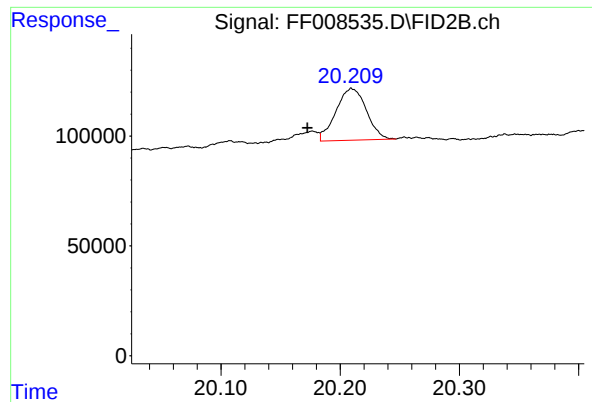

#16 N-HEXATRIACONTANE

R.T.: 20.209 min
Delta R.T.: 0.037 min
Response: 417752
Conc: 3.77 ug/ml

Instrument :
FID_F
ClientSampleId :

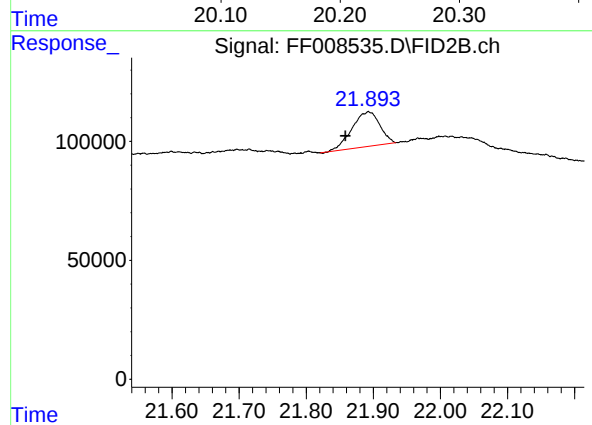

#18 N-TETRACONTANE

R.T.: 21.893 min
Delta R.T.: 0.034 min
Response: 420160
Conc: 3.98 ug/ml