

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
 Data File : FF008536.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jun 2021 23:24
 Operator : DD\AJ
 Sample : M2589-10 100X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 07 05:23:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
 Quant Title :
 QLast Update : Mon Jun 07 02:02:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
2) N-DECANE	4.528	554207	4.568 ug/ml
3) N-DODECANE	6.543	105872	0.849 ug/ml
7) N-EICOSANE	12.615f	1374478	10.764 ug/ml
14) N-DOTRIACONTANE	18.663	101266	0.841 ug/ml
15) N-TETRATRIACONTANE	19.439	116220	1.058 ug/ml
16) N-HEXATRIACONTANE	20.207	310199	2.798 ug/ml
18) N-TETRACONTANE	21.890	132170	1.251 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008536.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 23:24
Operator : DD\AJ
Sample : M2589-10 100X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 05:23:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

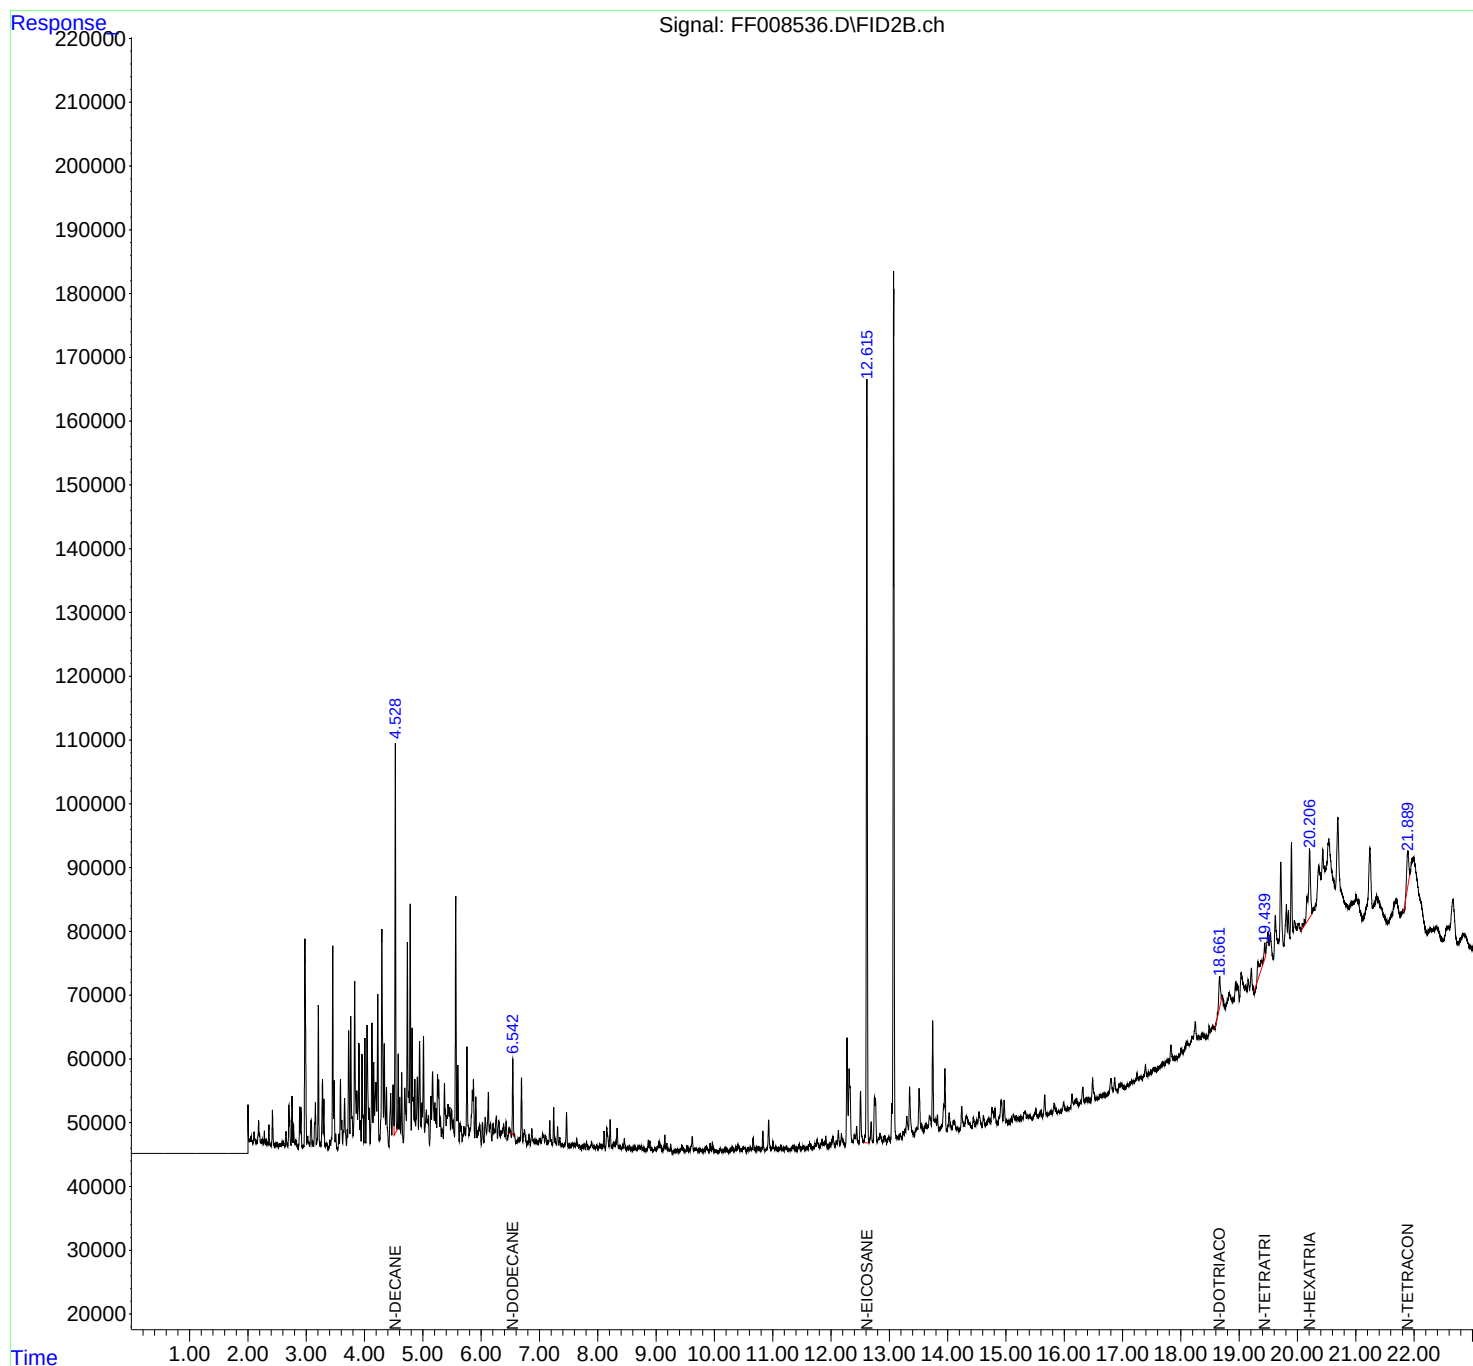


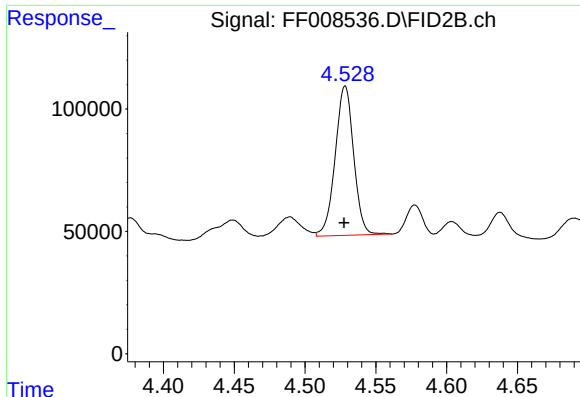

#2 N-DECANE


R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 554207
Conc: 4.57 ug/ml

Instrument :
FID_F
ClientSampleId :

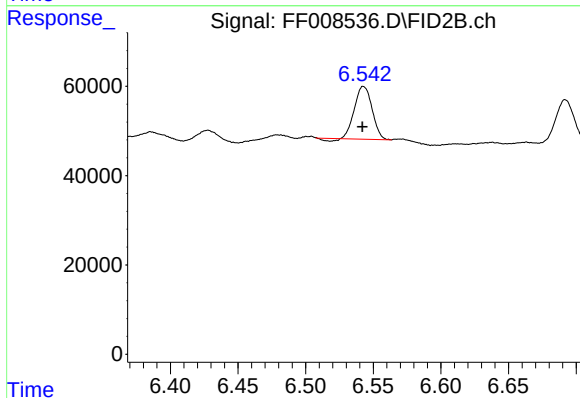


#3 N-DODECANE

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 105872
Conc: 0.85 ug/ml

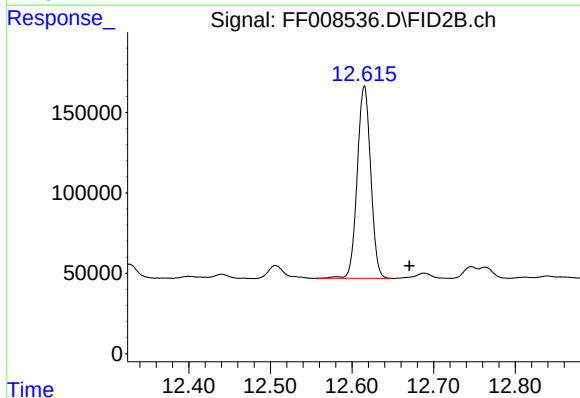


#7 N-EICOSANE

R.T.: 12.615 min
Delta R.T.: -0.055 min
Response: 1374478
Conc: 10.76 ug/ml

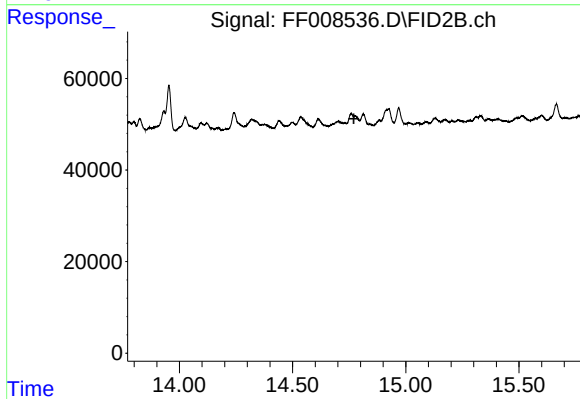

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.771 min
Response: 0
Conc: N.D.

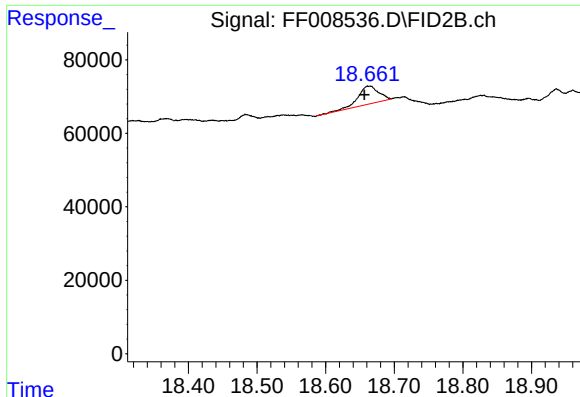

#14 N-DOTRIACONTANE


R.T.: 18.663 min
Delta R.T.: 0.006 min
Response: 101266
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

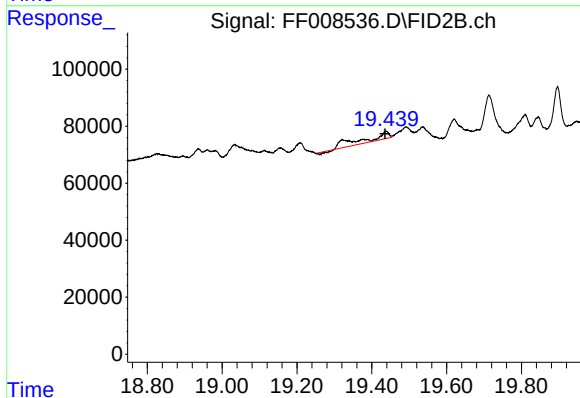


#15 N-TETRATRIACONTANE

R.T.: 19.439 min
Delta R.T.: 0.003 min
Response: 116220
Conc: 1.06 ug/ml

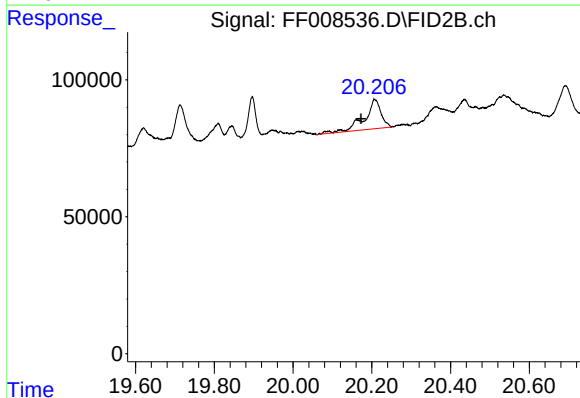

#16 N-HEXATRIACONTANE

R.T.: 20.207 min
Delta R.T.: 0.034 min
Response: 310199
Conc: 2.80 ug/ml

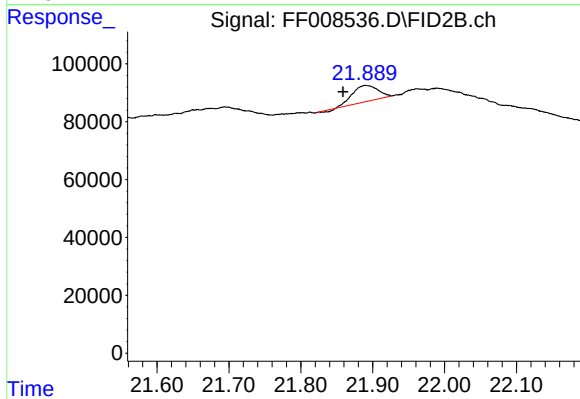

#18 N-TETRACONTANE

R.T.: 21.890 min
Delta R.T.: 0.031 min
Response: 132170
Conc: 1.25 ug/ml