

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008531.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 20:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 07 05:22:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.544	5101567	40.890 ug/ml
12) N-OCTACOSANE	16.946	5270432	44.429 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008531.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 20:46
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 07 05:22:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

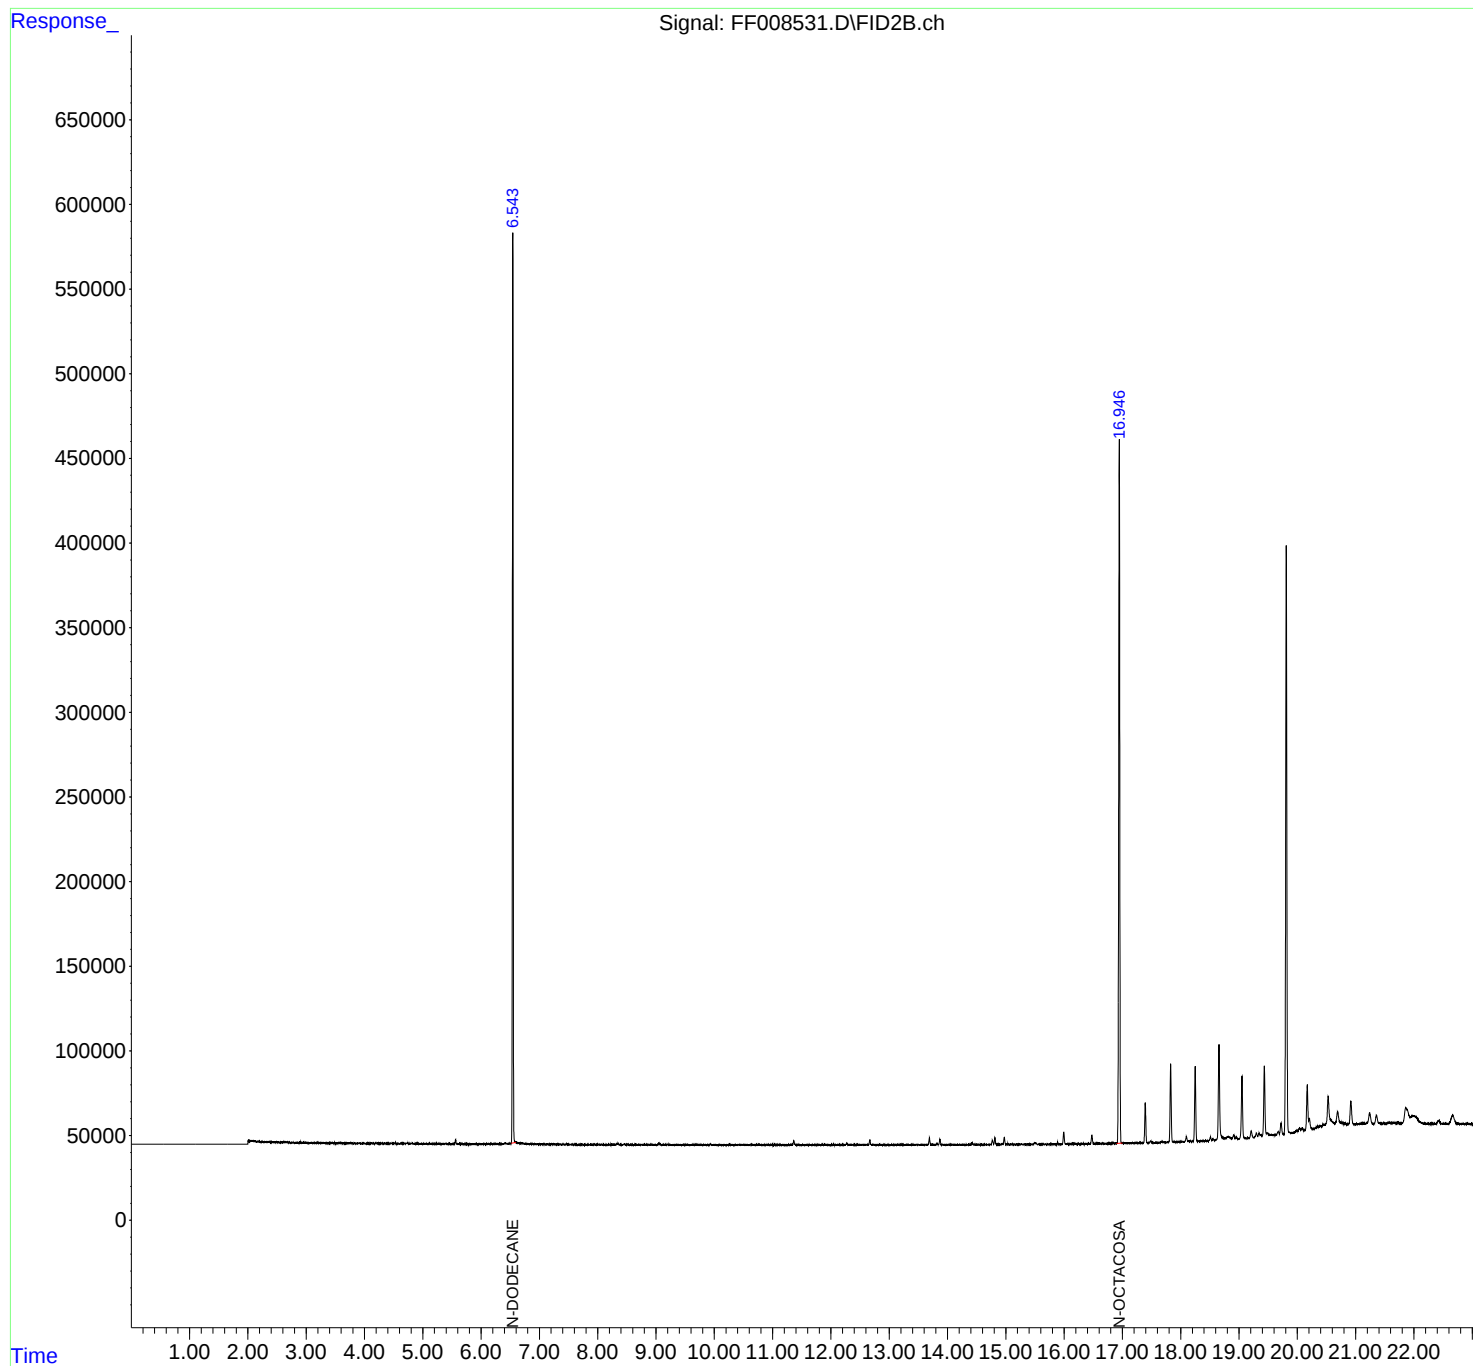


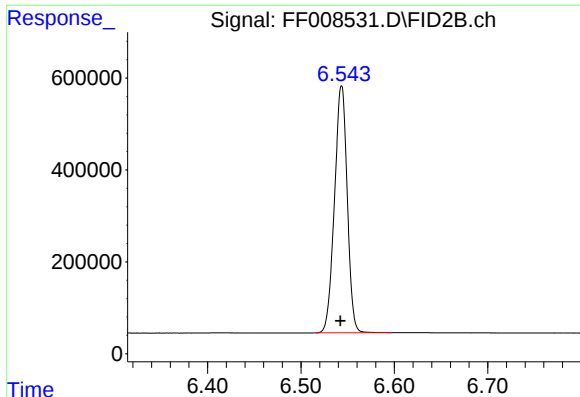

#3 N-DODECANE


R.T.: 6.544 min
Delta R.T.: 0.002 min
Response: 5101567
Conc: 40.89 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

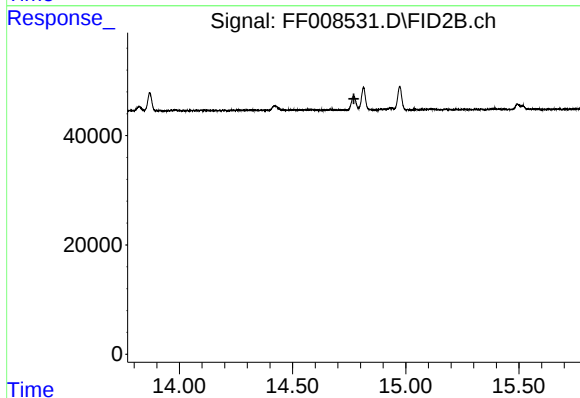

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.771 min
Response: 0
Conc: N.D.

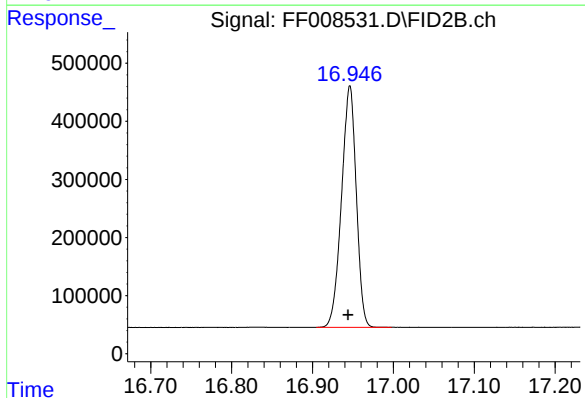

#12 N-OCTACOSANE

R.T.: 16.946 min
Delta R.T.: 0.003 min
Response: 5270432
Conc: 44.43 ug/ml