

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008533.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 21:49
Operator : DD\AJ
Sample : M2589-16 20X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
18-B11(4-6)

Manual Integrations
APPROVED

Ankita
6/7/2021 3:54:31 PM

Integration File: autoint1.e
Quant Time: Jun 07 05:22:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060621\
Data File : FF008533.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2021 21:49
Operator : DD\AJ
Sample : M2589-16 20X
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_F
ClientSampled :
18-B11(4-6)


Manual Integrations
APPROVED

Ankita
6/7/2021 3:54:31 PM

Integration File: autoint1.e
Quant Time: Jun 07 05:22:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060621.M
Quant Title :
QLast Update : Mon Jun 07 02:02:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

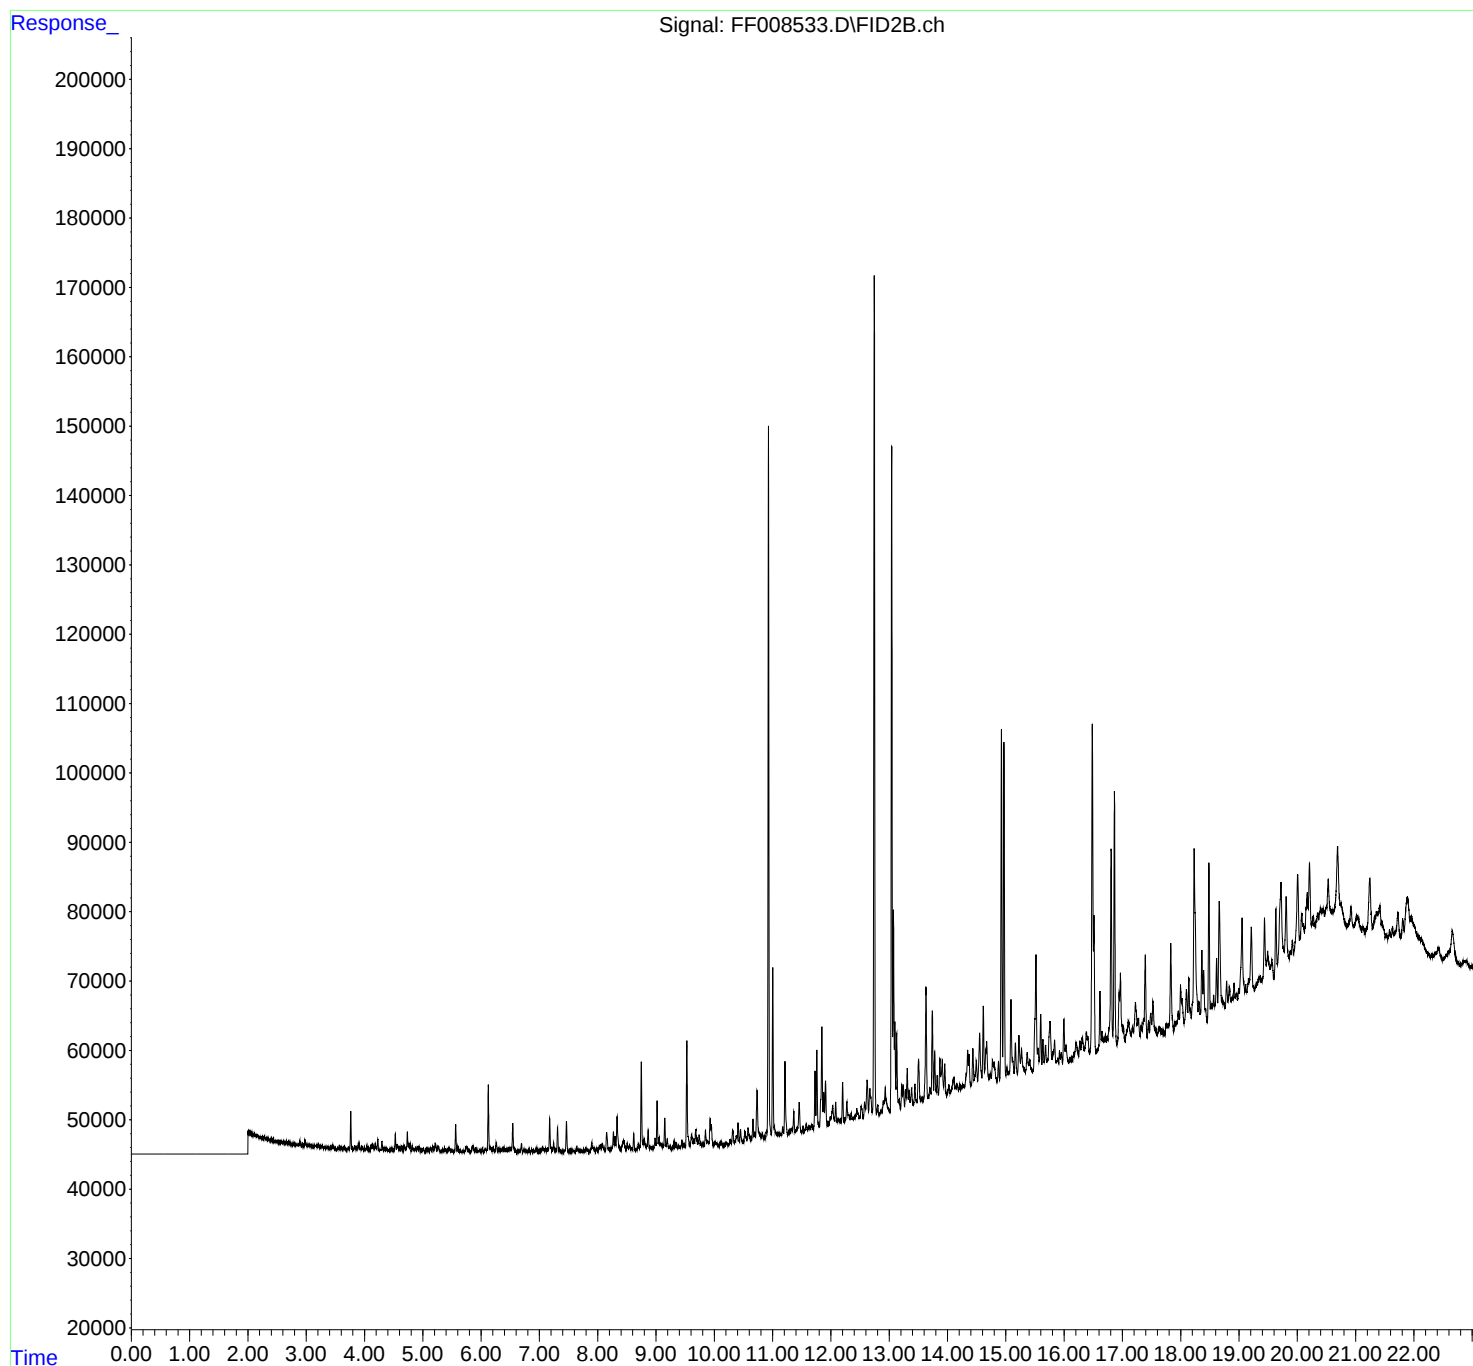

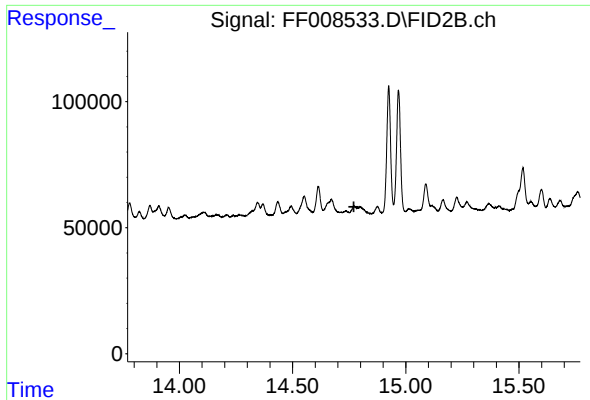

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.771 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
18-B11(4-6)

Manual Integrations
APPROVED

Ankita
6/7/2021 3:54:31 PM