

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060622\
Data File : FF010698.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2022 15:04
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 03:29:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 03:28:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) N-HEXATRIACONTANE	20.275	221079	2.571 ug/ml
18) N-TETRACONTANE	21.800	344012	3.590 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF060622\
Data File : FF010698.D
Signal(s) : FID2B.ch
Acq On : 06 Jun 2022 15:04
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 07 03:29:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF060622.M
Quant Title :
QLast Update : Tue Jun 07 03:28:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

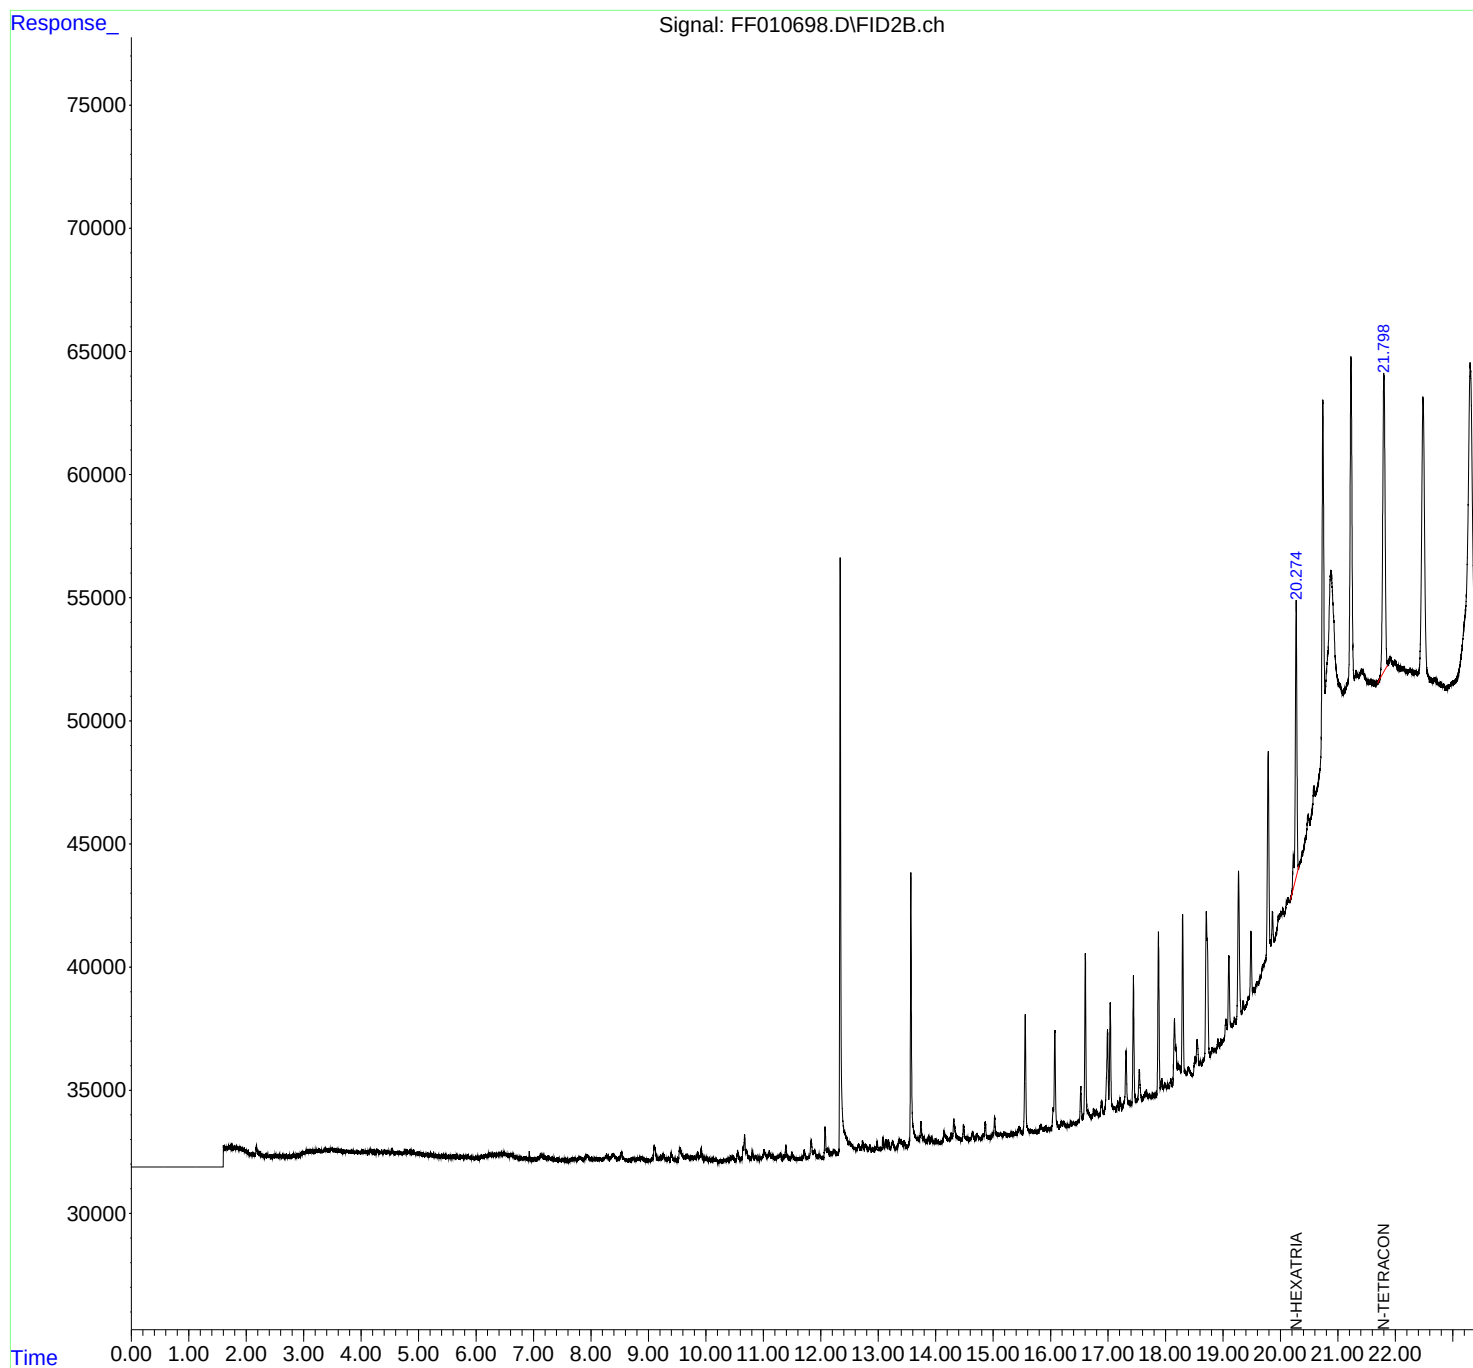


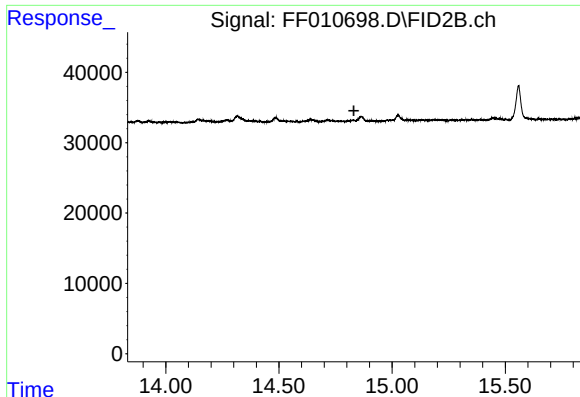

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.831 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

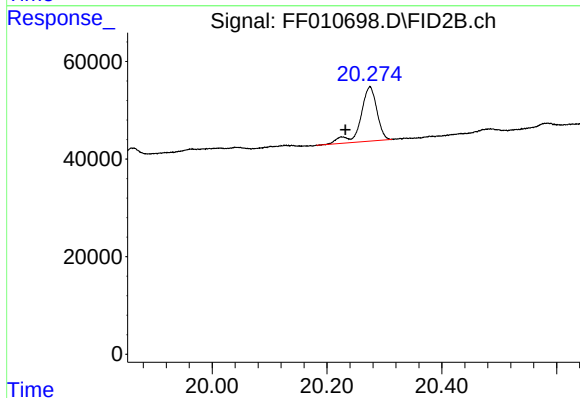

#16 N-HEXATRIACONTANE

R.T.: 20.275 min
Delta R.T.: 0.043 min
Response: 221079
Conc: 2.57 ug/ml

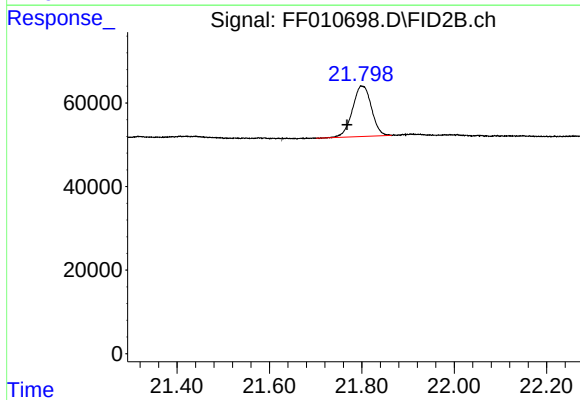

#18 N-TETRACONTANE

R.T.: 21.800 min
Delta R.T.: 0.032 min
Response: 344012
Conc: 3.59 ug/ml